


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102425\
Data File : BF144055.D
Acq On : 24 Oct 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 17:30:25 2025

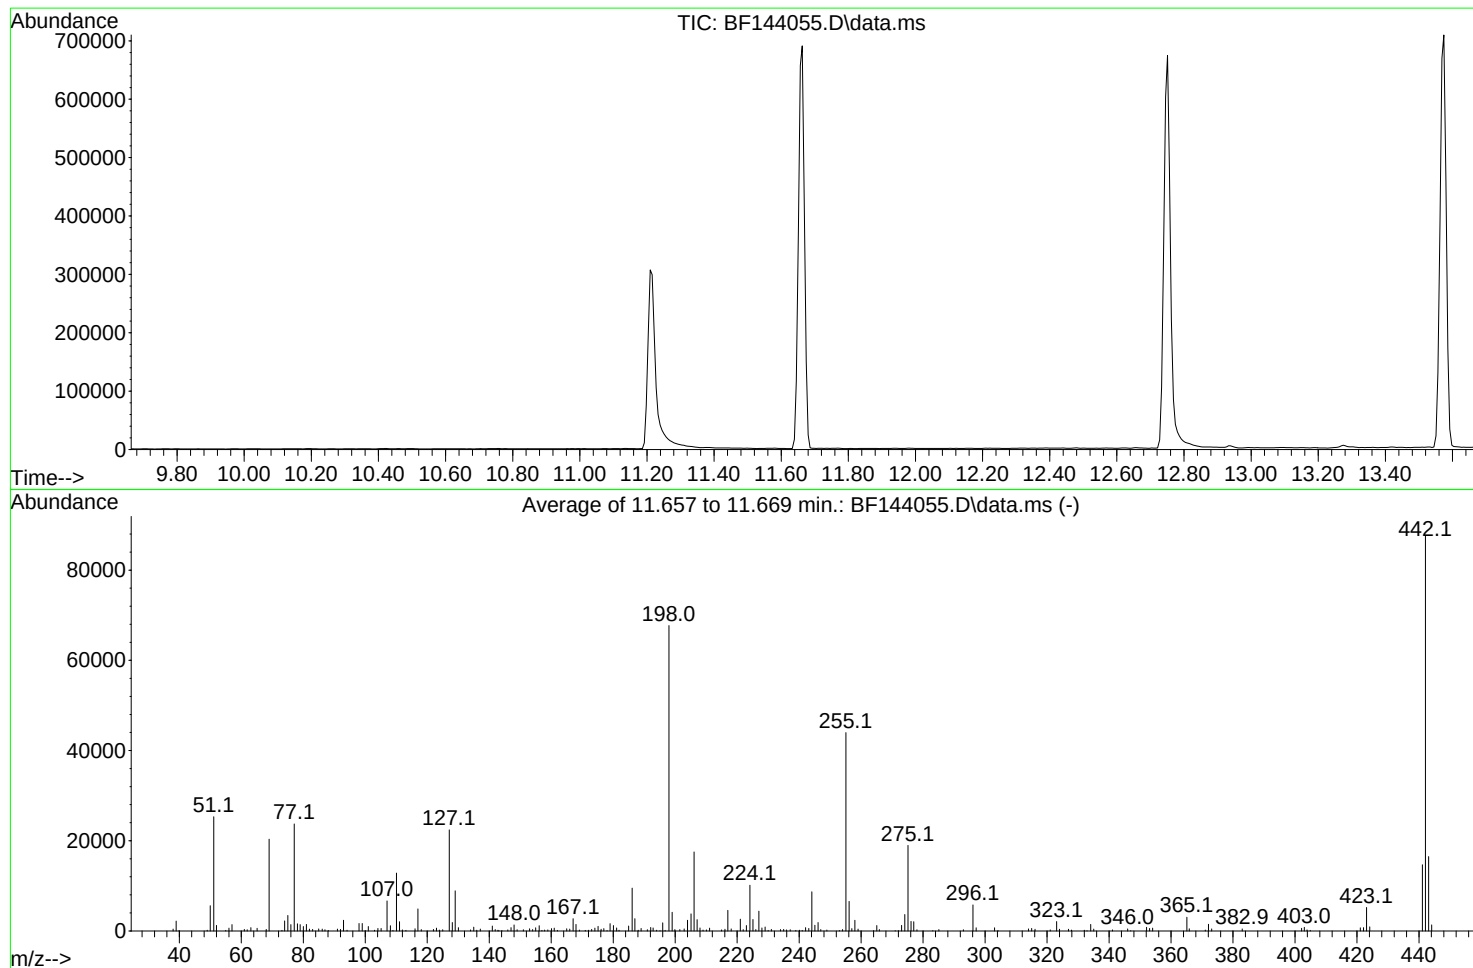




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	333	PASS
69	69	100	100	100.0	20363	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.2	133	PASS
198	198	100	100	100.0	67712	PASS
199	198	5	9	6.1	4142	PASS
365	198	1	100	4.5	3052	PASS
441	443	0.01	150	89.0	14677	PASS
442	442	100	100	100.0	87547	PASS
443	442	15	24	18.8	16486	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102425\
Data File : BF144055.D
Acq On : 24 Oct 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 24 10:43:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

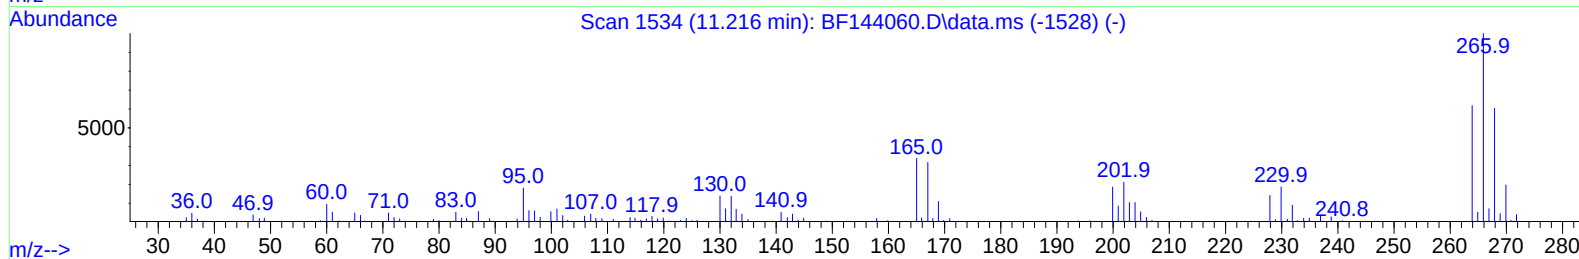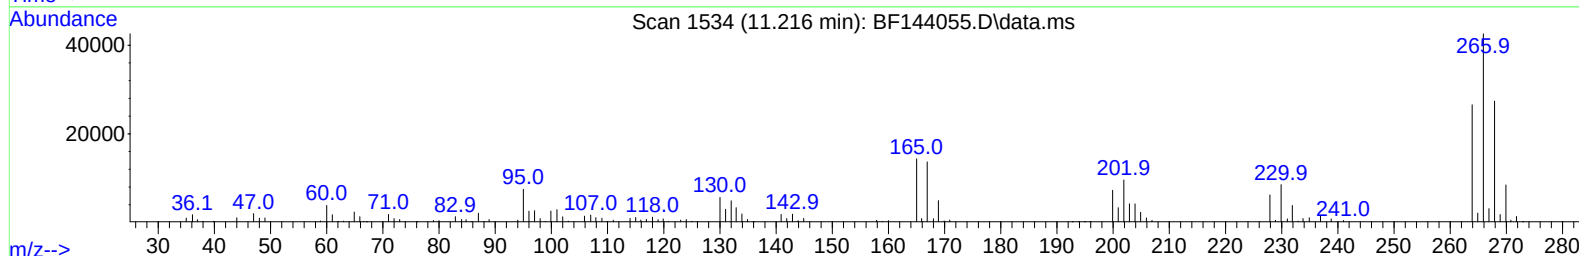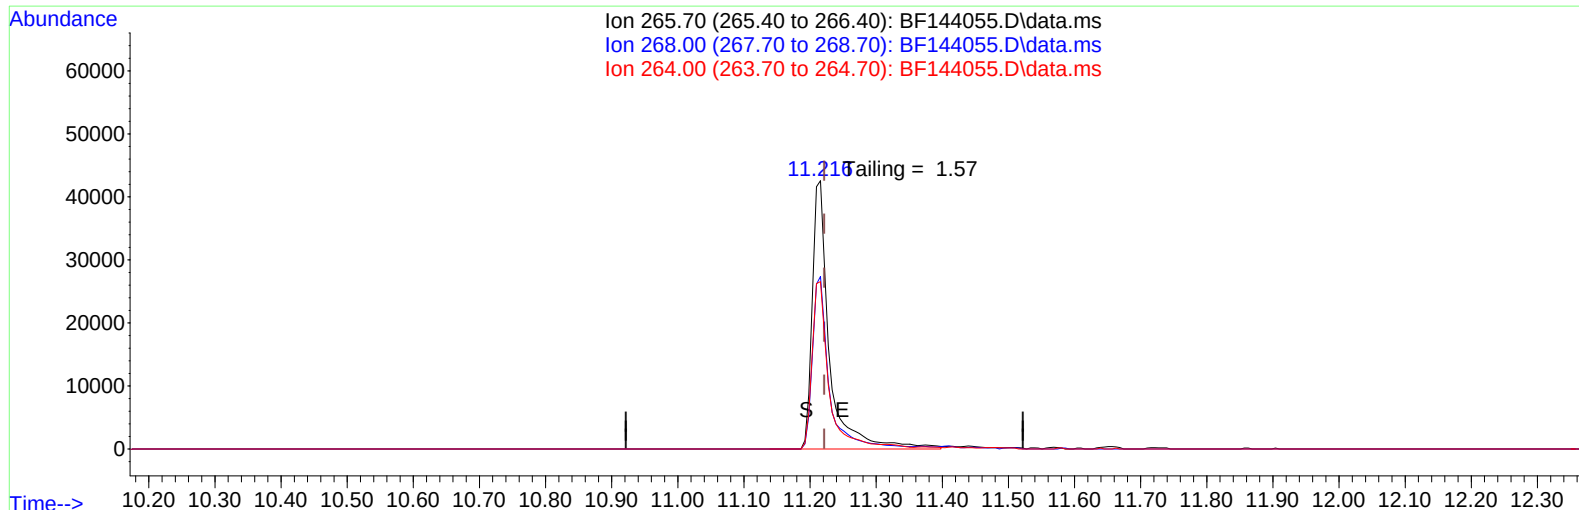

TIC: BF144055.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 43857.19 ng




response 76701

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.29
264.00	64.70	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102425\
Data File : BF144055.D
Acq On : 24 Oct 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 24 10:43:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

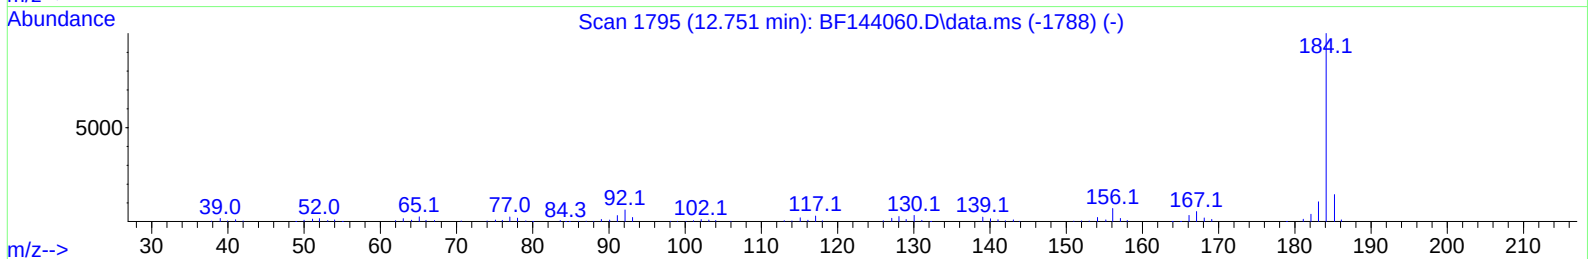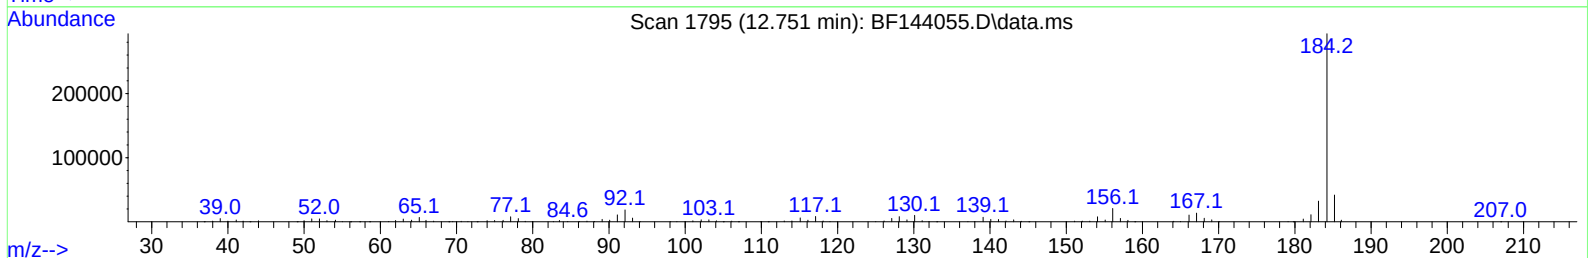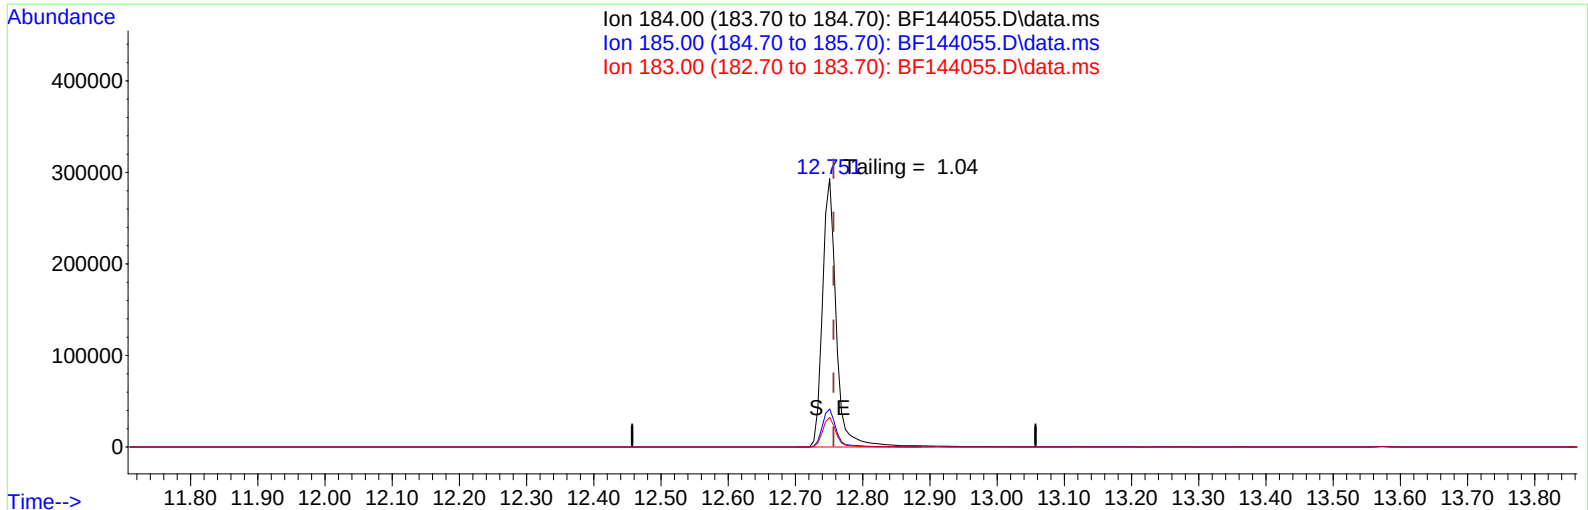

TIC: BF144055.D\data.ms

(77) Benzidine

12.751min (-0.006) 0.00 ng

response 416414

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.23
183.00	11.00	11.07
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
10/24/2025	BNA_F	<u>BF144055.D</u>
Compound Name	Response	Retention Time
DDT	192449	13.574
DDD	3266	13.274
DDE	1346	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4612	197061	2.34