
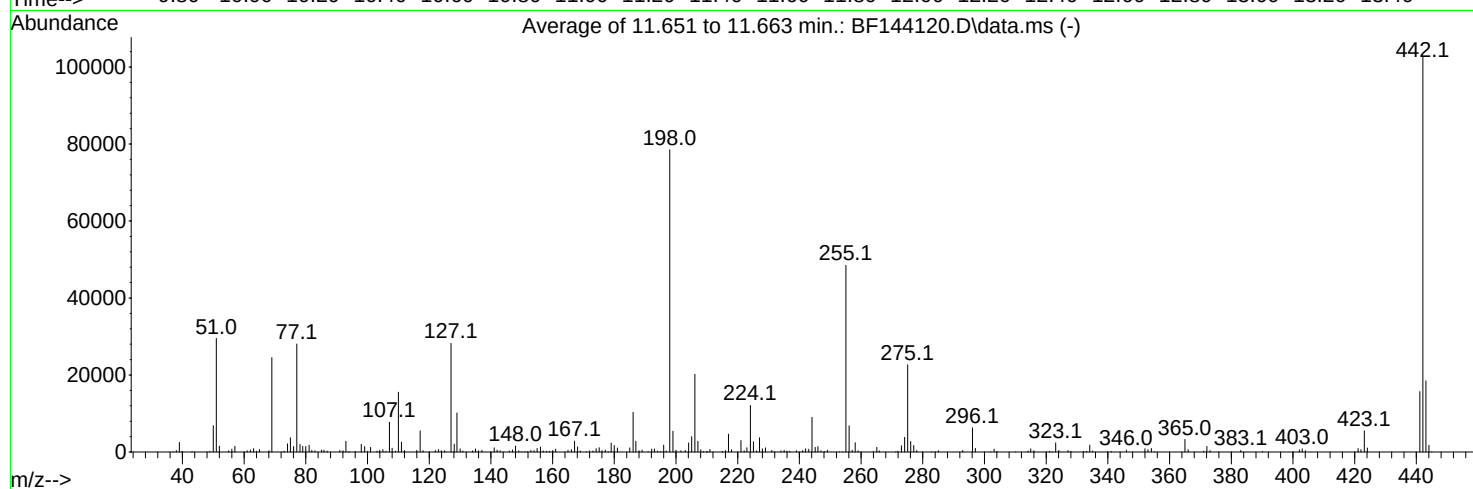


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102925\
Data File : BF144120.D
Acq On : 29 Oct 2025 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 17:30:25 2025

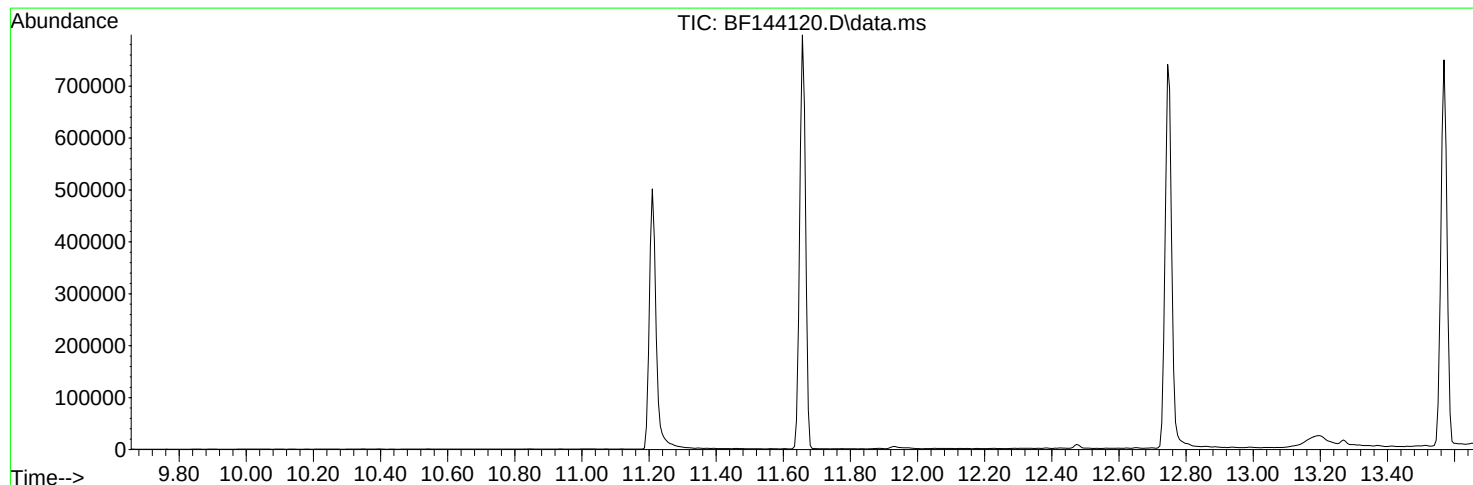




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.3	329	PASS
69	69	100	100	100.0	24539	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.4	309	PASS
198	198	100	100	100.0	78523	PASS
199	198	5	9	6.9	5389	PASS
365	198	1	100	4.2	3266	PASS
441	443	0.01	150	84.9	15712	PASS
442	442	100	100	100.0	102557	PASS
443	442	15	24	18.0	18498	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102925\
Data File : BF144120.D
Acq On : 29 Oct 2025 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 29 12:26:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

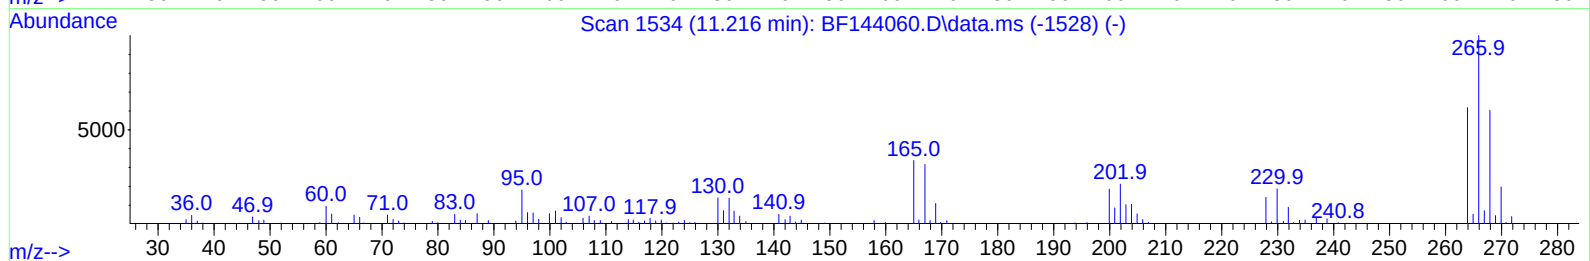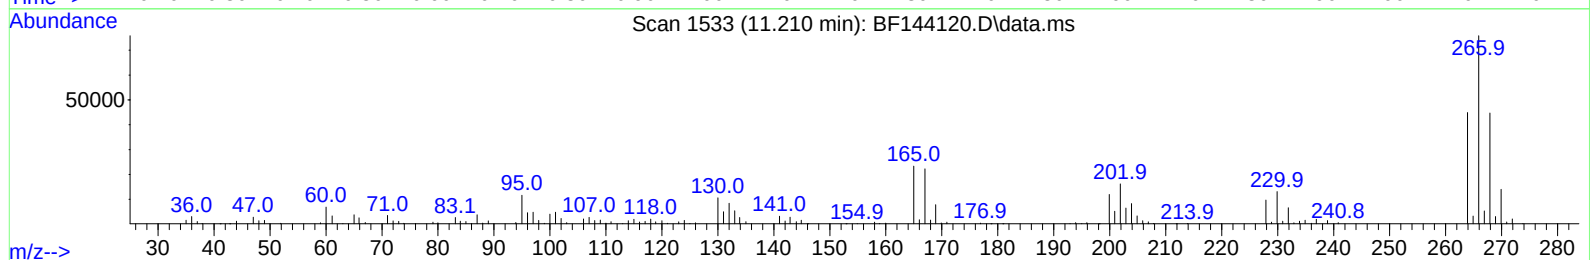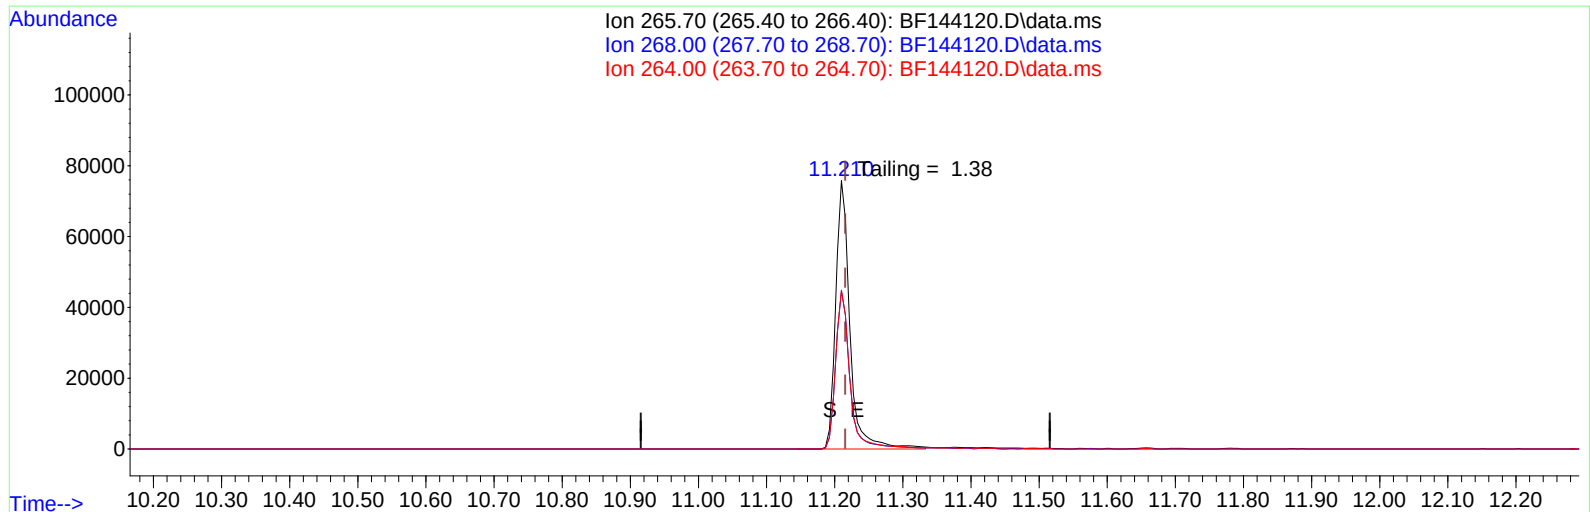

TIC: BF144120.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 40226.81 ng




response 108496

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	59.00
264.00	61.70	59.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102925\
Data File : BF144120.D
Acq On : 29 Oct 2025 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 29 12:26:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

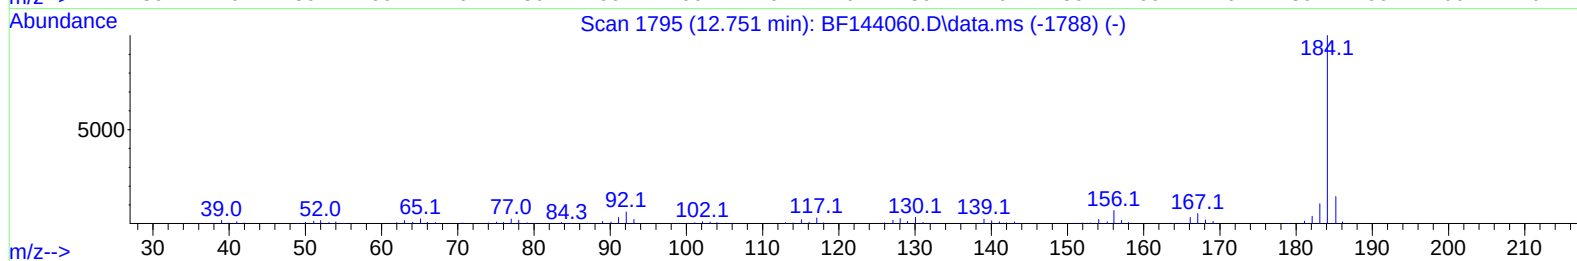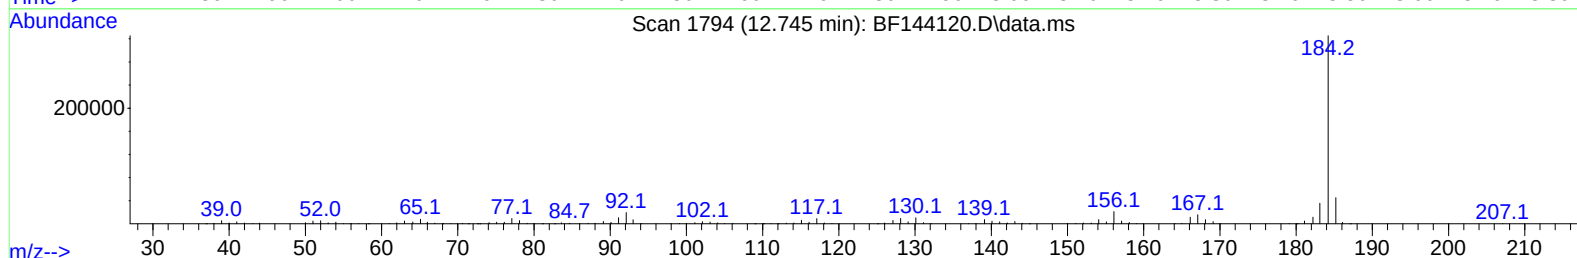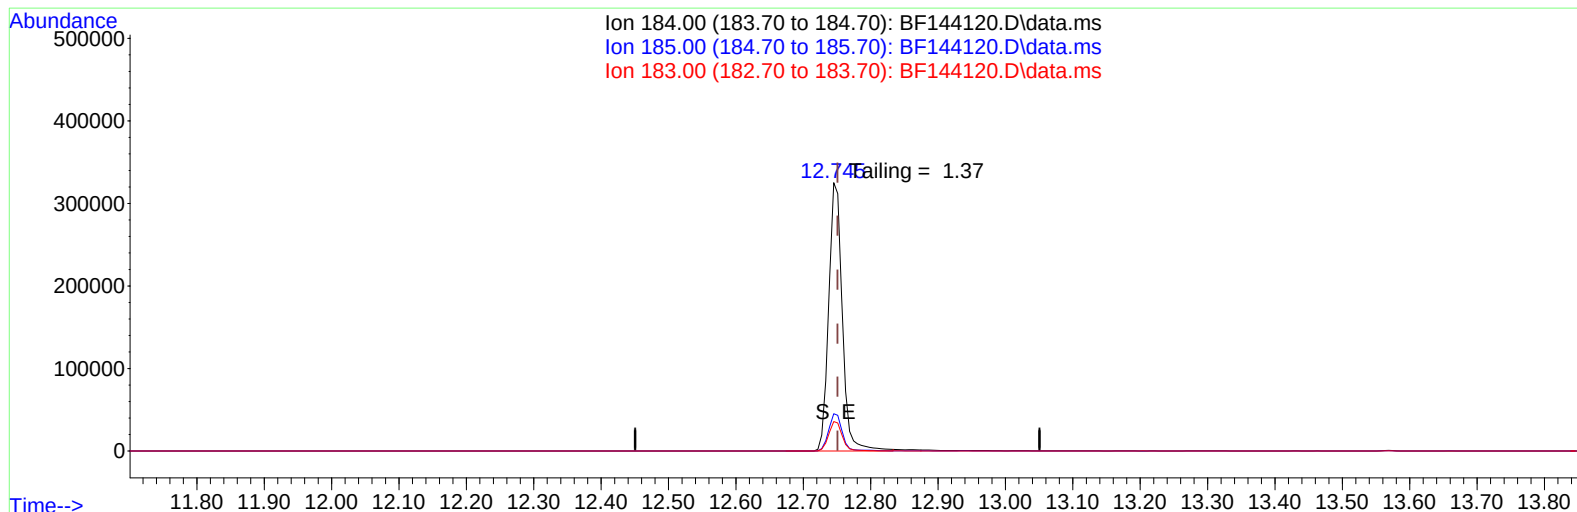

TIC: BF144120.D\data.ms

(77) Benzidine

12.745min (-0.006) 267936.77 ng

response 458627

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.88
183.00	10.60	10.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/29/2025	BNA_F	<u>BF144120.D</u>
Compound Name	Response	Retention Time
DDT	197272	13.569
DDD	5071	13.269
DDE	134	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5205	202477	2.57

Instrument :
BNA_F
ClientSampleId :
DFTPP