
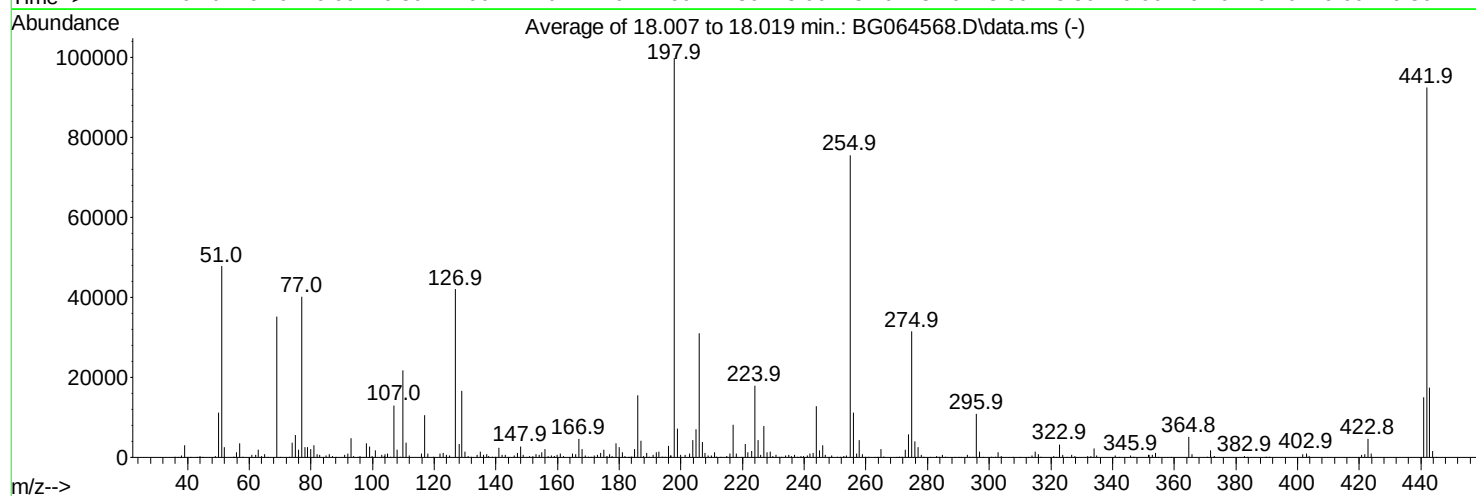


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102425\
Data File : BG064568.D
Acq On : 24 Oct 2025 8:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 16:40:26 2025

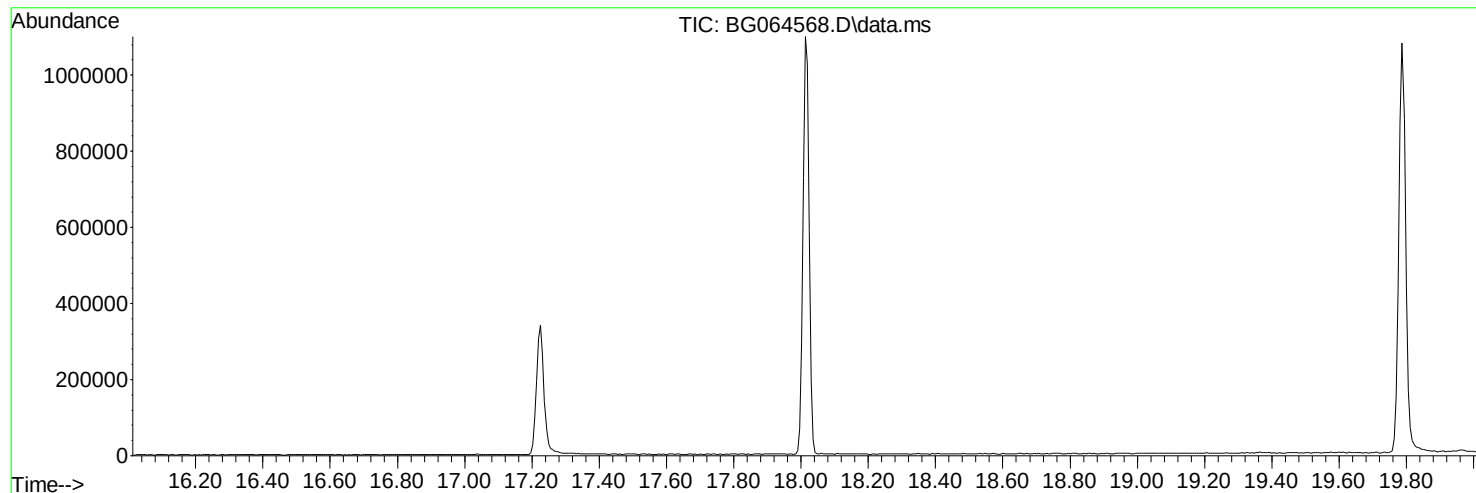




AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2533

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	35203	PASS
70	69	0.00	2	0.2	70	PASS
197	198	0.00	2	0.4	428	PASS
198	198	100	100	100.0	99864	PASS
199	198	5	9	7.2	7222	PASS
365	198	1	100	5.1	5094	PASS
441	443	0.01	150	86.3	15073	PASS
442	442	100	100	100.0	92525	PASS
443	442	15	24	18.9	17468	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102425\
Data File : BG064568.D
Acq On : 24 Oct 2025 8:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 24 12:18:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 12:16:12 2025
Response via : Initial Calibration

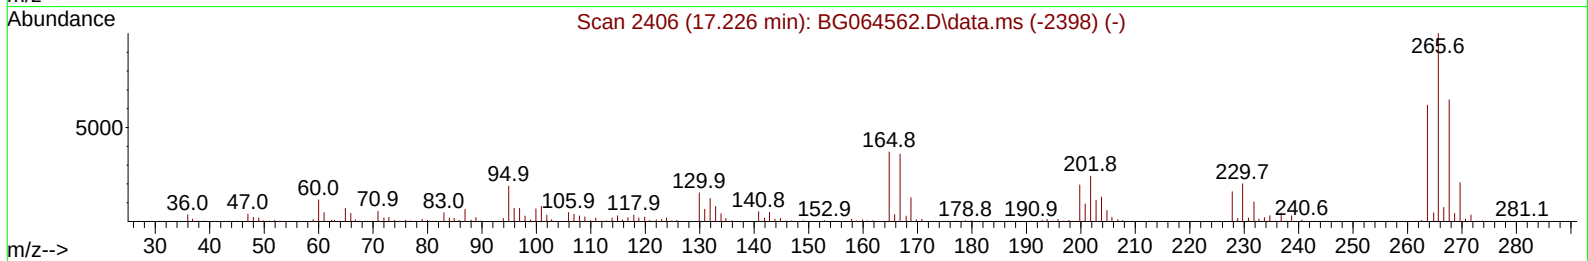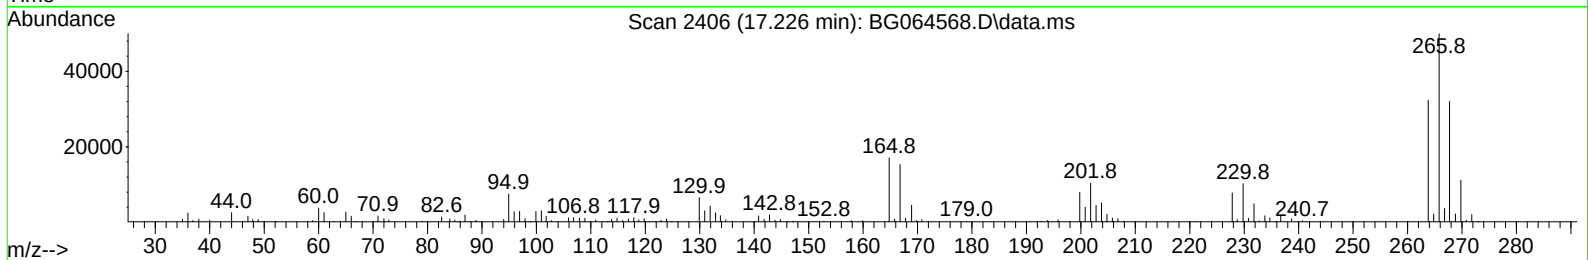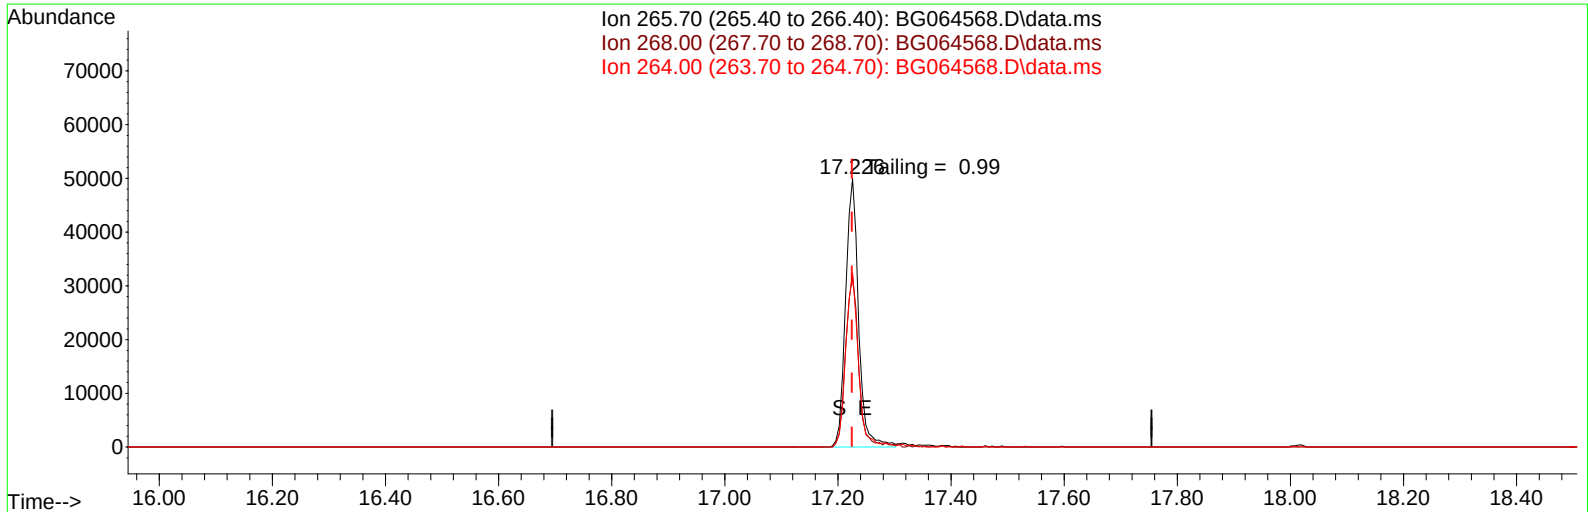

TIC: BG064568.D\data.ms

(70) Pentachlorophenol (C)

17.226min (+ 0.001) 15878.32 ng




response 79720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.10	64.11
264.00	61.90	64.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102425\
Data File : BG064568.D
Acq On : 24 Oct 2025 8:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 24 12:18:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 12:16:12 2025
Response via : Initial Calibration

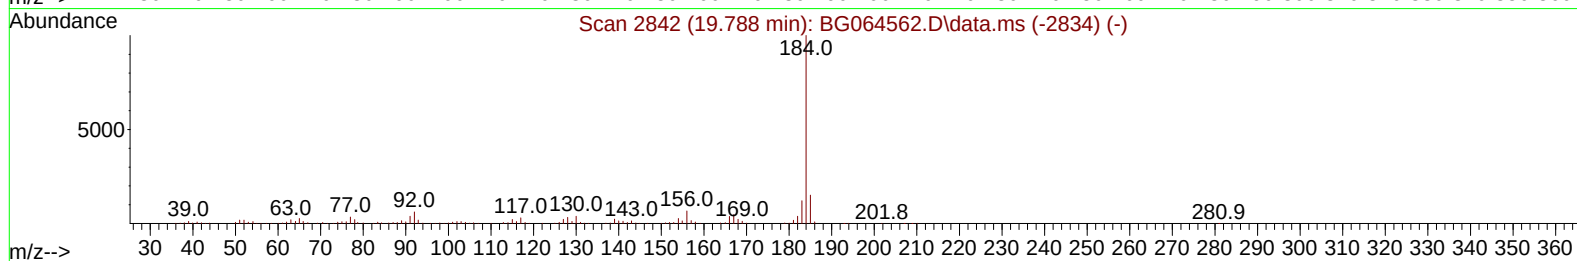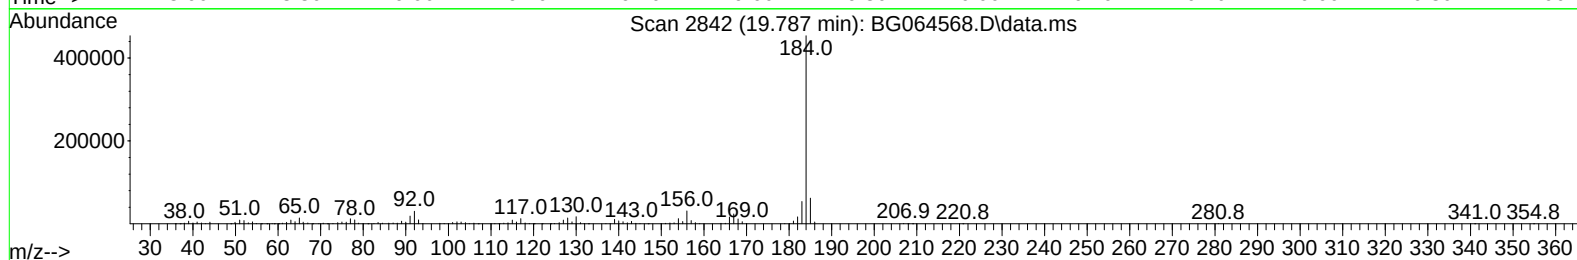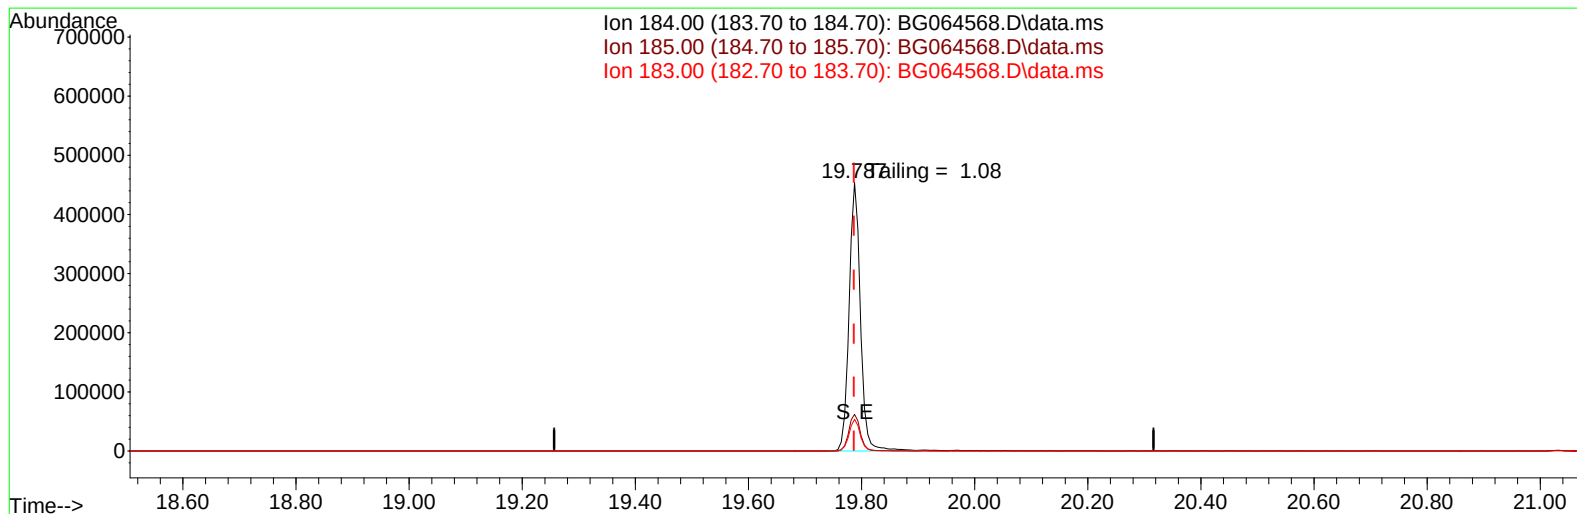

TIC: BG064568.D\data.ms

(77) Benzidine

19.787min (+ 0.001) 0.00 ng

response 632825

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.68
183.00	12.10	11.84
0.00	0.00	0.00

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/24/2025	BNA_G	<u>BG064568.D</u>
Compound Name	Response	Retention Time
DDT	249894	21.033
DDD	4771	20.586
DDE	827	20.087
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5598	255492	2.19