


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
Data File : BG064599.D
Acq On : 28 Oct 2025 13:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 16:40:26 2025

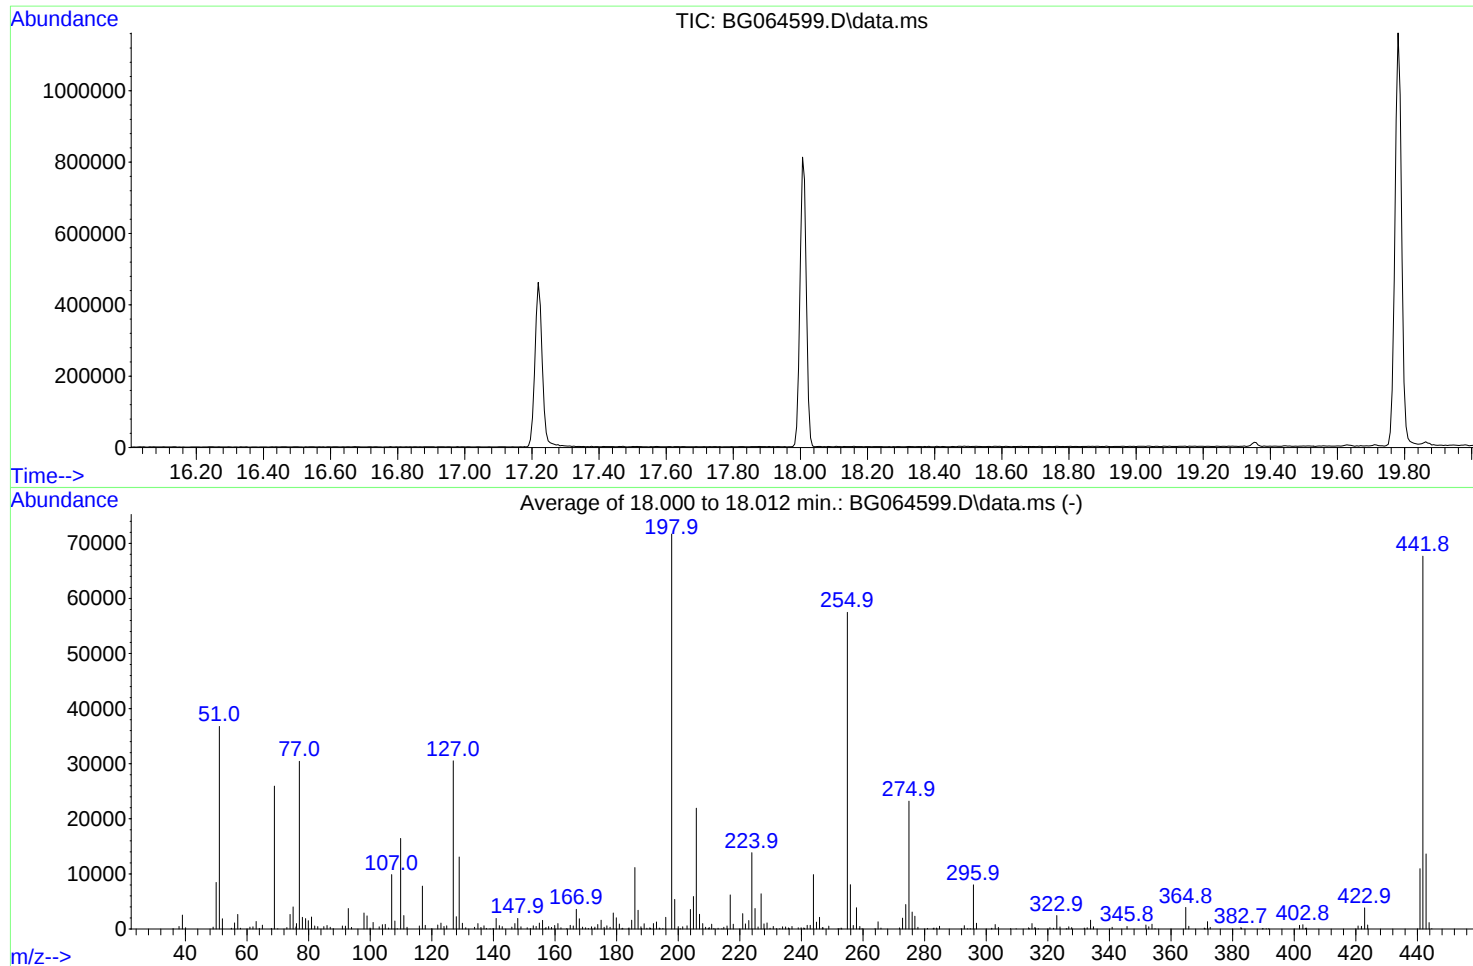

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.5	120	PASS
69	69	100	100	100.0	25923	PASS
70	69	0.00	2	0.2	56	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71661	PASS
199	198	5	9	7.5	5384	PASS
365	198	1	100	5.5	3911	PASS
441	443	0.01	150	80.3	10936	PASS
442	442	100	100	100.0	67661	PASS
443	442	15	24	20.1	13611	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/28/2025	BNA_G	<u>BG064599.D</u>
Compound Name	Response	Retention Time
DDT	283202	21.02
DDD	2284	20.574
DDE	0	19.706
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2284	285486	0.80

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
Data File : BG064599.D
Acq On : 28 Oct 2025 13:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 28 13:46:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

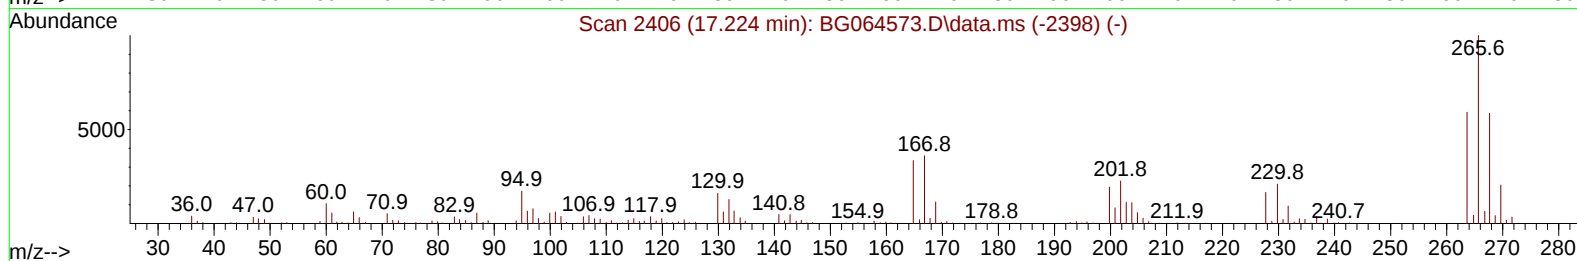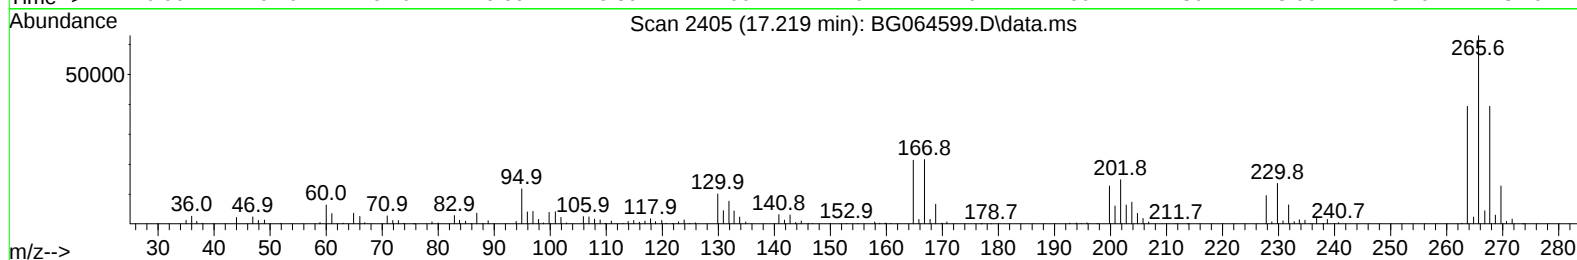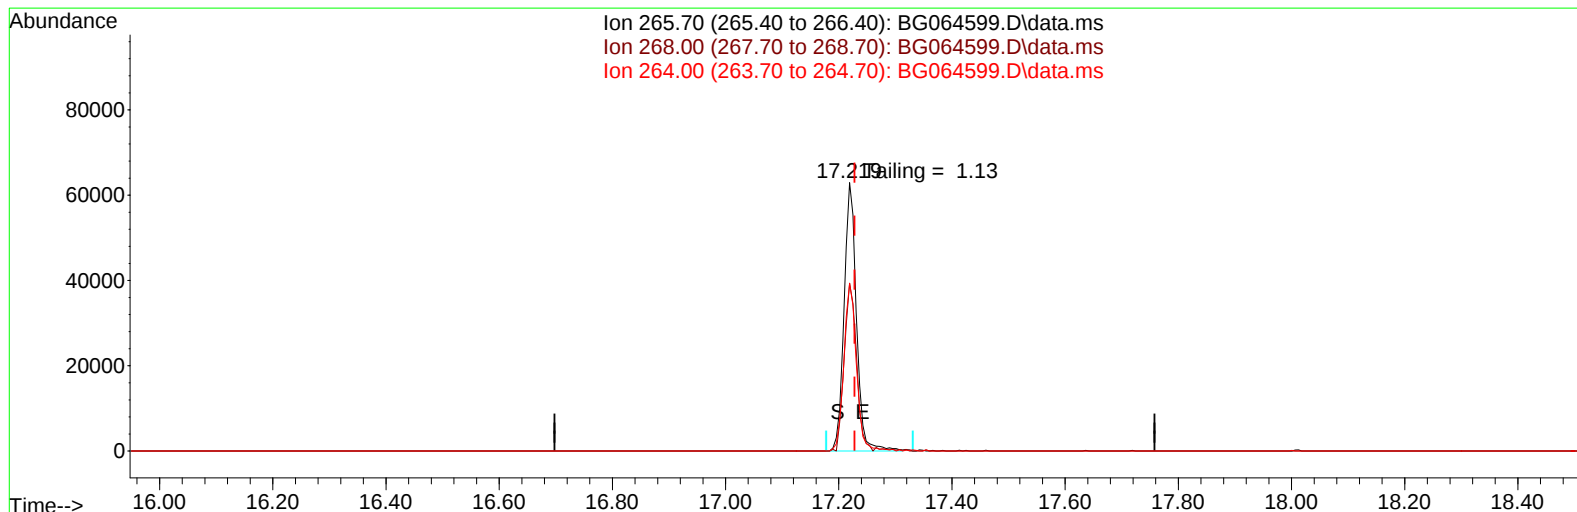

TIC: BG064599.D\data.ms

(70) Pentachlorophenol (C)

17.219min (-0.009) 17647.50 ng




response 95812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	67.39
264.00	59.10	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
Data File : BG064599.D
Acq On : 28 Oct 2025 13:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 28 13:46:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

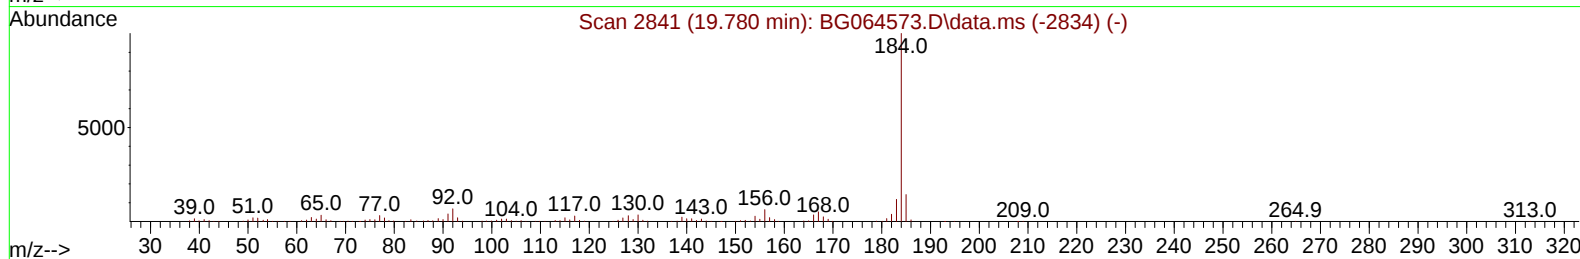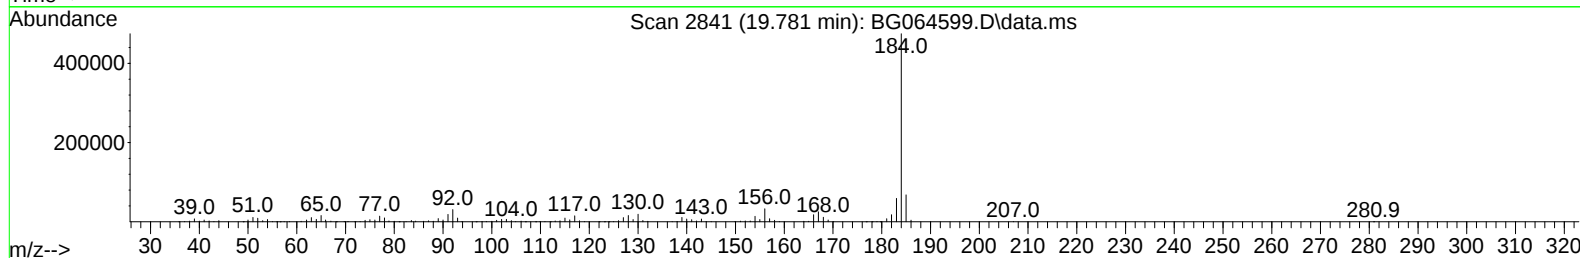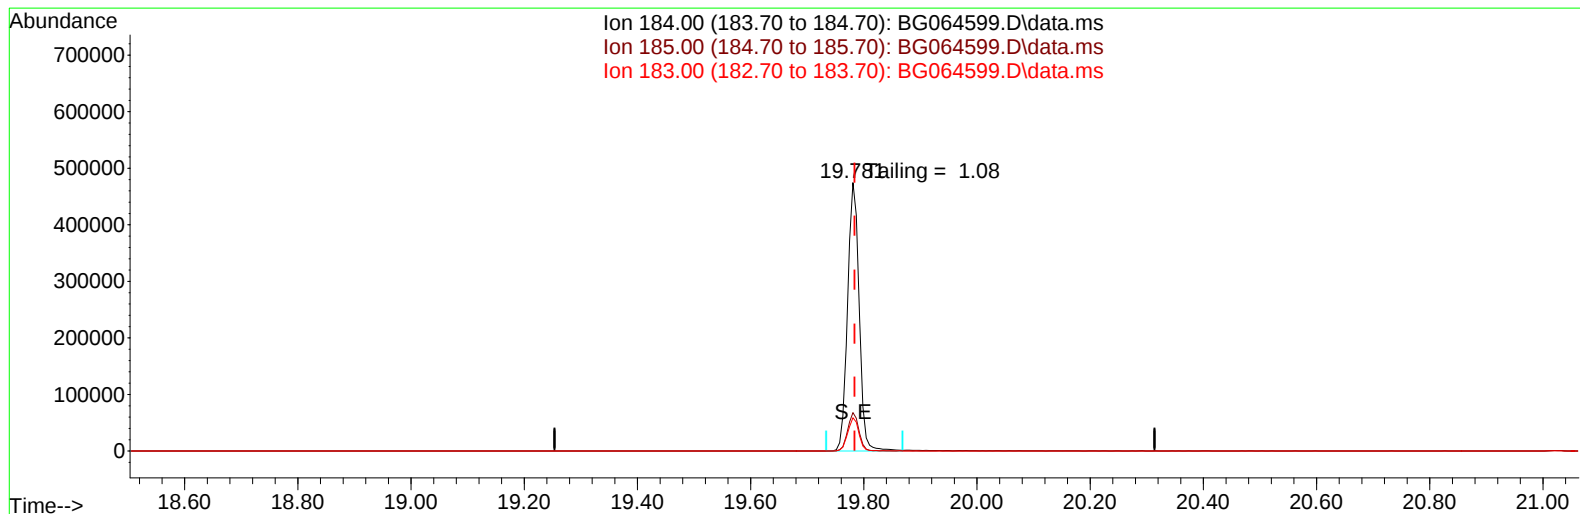

TIC: BG064599.D\data.ms

(77) Benzidine

19.781min (-0.003) 0.00 ng

response 671639

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.33
183.00	11.80	12.43
0.00	0.00	0.00