


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102925\
Data File : BG064617.D
Acq On : 29 Oct 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 16:40:26 2025

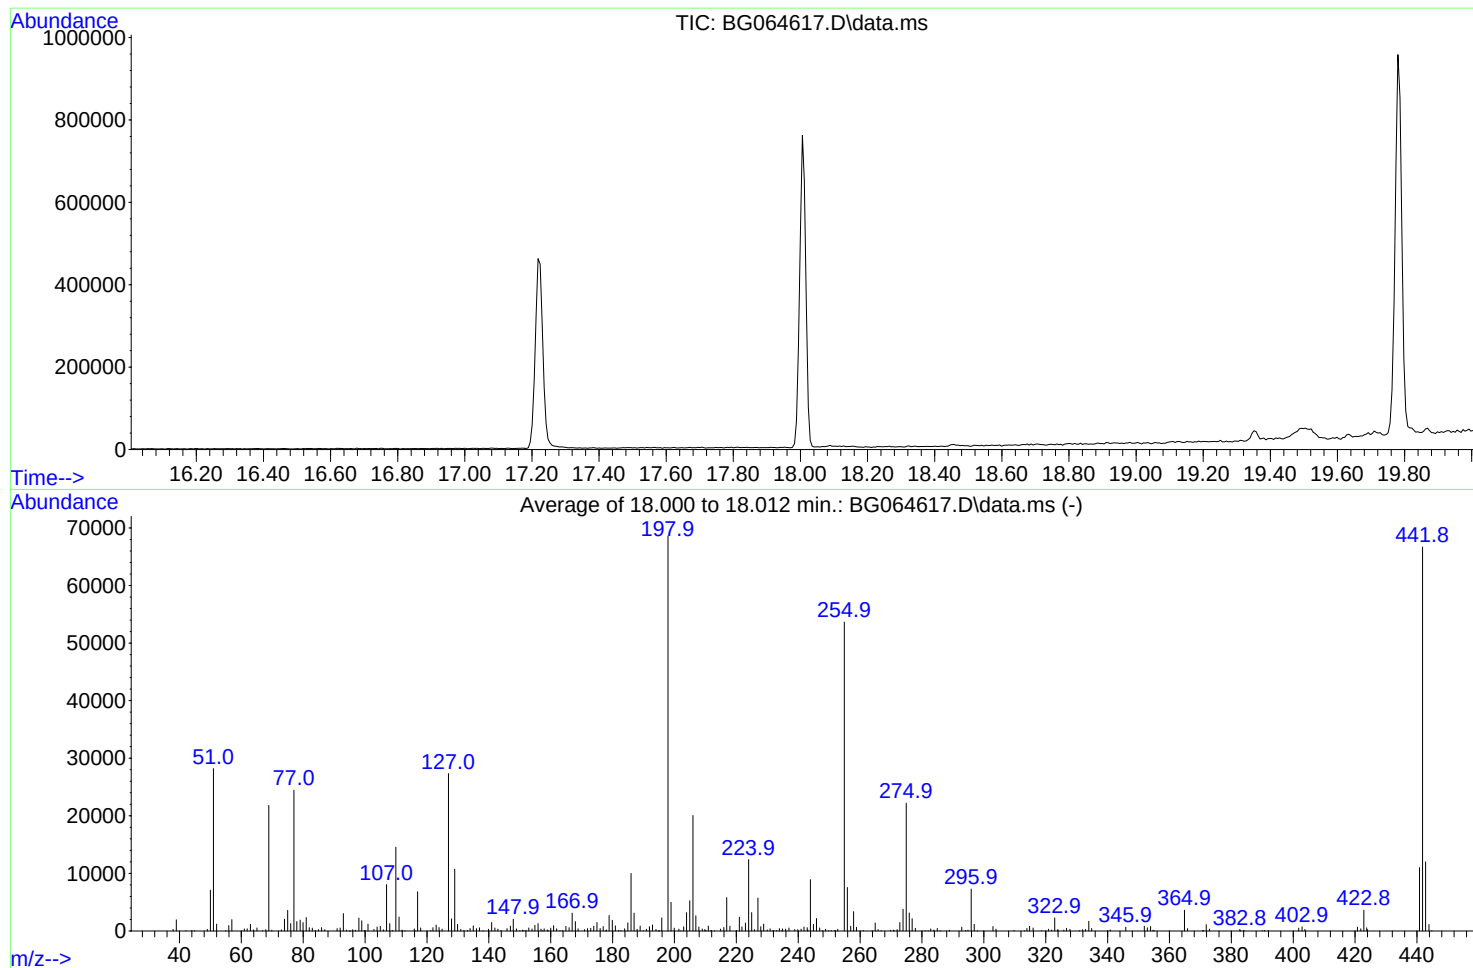

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.0	229	PASS
69	69	100	100	100.0	21821	PASS
70	69	0.00	2	0.6	135	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68565	PASS
199	198	5	9	7.3	4984	PASS
365	198	1	100	5.3	3612	PASS
441	443	0.01	150	91.7	11008	PASS
442	442	100	100	100.0	66685	PASS
443	442	15	24	18.0	12010	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
10/29/2025	BNA_G	<u>BG064617.D</u>
Compound Name	Response	Retention Time
DDT	244663	21.026
DDD	3569	20.573
DDE	0	19.706
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3569	248232	1.44

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102925\
Data File : BG064617.D
Acq On : 29 Oct 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 29 11:21:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

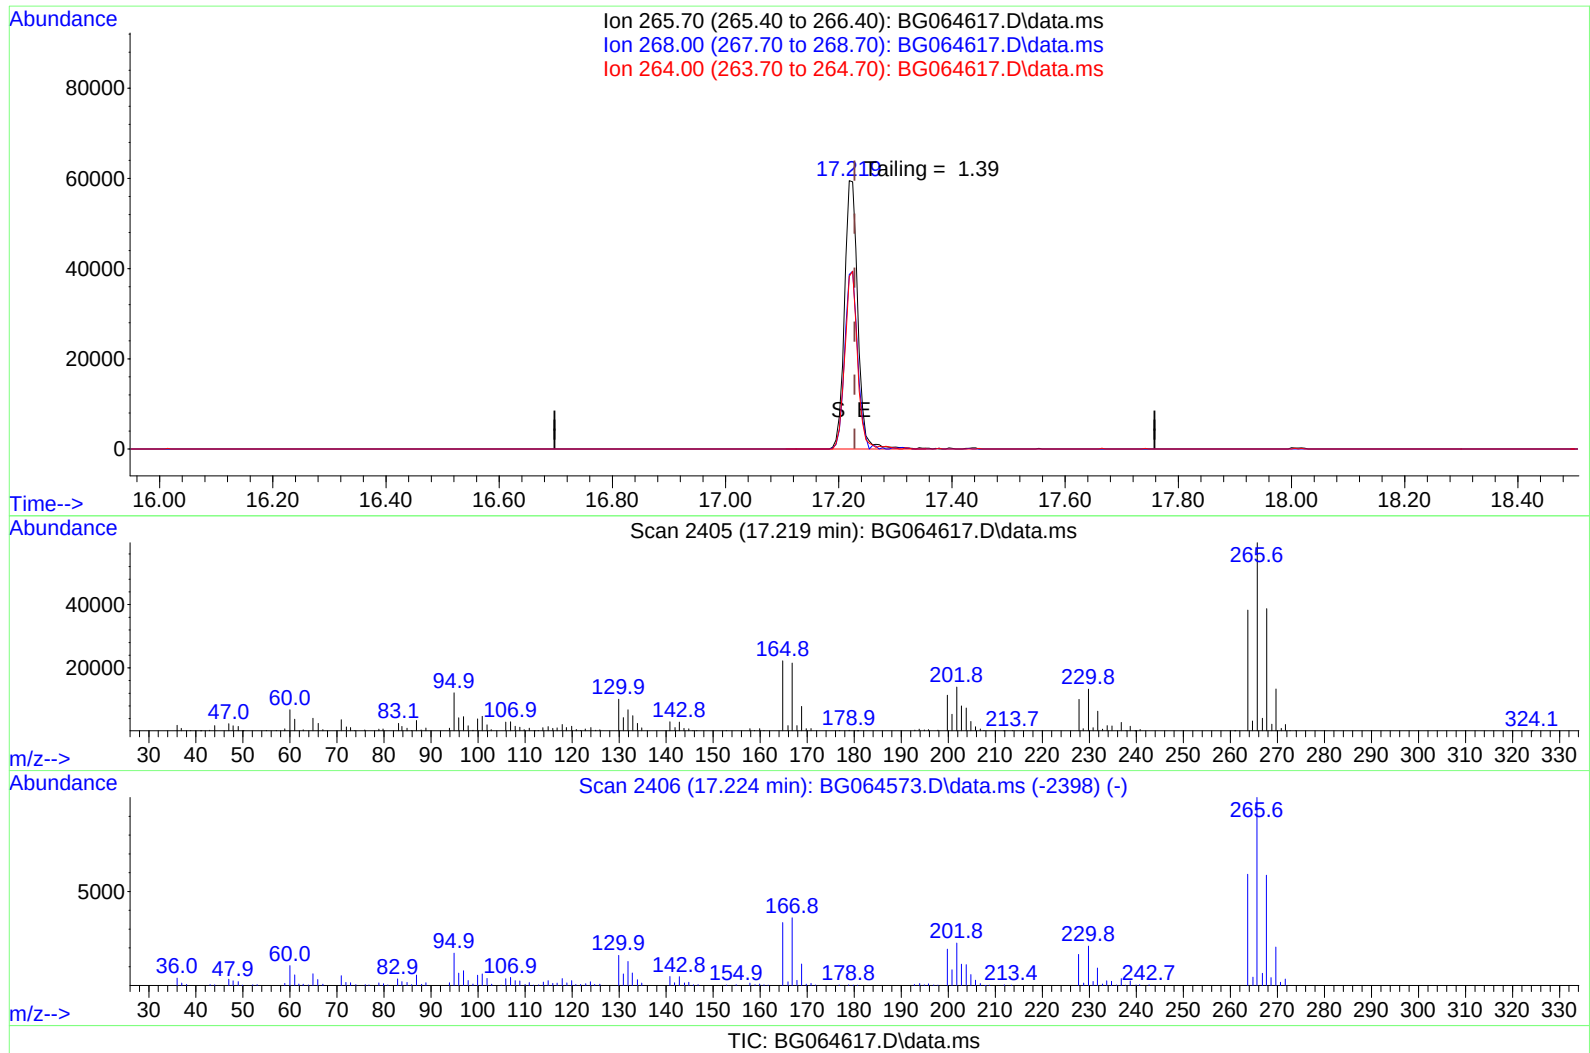

(70) Pentachlorophenol (C)

17.219min (-0.009) 35052.04 ng




response 97221

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.04
264.00	59.10	69.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102925\
Data File : BG064617.D
Acq On : 29 Oct 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 29 11:21:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

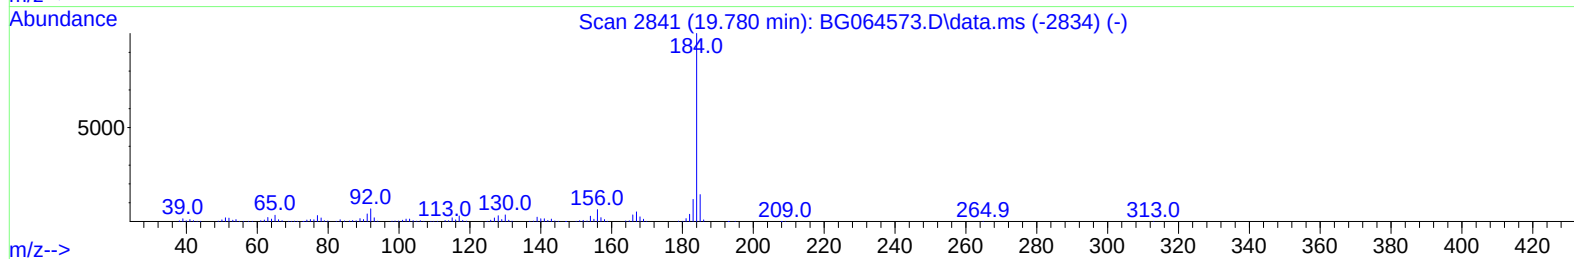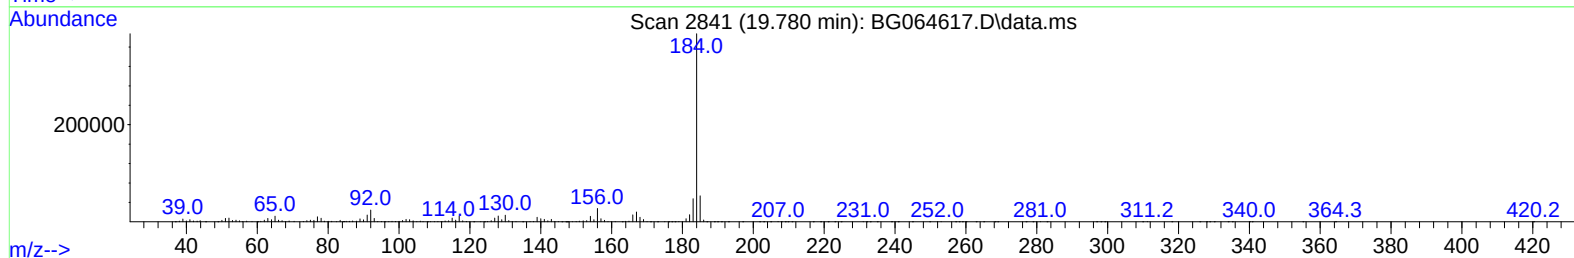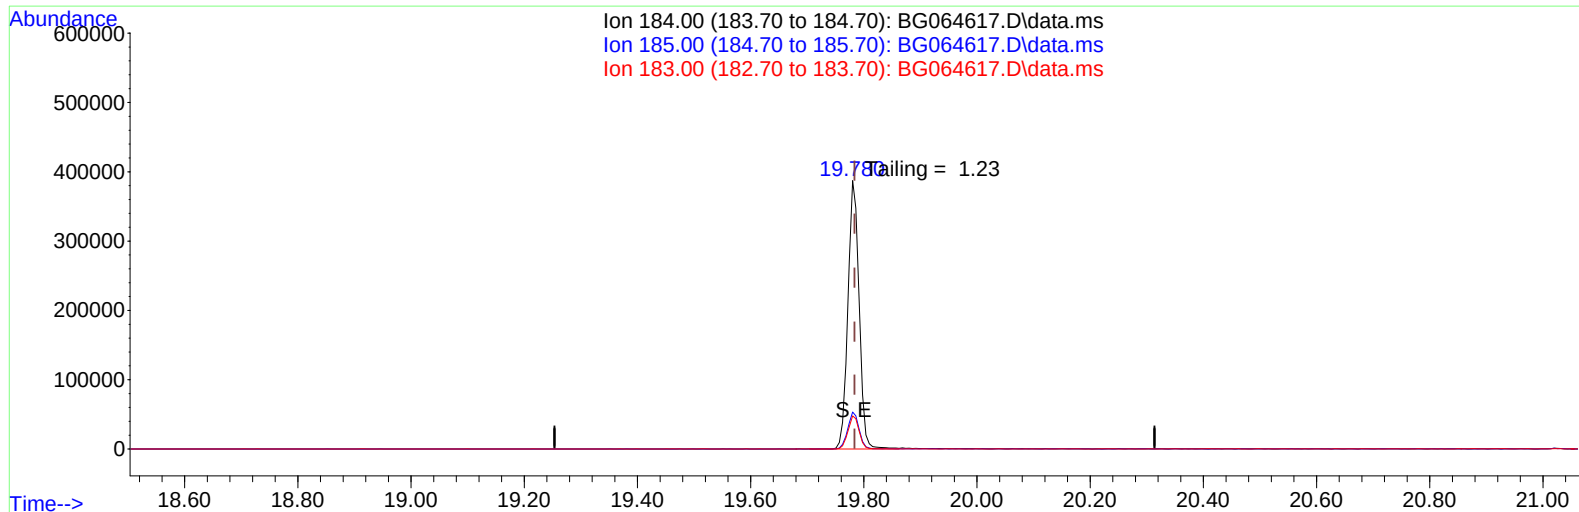

TIC: BG064617.D\data.ms

(77) Benzidine

19.780min (-0.003) 345166.57 ng

response 533588

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.80
183.00	11.80	12.33
0.00	0.00	0.00