


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102825\
Data File : BF144096.D
Acq On : 28 Oct 2025 12:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 17:30:25 2025

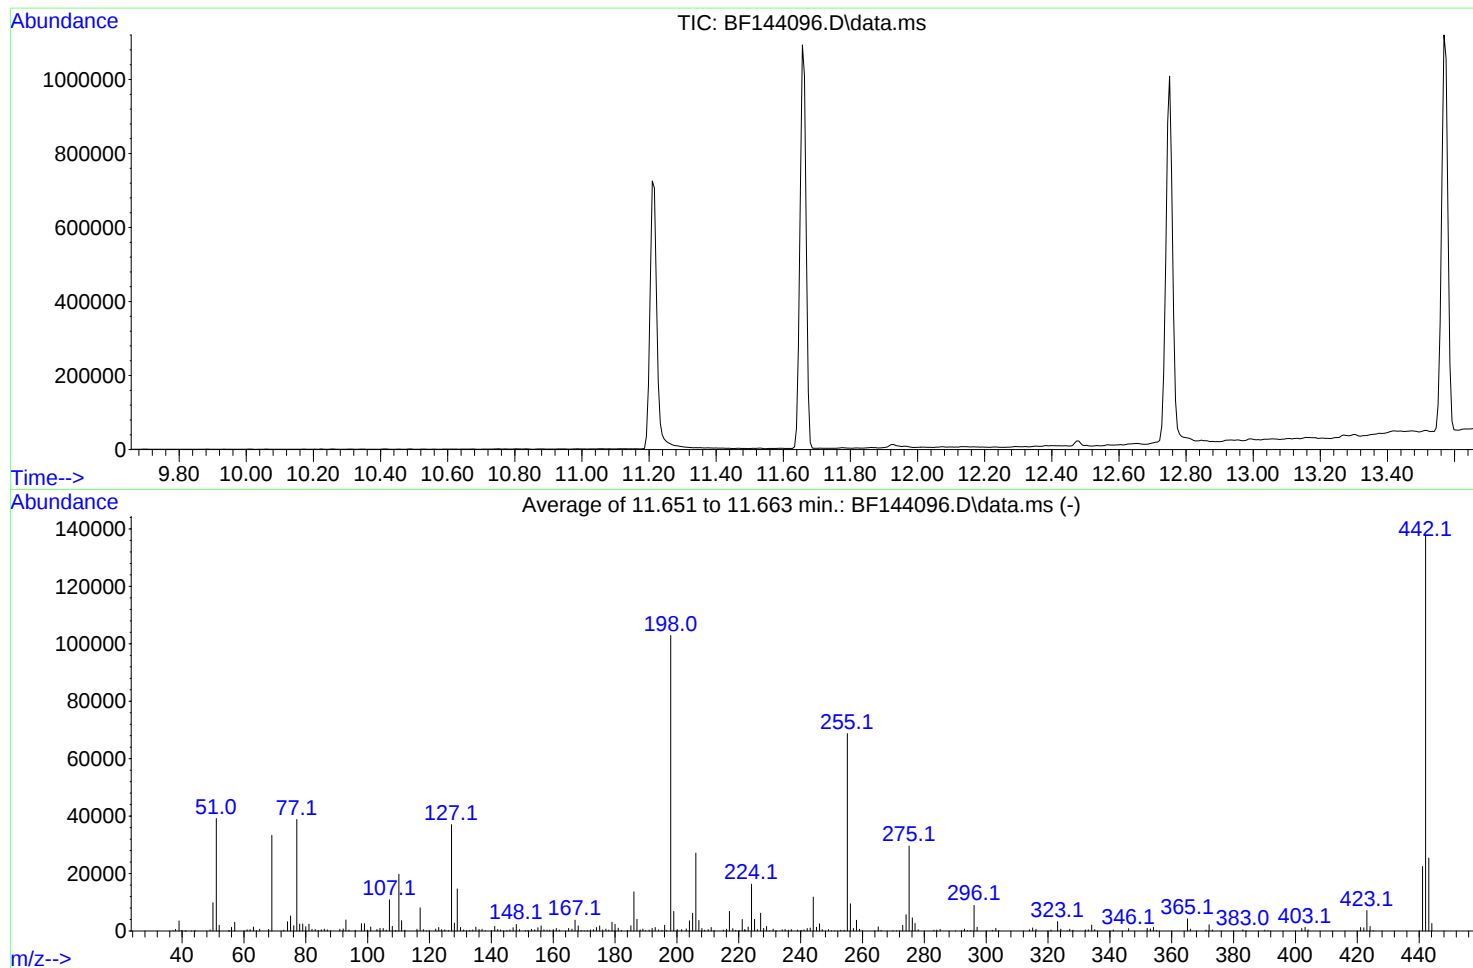

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	551	PASS
69	69	100	100	100.0	33349	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102923	PASS
199	198	5	9	6.6	6806	PASS
365	198	1	100	4.1	4261	PASS
441	443	0.01	150	88.4	22452	PASS
442	442	100	100	100.0	137480	PASS
443	442	15	24	18.5	25399	PASS