

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102825\
 Data File : PD090890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 17:24
 Operator : AR\AJ
 Sample : Q3434-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PR132-WC2-20251022

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/29/2025
 Supervised By : Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:45:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.872	65153787	582.8E6	20.922	19.571m
28)	SA Decachlor...	9.061	8.058	64071886	417.3E6	13.697	13.775

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102825\
Data File : PD090890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 17:24
Operator : AR\AJ
Sample : Q3434-02
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PR132-WC2-20251022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:45:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

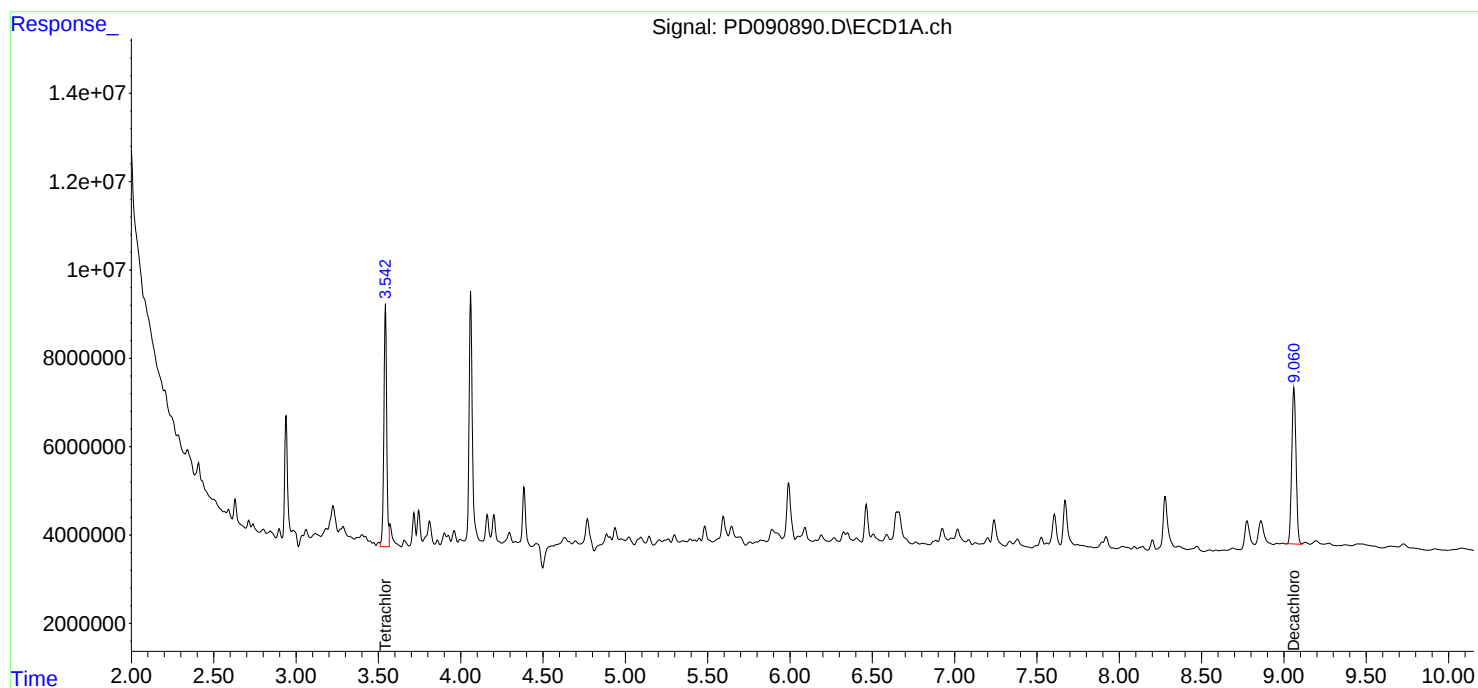

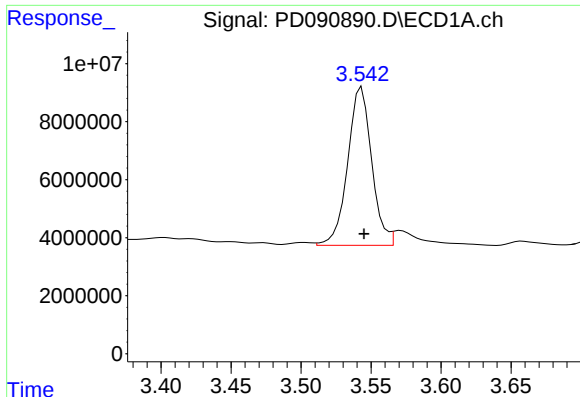


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 65153787
Conc: 20.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PR132-WC2-20251022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

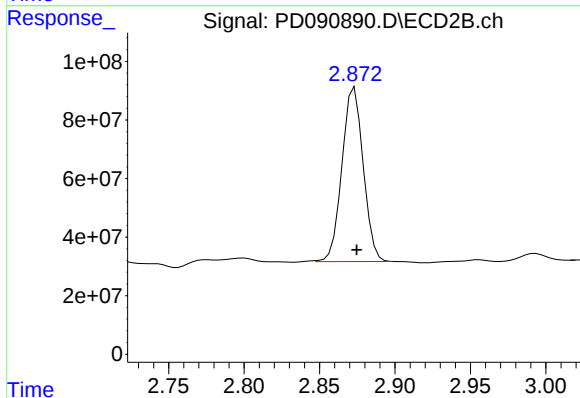


#1 Tetrachloro-m-xylene

R.T.: 2.872 min
Delta R.T.: -0.003 min
Response: 582773028
Conc: 19.57 ng/ml m

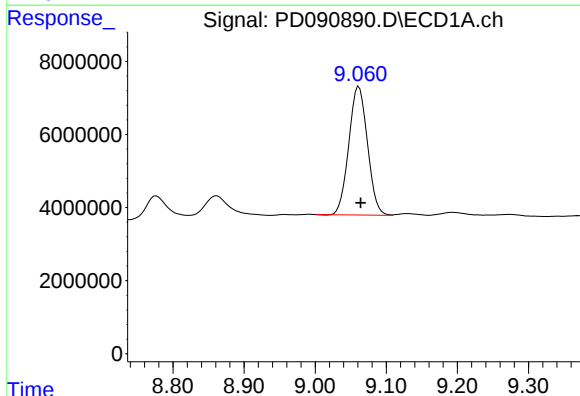

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: -0.003 min
Response: 64071886
Conc: 13.70 ng/ml

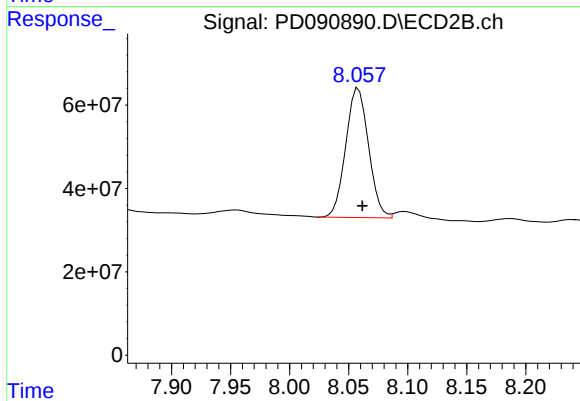

#28 Decachlorobiphenyl

R.T.: 8.058 min
Delta R.T.: -0.003 min
Response: 417252599
Conc: 13.77 ng/ml