

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103025\
Data File : FF016634.D
Signal(s) : FID2B.ch
Acq On : 30 Oct 2025 12:22
Operator : YP\AJ
Sample : PB170324BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB170324BL

Integration File: autoint1.e
Quant Time: Oct 31 02:20:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.057	1694064	16.215 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103025\
Data File : FF016634.D
Signal(s) : FID2B.ch
Acq On : 30 Oct 2025 12:22
Operator : YP\AJ
Sample : PB170324BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB170324BL

Integration File: autoint1.e
Quant Time: Oct 31 02:20:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

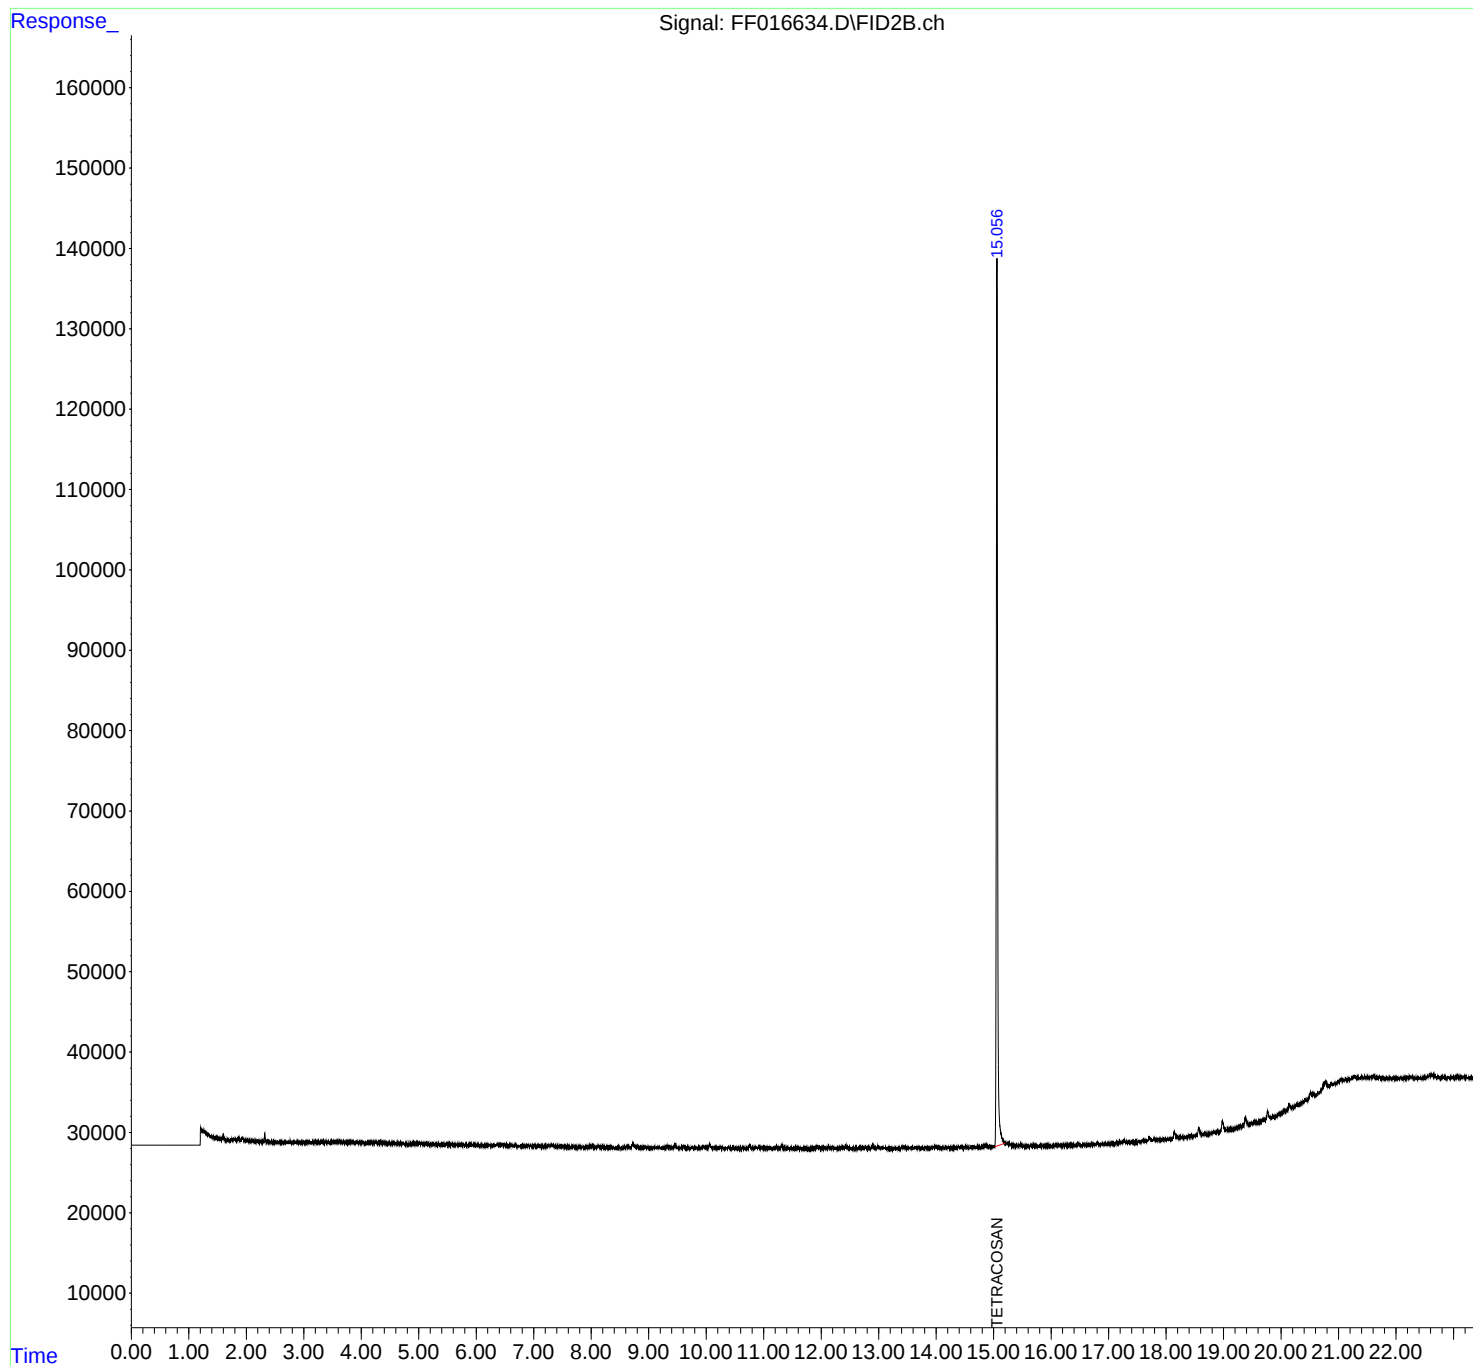

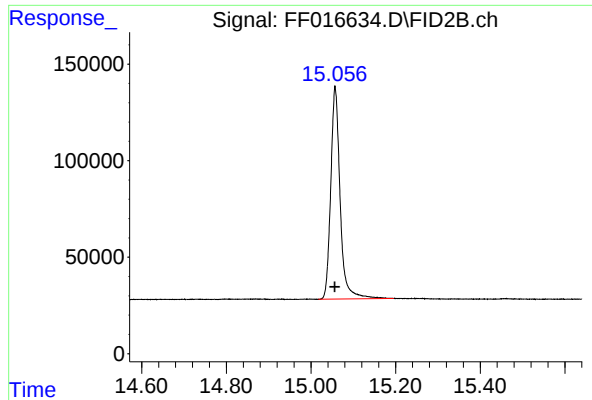

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.057 min
Delta R.T.: 0.001 min
Response: 1694064
Conc: 16.22 ug/ml

Instrument :
FID_F
ClientSampleId :
PB170324BL