

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103025\
Data File : FF016636.D
Signal(s) : FID2B.ch
Acq On : 30 Oct 2025 13:21
Operator : YP\AJ
Sample : Q3434-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PR132-WC1-20251022

Integration File: autoint1.e
Quant Time: Oct 31 02:21:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.056	1134151	10.856 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103025\
Data File : FF016636.D
Signal(s) : FID2B.ch
Acq On : 30 Oct 2025 13:21
Operator : YP\AJ
Sample : Q3434-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PR132-WC1-20251022

Integration File: autoint1.e
Quant Time: Oct 31 02:21:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

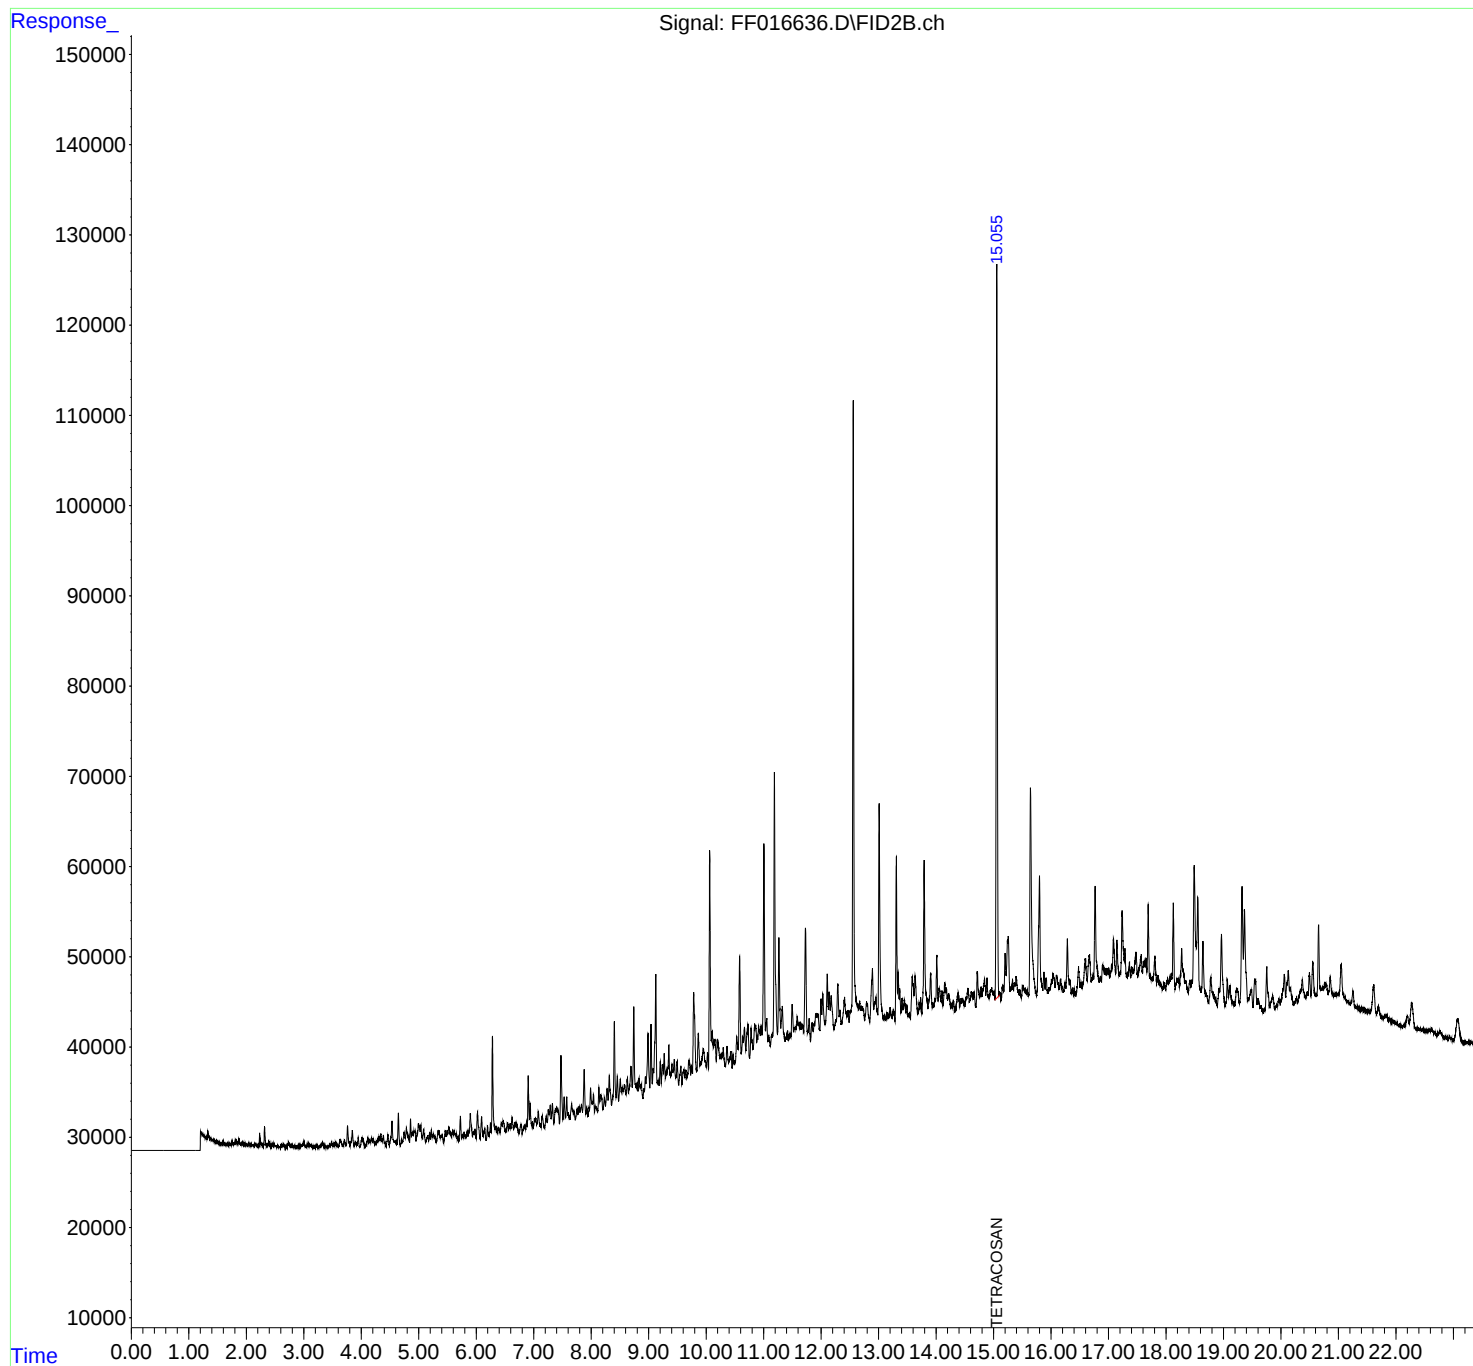

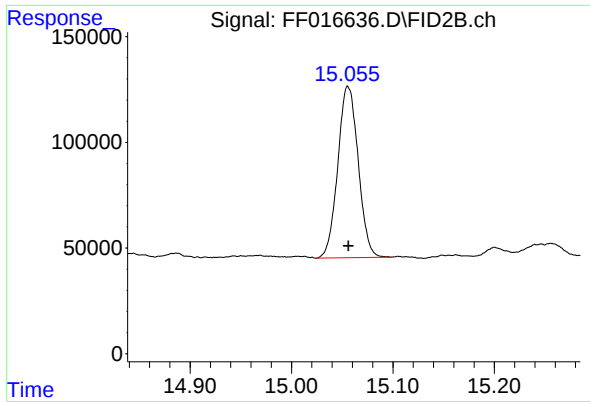

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.056 min
Delta R.T.: 0.000 min
Response: 1134151
Conc: 10.86 ug/ml

Instrument :
FID_F
ClientSampleId :
PR132-WC1-20251022