

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102925\  
 Data File : BG064621.D  
 Acq On : 29 Oct 2025 13:25  
 Operator : RC/JU  
 Sample : PB170215BL  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB170215BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102425.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064621.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.749       | 445           | 453         | 461          | rBV      | 736299         | 1176882       | 29.66%          | 8.360%        |
| 2         | 7.353       | 717           | 726         | 733          | rBV      | 746346         | 1274418       | 32.12%          | 9.053%        |
| 3         | 8.216       | 866           | 873         | 880          | rVB      | 126297         | 212505        | 5.36%           | 1.510%        |
| 4         | 9.380       | 1063          | 1071        | 1078         | rBV      | 442409         | 777277        | 19.59%          | 5.522%        |
| 5         | 11.043      | 1344          | 1354        | 1362         | rBV      | 162352         | 294281        | 7.42%           | 2.090%        |
| 6         | 13.469      | 1760          | 1767        | 1774         | rBV      | 1202173        | 1855560       | 46.77%          | 13.181%       |
| 7         | 14.838      | 1993          | 2000        | 2008         | rBV      | 270056         | 418534        | 10.55%          | 2.973%        |
| 8         | 16.313      | 2244          | 2251        | 2263         | rBV      | 1042193        | 1646496       | 41.50%          | 11.696%       |
| 9         | 17.576      | 2459          | 2466        | 2473         | rBV      | 394044         | 587050        | 14.80%          | 4.170%        |
| 10        | 20.167      | 2901          | 2907        | 2917         | rBV      | 3054784        | 3967474       | 100.00%         | 28.184%       |
| 11        | 21.848      | 3186          | 3193        | 3201         | rBV2     | 492613         | 821231        | 20.70%          | 5.834%        |
| 12        | 24.286      | 3601          | 3608        | 3615         | rVB3     | 25469          | 62345         | 1.57%           | 0.443%        |
| 13        | 25.191      | 3751          | 3762        | 3772         | rBV      | 308414         | 911115        | 22.96%          | 6.472%        |
| 14        | 26.495      | 3977          | 3984        | 3996         | rVB5     | 25920          | 72023         | 1.82%           | 0.512%        |




Sum of corrected areas: 14077191

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102925\  
Data File : BG064621.D  
Acq On : 29 Oct 2025 13:25  
Operator : RC/JU  
Sample : PB170215BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB170215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

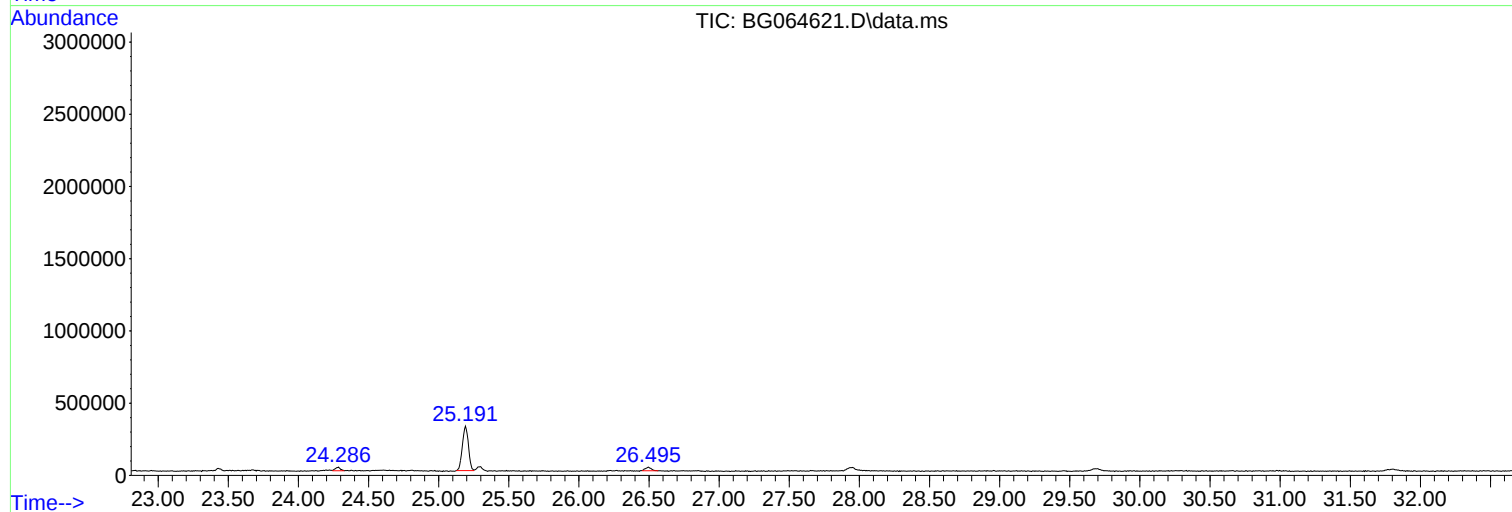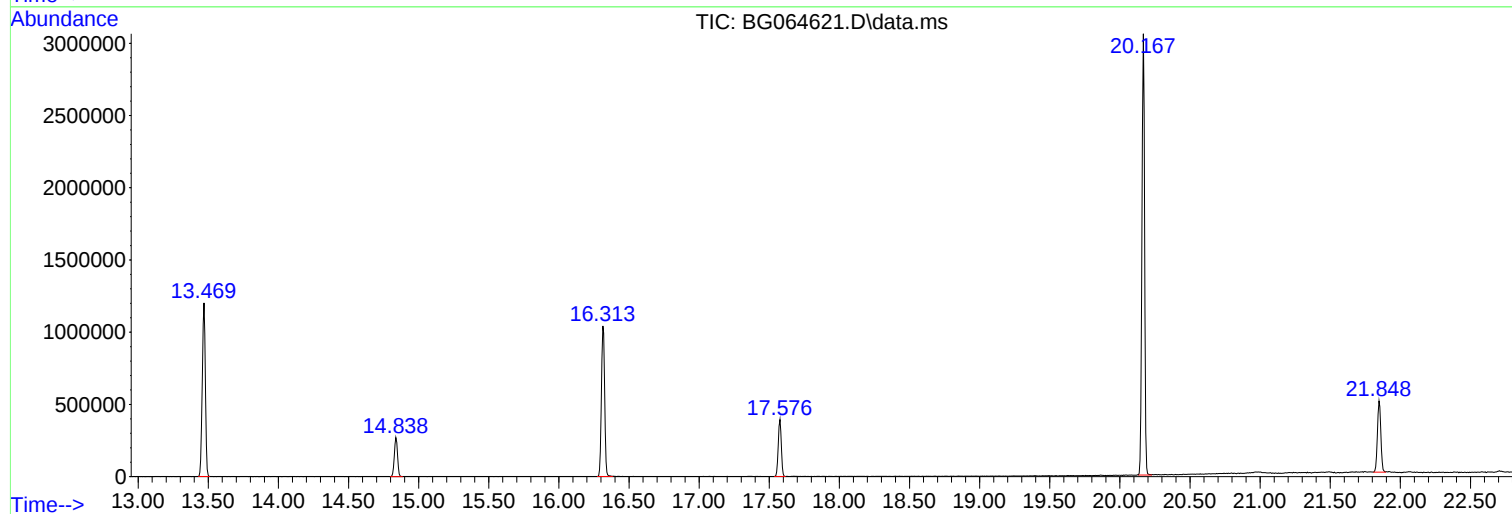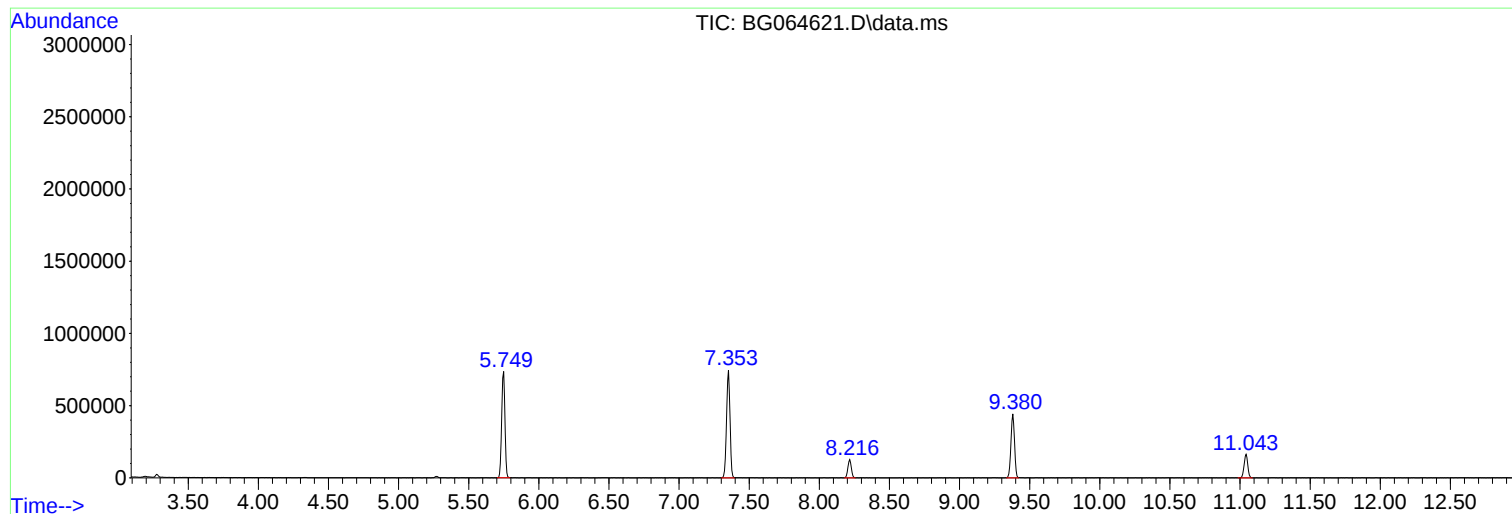

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102925\  
Data File : BG064621.D  
Acq On : 29 Oct 2025 13:25  
Operator : RC/JU  
Sample : PB170215BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB170215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102925\  
Data File : BG064621.D  
Acq On : 29 Oct 2025 13:25  
Operator : RC/JU  
Sample : PB170215BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB170215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|