


LB137666

7470A

INSTRUMENT ID:CV1

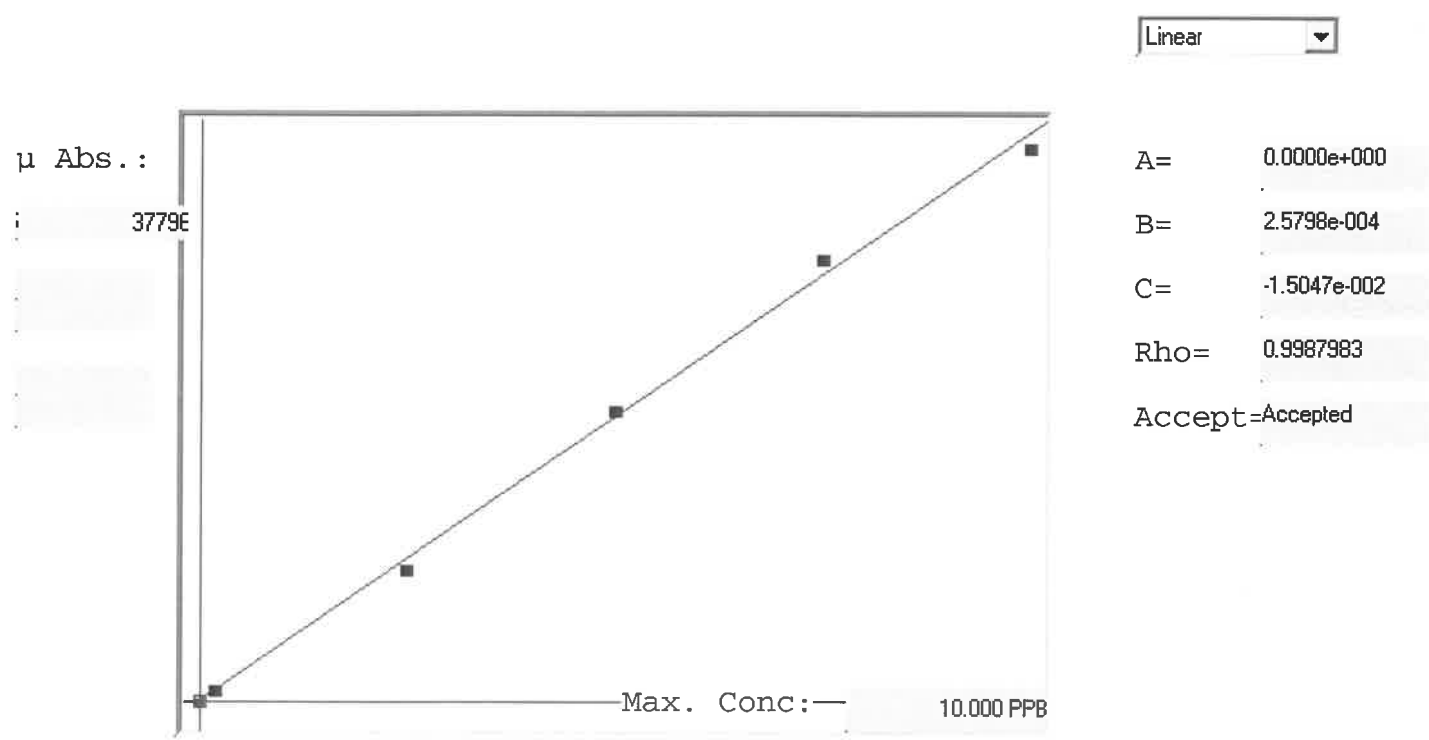

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.014	-0.014	3	0.000	3	0			
0.2	0.200	0.214	0.014	888	0.0 %	888	0			
2.5	2.500	2.346	-0.154	9153	0.0 %	9153	0			
5.0	5.000	5.123	0.123	19918	0.0 %	19918				
7.5	7.500	7.795	0.295	30274	0.0 %	30274				
10.0	10.000	9.736	-0.264	37796	0.0 %	37796				

LB170666 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Oct 2025 08:50:10

Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	50	-	3	PPB	Std	0.0000	7470A	28 Oct 2025 09:02:38
S	0.2 - 1	51.2	-	888	PPB	Std	0.2000	7470A	28 Oct 2025 09:04:56
S	2.5 - 1	52.5	-	9153	PPB	Std	2.5000	7470A	28 Oct 2025 09:07:13
S	5.0 - 1	55	-	19918	PPB	Std	5.0000	7470A	28 Oct 2025 09:09:30
S	7.5 - 1	57.5	-	30274	PPB	Std	7.5000	7470A	28 Oct 2025 09:11:49
S	10.0 - 1	510	-	37796	PPB	Std	10.0000	7470A	28 Oct 2025 09:17:09
U	ICV89 - 1	ICV89	3.7484	14588	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:25:36
U	ICB89 - 1	ICB89	-0.0705	-215	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:27:52
U	CCV93 - 1	CCV93	5.2312	20336	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:30:10
U	CCB93 - 1	CCB93	-0.0723	-222	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:32:25
U	CRA - 1	CRA	0.2053	854	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:34:45
U	HighStd - 1	HighStd	9.6752	37562	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:37:00
U	ChkStd - 1	ChkStd	6.5379	25401	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:39:15
U	PB170268BL - 1	PBW	-0.0171	-8	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:44:28
U	PB170268BS - 1	LCSW	3.8023	14797	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:46:43
U	Q3439-04 - 1	TP-9	-0.0705	-215	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:49:00
U	Q3439-08 - 1	TP-10	-0.0163	-5	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:51:19
U	Q3440-04 - 1	JB-2	0.0244	153	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:53:36
U	Q3446-01 - 1	SB-14	-0.0218	-26	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:55:53
U	Q3446-02 - 1	SB-15	-0.0254	-40	PPB	SMPL	-7470A	-7470A	28 Oct 2025 09:58:08
U	CCV94 - 1	CCV94	4.8742	18952	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:00:24
U	CCB94 - 1	CCB94	-0.0138	5	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:05:25
U	Q3446-03 - 1	SB-16	-0.0032	46	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:07:40
U	Q3446-04 - 1	SB-17	-0.0076	29	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:09:55
U	Q3446-05 - 1	SB-18	-0.0145	2	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:12:10
U	Q3446-06 - 1	SB-19	-0.0050	39	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:14:26
U	Q3446-07 - 1	SB-20	-0.0212	-24	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:16:42
U	Q3446-08 - 1	SB-21	-0.0140	4	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:18:58
U	Q3447-02 - 1	P001-TW1-251023-01	-0.0158	-3	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:21:15
U	Q3447-04 - 1	P001-TW2-251023-01	-0.0143	3	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:23:32
U	Q3447-06 - 1	P001-TW3-251023-01	-0.0148	1	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:25:48
U	Q3447-08 - 1	P001-TW4-251023-01	-0.0158	-3	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:28:04
U	CCV95 - 1	CCV95	4.6949	18257	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:30:20
U	CCB95 - 1	CCB95	-0.0264	-44	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:35:23
U	Q3449-06 - 1	CF-620-COMP-41	-0.0179	-11	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:37:38
U	Q3451-04 - 1	TP-11	-0.0112	15	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:39:54
U	Q3451-08 - 1	TP-12	-0.0042	42	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:42:09
U	Q3452-04 - 1	JB-1	-0.0042	42	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:44:25
U	Q3452-04DUP - 1	JB-1DUP	-0.0058	36	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:46:41
U	Q3452-04MS - 1	JB-1MS	3.9460	15354	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:48:57
U	Q3452-04MSD - 1	JB-1MSD	3.9684	15441	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:51:13
U	PB170239TB - 1	PB170239TB	-0.0806	-254	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:53:33
U	Q3452-04LX5 - 1		-0.0150	0	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:55:53
U	Q3452-04A - 1		3.5482	13812	PPB	SMPL	-7470A	-7470A	28 Oct 2025 10:58:09
U	CCV96 - 1	CCV96	5.1631	20072	PPB	SMPL	-7470A	-7470A	28 Oct 2025 11:00:24
U	CCB96 - 1	CCB96	-0.0819	-259	PPB	SMPL	-7470A	-7470A	28 Oct 2025 11:02:43