

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102825\
 Data File : PP076120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 12:09
 Operator : YP\AJ
 Sample : Q3447-01RE 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P001-TW1-251023-01RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/29/2025
 Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 14:05:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.624	3.812f	3834805	123.2E6	2.683m	18.622m#
2) SA Decachlor...	10.407	8.780	3032665	1788403	2.817	0.217 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102825\
Data File : PP076120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 12:09
Operator : YP\AJ
Sample : Q3447-01RE 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
P001-TW1-251023-01RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 14:05:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

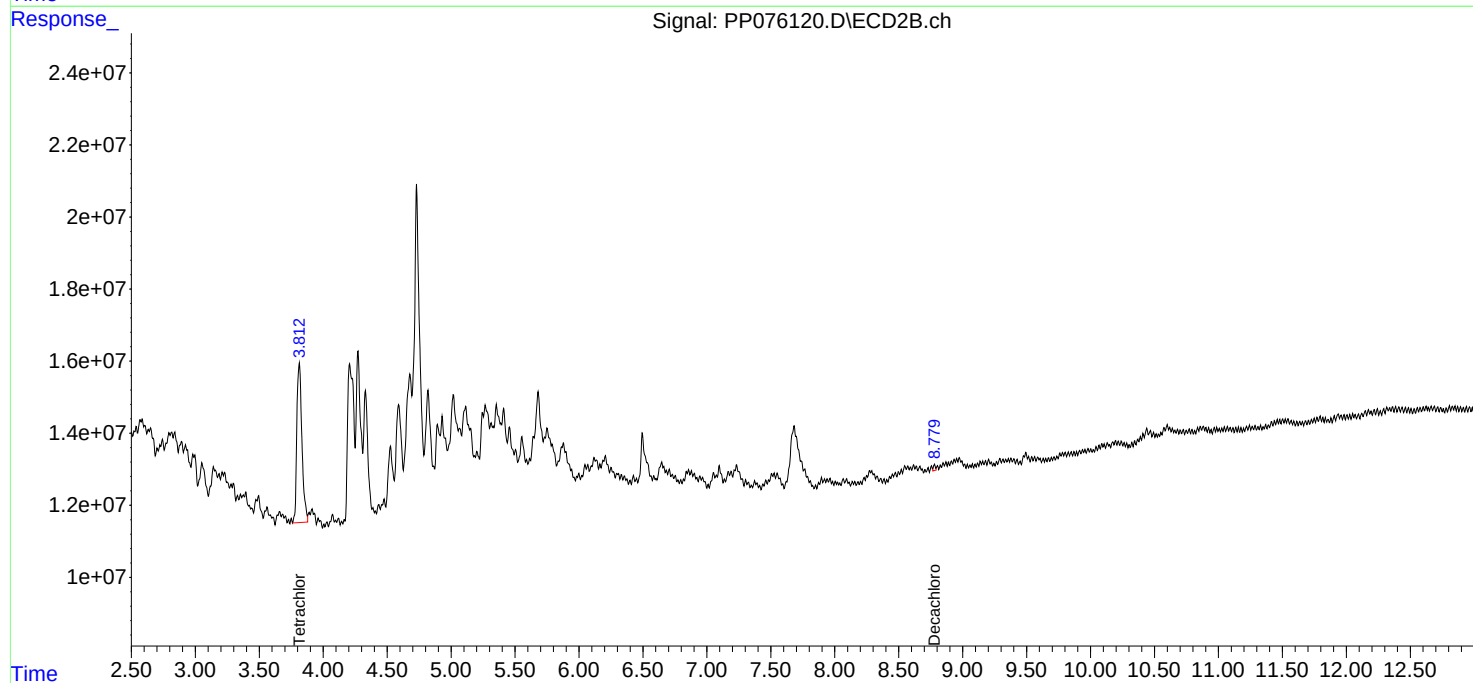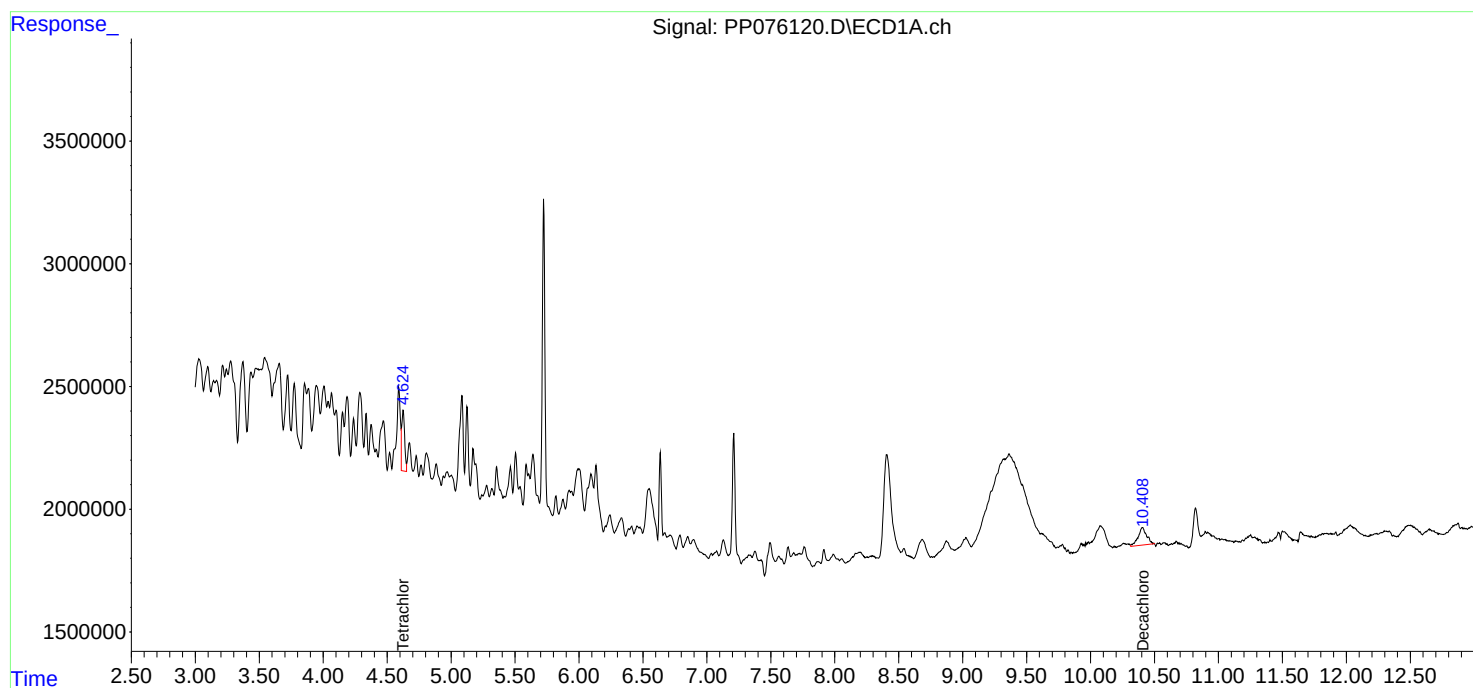

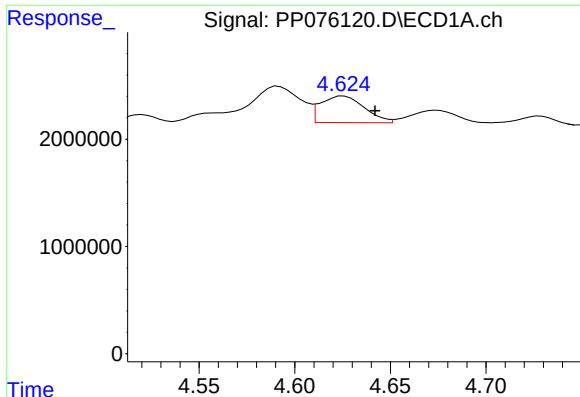


#1 Tetrachloro-m-xylene

R.T.: 4.624 min
Delta R.T.: -0.018 min
Response: 3834805
Conc: 2.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
P001-TW1-251023-01RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

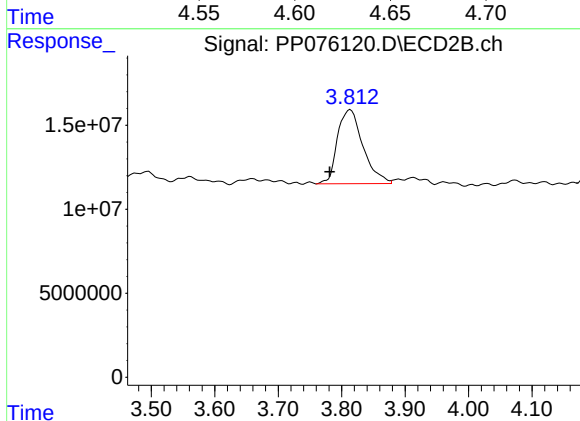


#1 Tetrachloro-m-xylene

R.T.: 3.812 min
Delta R.T.: 0.031 min
Response: 123244980
Conc: 18.62 ng/ml m

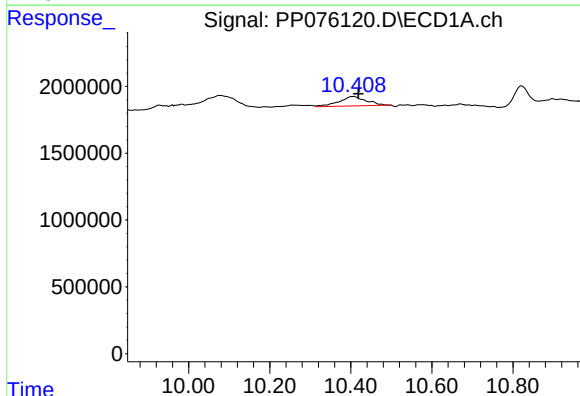

#2 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.012 min
Response: 3032665
Conc: 2.82 ng/ml

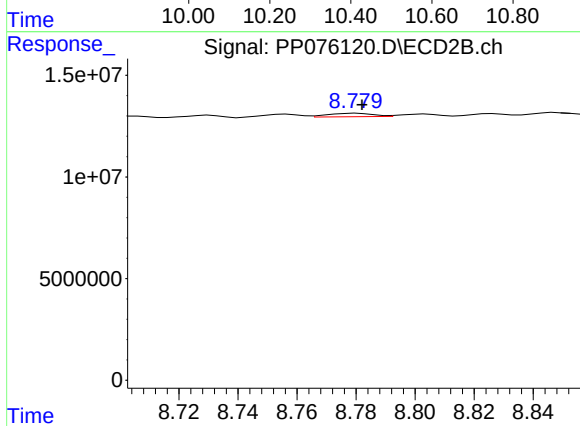

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.002 min
Response: 1788403
Conc: 0.22 ng/ml