

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102425\
 Data File : PD090826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2025 16:38
 Operator : AR\AJ
 Sample : Q3447-07 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P001-TW4-251023-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/27/2025
 Supervised By : mohammad ahmed 10/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 23:39:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.876	2706320	18053065	0.869	0.606m#
2) SA Decachlor...	9.084	8.060	43974566	34651815	9.400m	1.144m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102425\
Data File : PD090826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2025 16:38
Operator : AR\AJ
Sample : Q3447-07 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P001-TW4-251023-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/27/2025
Supervised By :mohammad ahmed 10/28/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 23:39:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

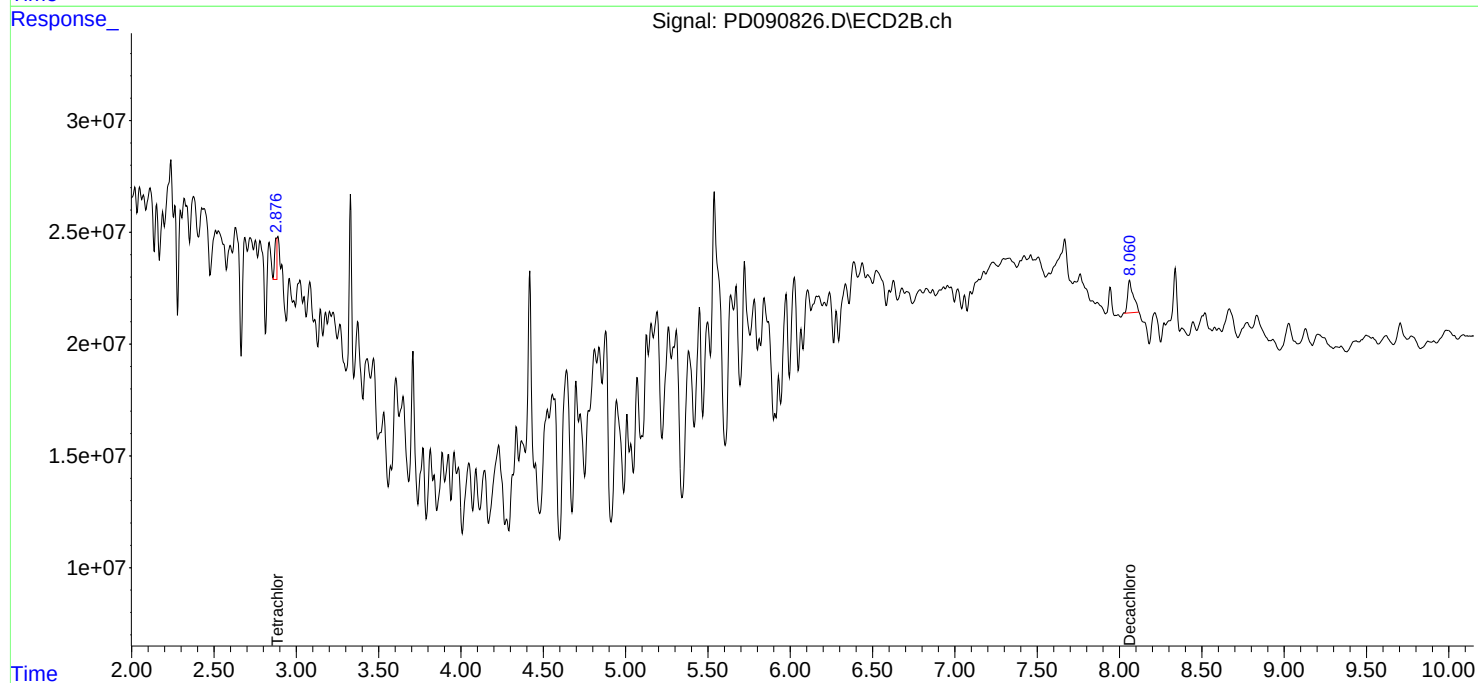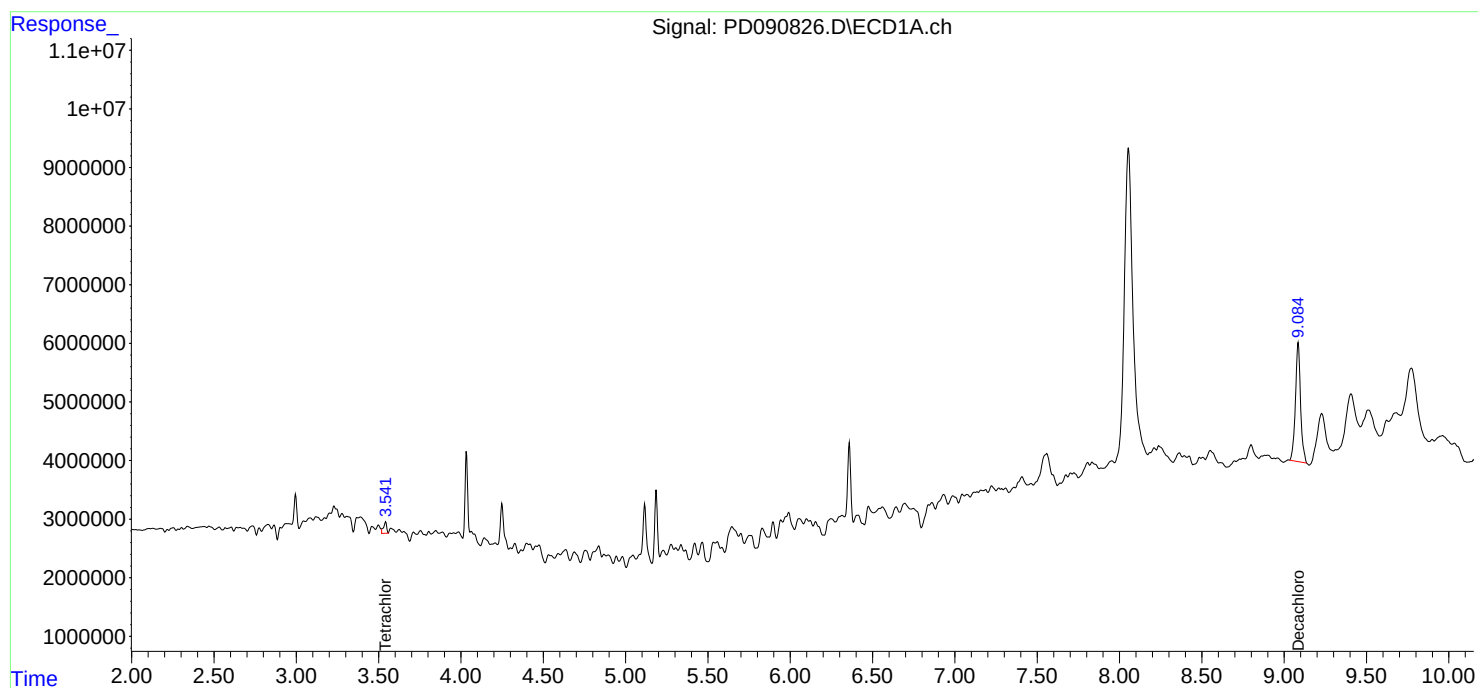

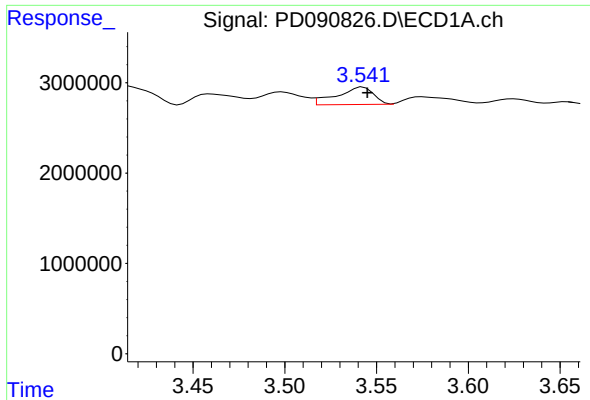


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 2706320
Conc: 0.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
P001-TW4-251023-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/27/2025
Supervised By :mohammad ahmed 10/28/2025

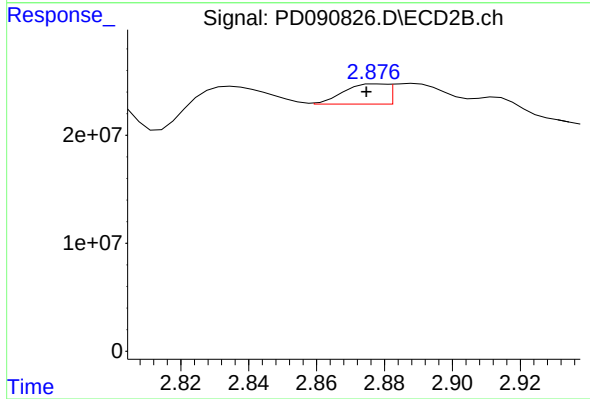


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.001 min
Response: 18053065
Conc: 0.61 ng/ml m

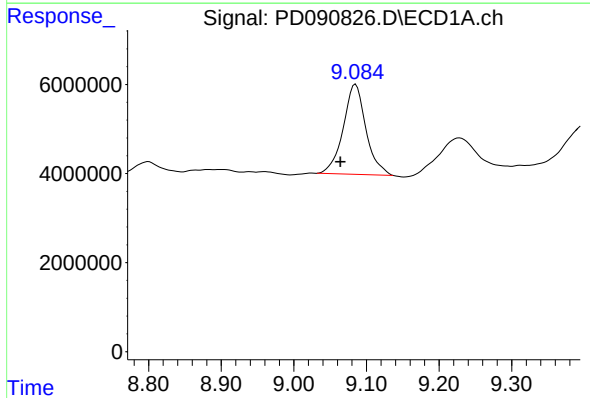

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.020 min
Response: 43974566
Conc: 9.40 ng/ml m

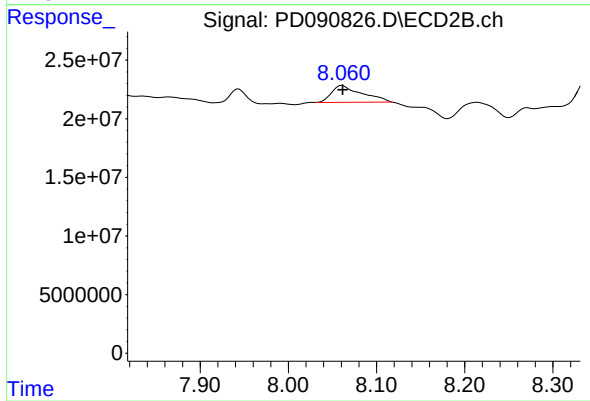

#28 Decachlorobiphenyl

R.T.: 8.060 min
Delta R.T.: -0.002 min
Response: 34651815
Conc: 1.14 ng/ml m