


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102725\
Data File : BG064582.D
Acq On : 27 Oct 2025 11:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 16:40:26 2025

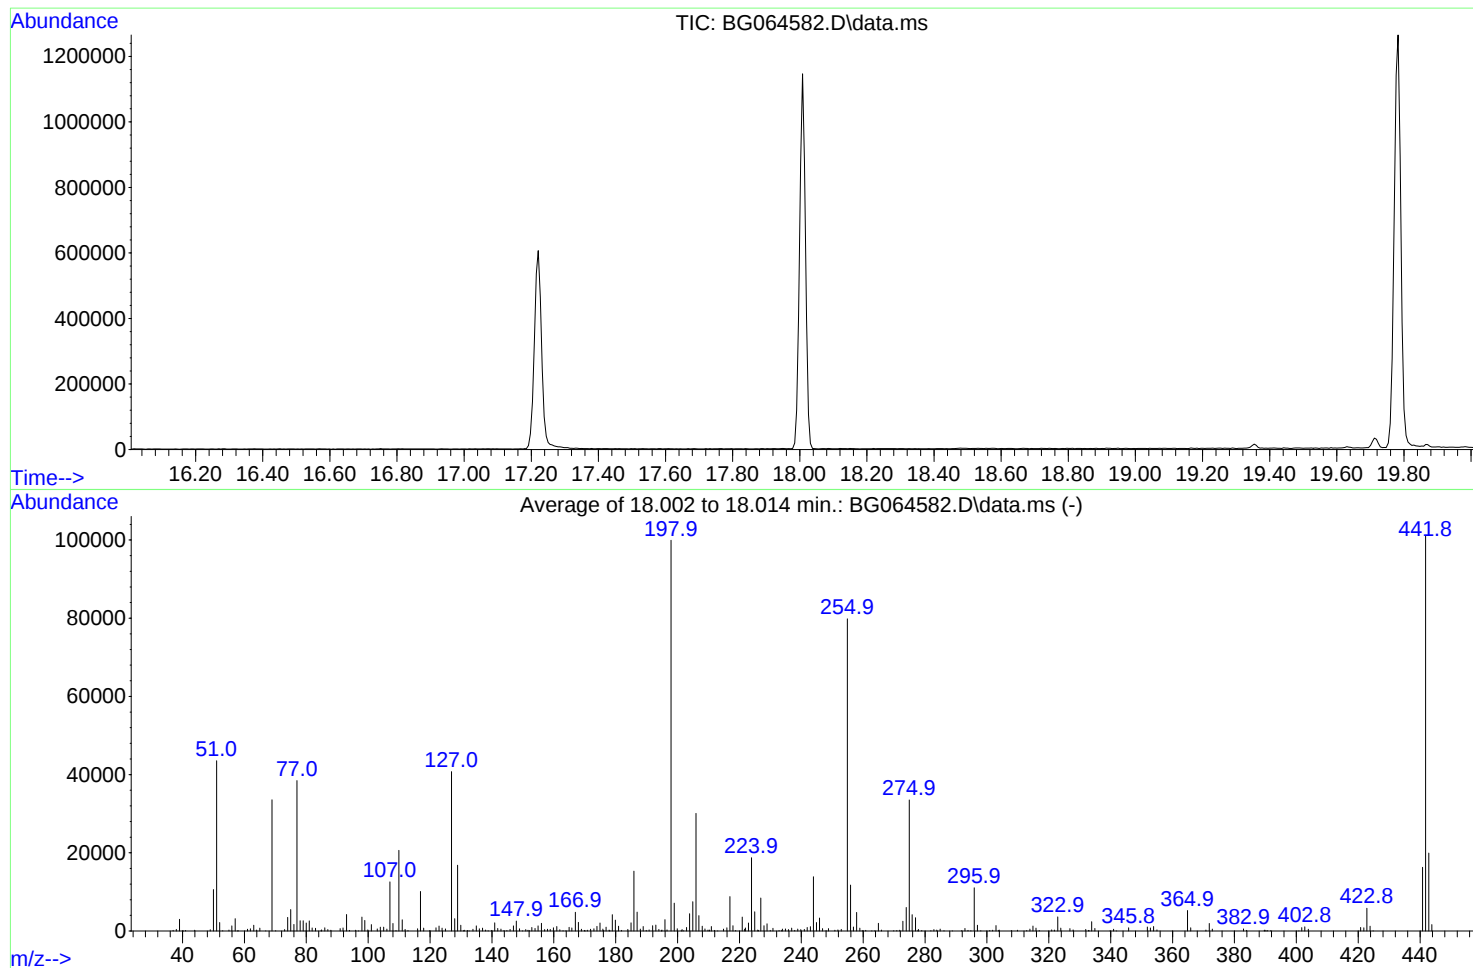

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	33541	PASS
70	69	0.00	2	0.2	69	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99925	PASS
199	198	5	9	7.1	7116	PASS
365	198	1	100	5.2	5240	PASS
441	443	0.01	150	81.8	16292	PASS
442	442	100	100	100.0	100981	PASS
443	442	15	24	19.7	19929	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/27/2025	BNA_G	<u>BG064582.D</u>
Compound Name	Response	Retention Time
DDT	310182	21.022
DDD	7570	20.576
DDE	57	19.706
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7627	317809	2.40

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102725\
Data File : BG064582.D
Acq On : 27 Oct 2025 11:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 27 11:58:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

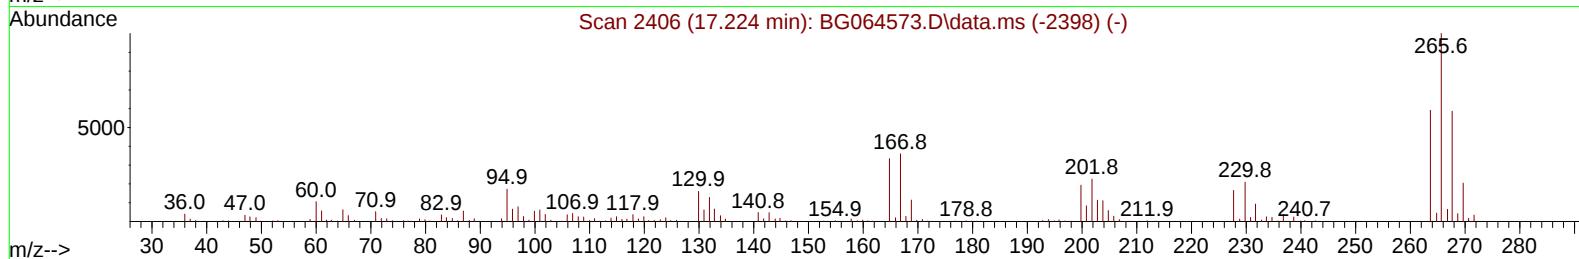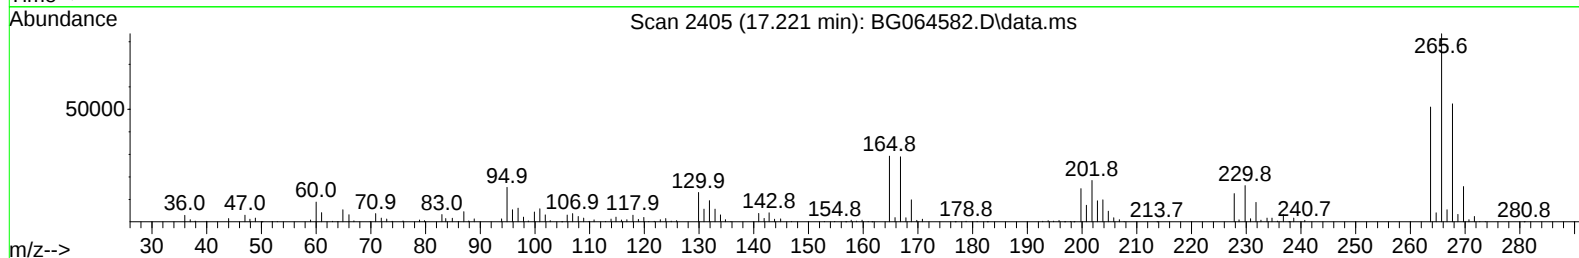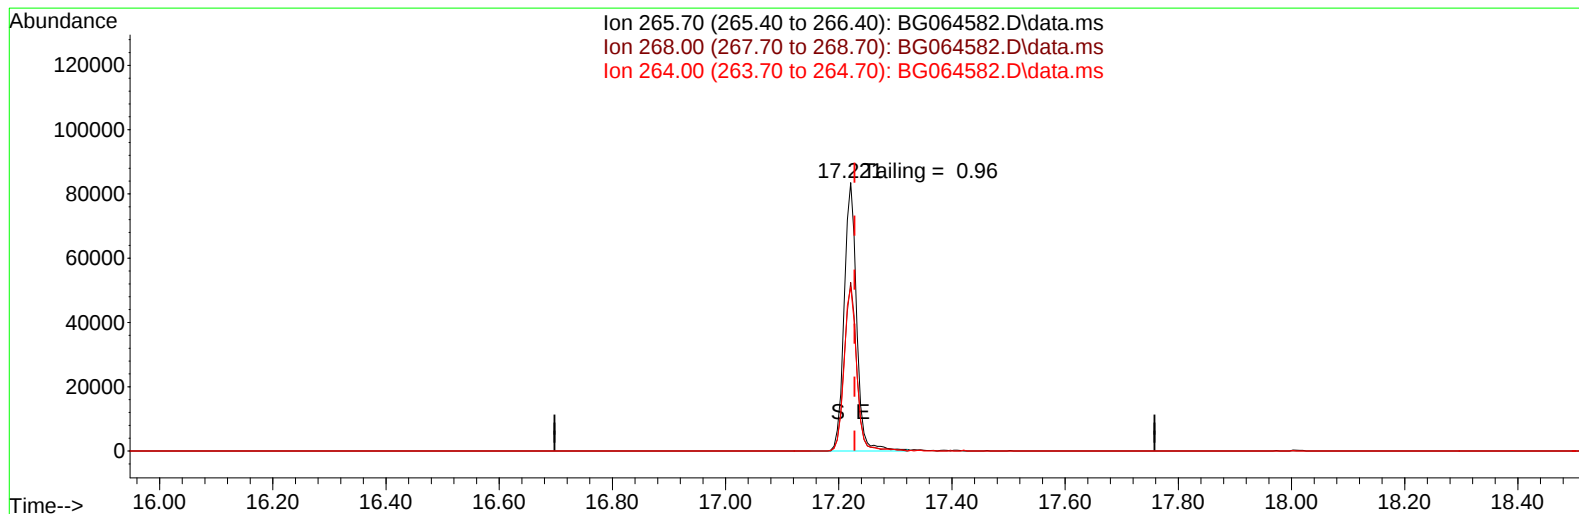

TIC: BG064582.D\data.ms

(70) Pentachlorophenol (C)

17.221min (-0.007) 22087.76 ng




response 128671

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	66.87
264.00	59.10	66.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102725\
Data File : BG064582.D
Acq On : 27 Oct 2025 11:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 27 11:58:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

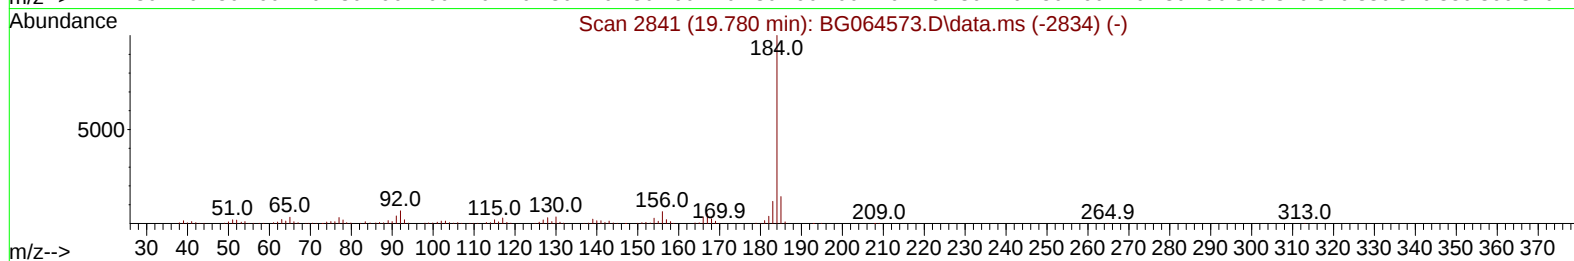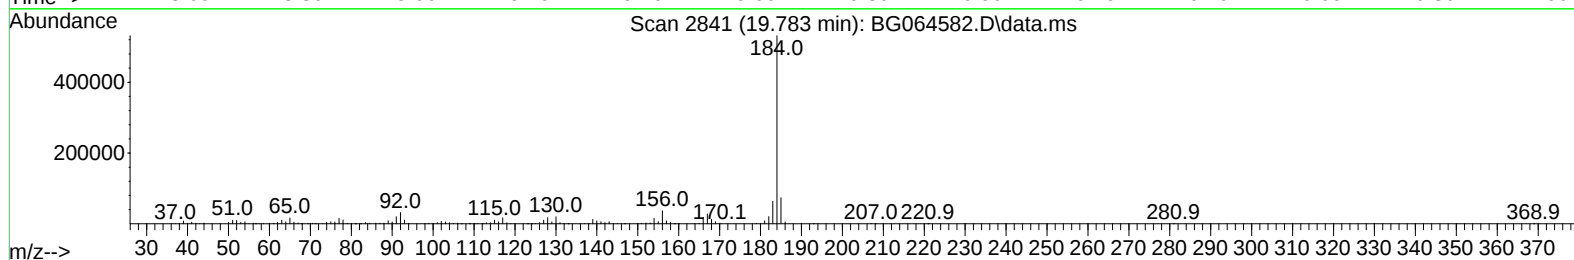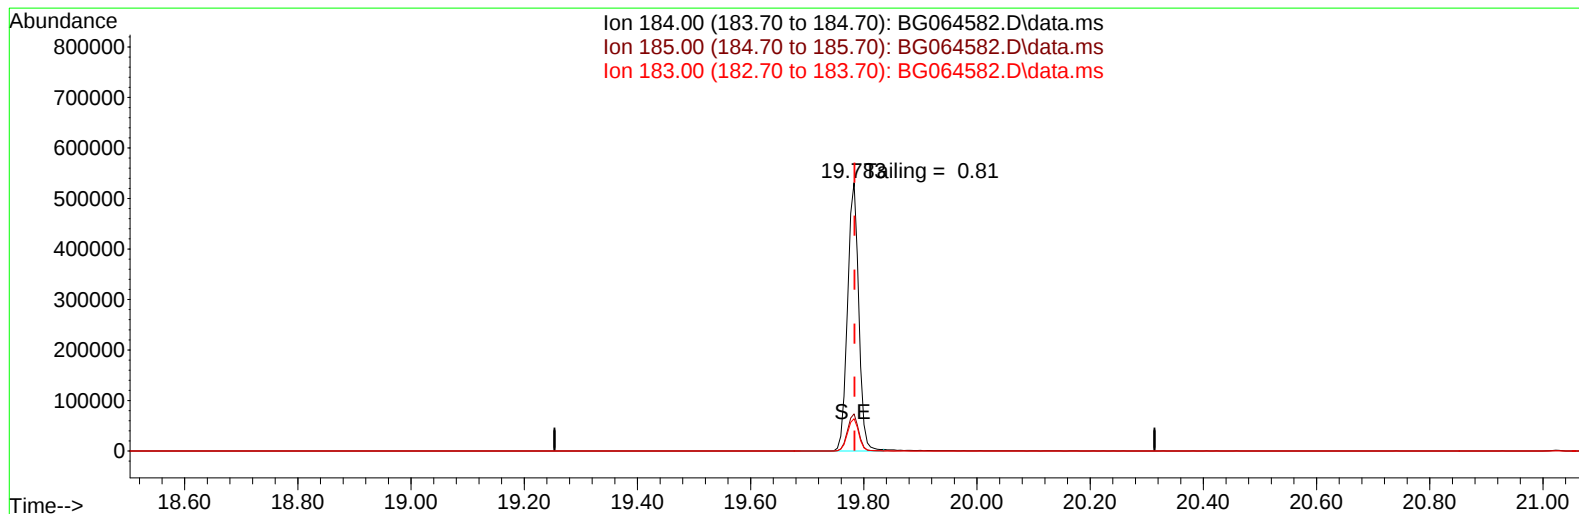

TIC: BG064582.D\data.ms

(77) Benzidine

19.783min (-0.001) 0.00 ng

response 736001

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.87
183.00	11.80	12.04
0.00	0.00	0.00