
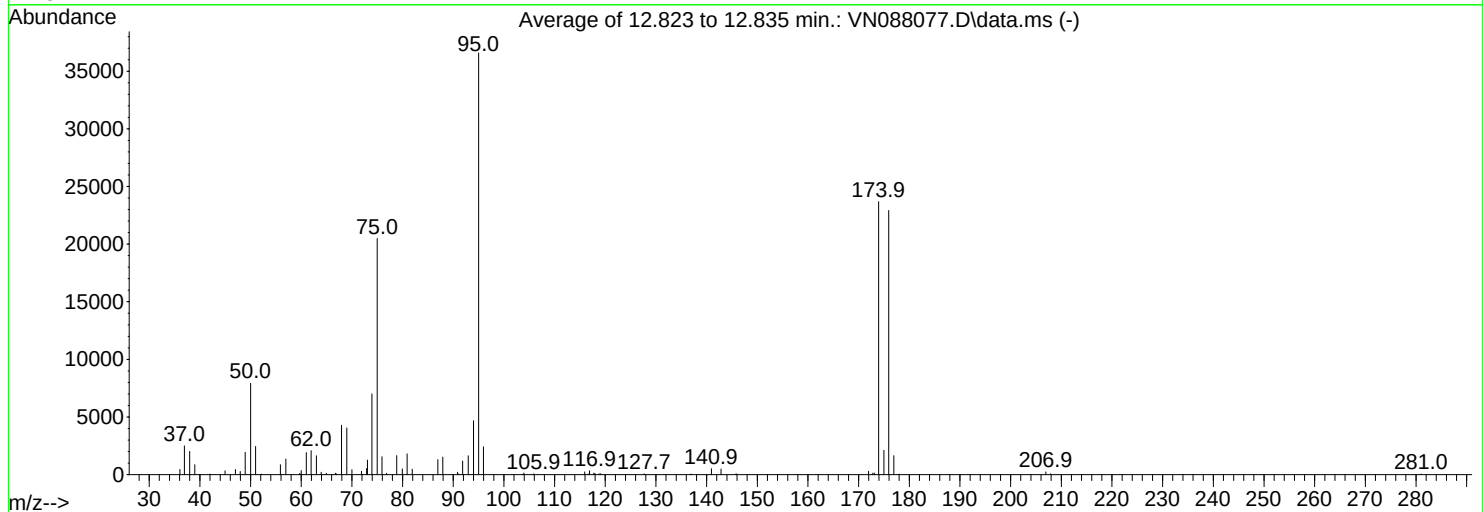


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102325\
Data File : VN088077.D
Acq On : 23 Oct 2025 09:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Title : SW846 8260
Last Update : Sat Oct 25 00:15:22 2025

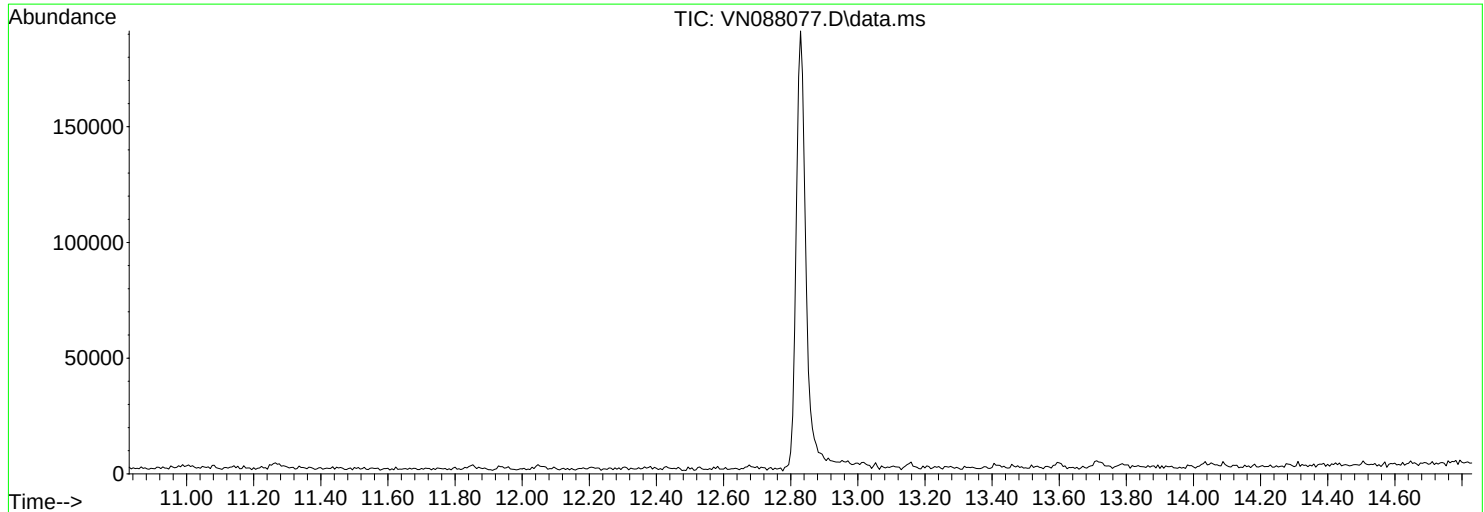

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	7924	PASS
75	95	30	60	56.0	20496	PASS
95	95	100	100	100.0	36595	PASS
96	95	5	9	6.6	2412	PASS
173	174	0.00	2	0.6	141	PASS
174	95	50	100	64.7	23688	PASS
175	174	5	9	8.9	2114	PASS
176	174	95	101	96.8	22925	PASS
177	176	5	9	7.2	1653	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	458	50.00	7924	64.95	132	75.95	155
36.95	2501	51.00	2446	66.75	129	76.85	12
38.00	2013	52.20	50	67.00	76	78.85	165
39.00	861	55.90	867	67.95	4293	79.95	50
39.85	28	56.95	1354	69.00	4051	80.90	1809
42.00	57	59.70	109	70.00	424	81.90	470
43.90	19	60.00	356	71.90	286	86.95	1303
44.95	328	61.00	1910	72.90	530	87.95	1532
47.00	441	61.95	2077	73.05	1259	90.85	210
47.95	276	63.00	1644	73.95	7010	91.10	62
48.95	1951	63.95	214	75.00	20496	91.85	1175

Average of 12.823 to 12.835 min.: VN088077.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	1644	117.95	115	173.95	23688		
94.00	4674	118.80	84	175.00	2114		
95.00	36595	119.10	82	175.95	22925		
95.95	2412	127.70	70	176.95	1653		
103.80	60	136.90	63	178.00	54		
103.95	139	140.95	512	206.95	238		
105.90	74	142.85	486	207.90	72		
115.95	231	145.80	89	281.00	50		
116.60	62	171.95	296				
116.90	332	172.80	135				
117.75	138	173.10	141				

Instrument :

MSVOA_N

ClientSampleId :

BFB