
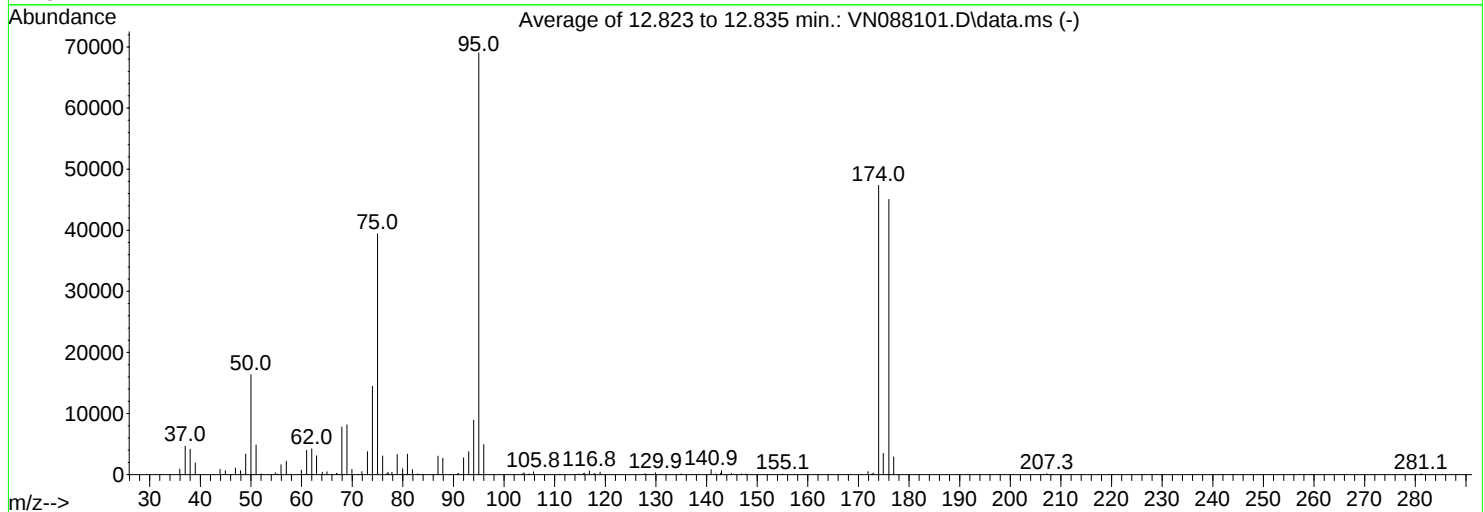


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102725\
Data File : VN088101.D
Acq On : 27 Oct 2025 09:58
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Title : SW846 8260
Last Update : Sat Oct 25 00:15:22 2025

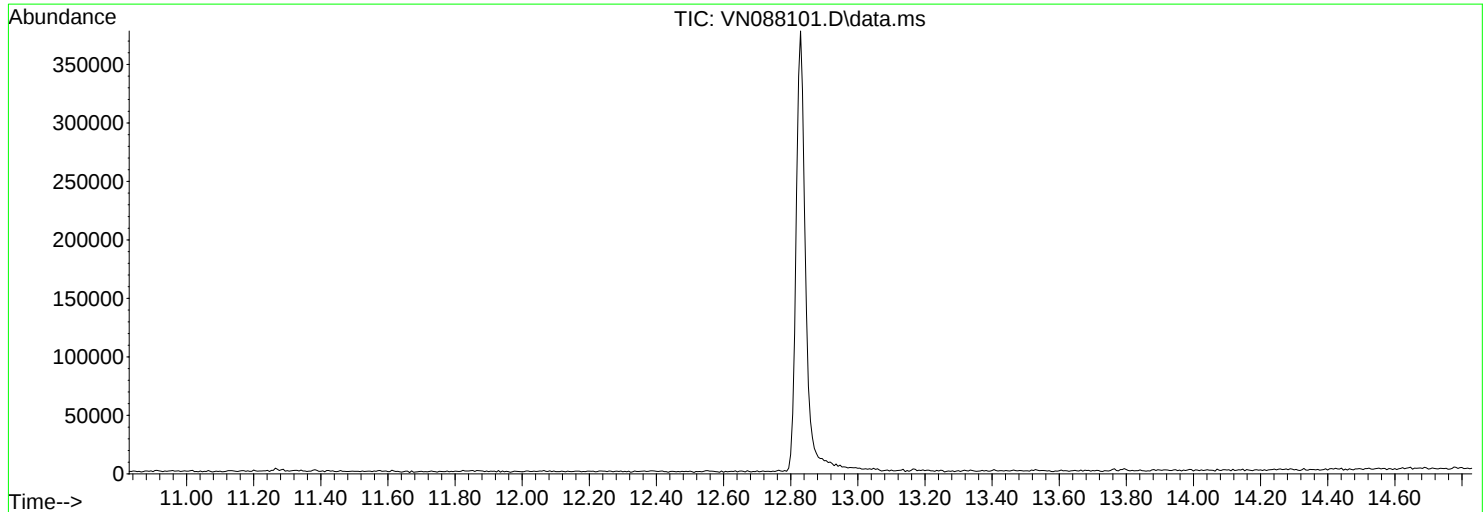

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	16367	PASS
75	95	30	60	57.1	39427	PASS
95	95	100	100	100.0	69032	PASS
96	95	5	9	7.1	4924	PASS
173	174	0.00	2	0.6	268	PASS
174	95	50	100	68.6	47325	PASS
175	174	5	9	7.4	3492	PASS
176	174	95	101	95.2	45051	PASS
177	176	5	9	6.5	2918	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	920	52.05	141	65.00	485	76.00	306
37.00	4661	54.80	326	66.90	226	76.90	241
38.00	4179	55.20	100	67.10	97	77.10	38
39.00	1917	55.95	1627	67.95	7794	77.85	38
43.90	874	57.00	2206	68.95	8159	78.90	3298
44.95	660	57.90	82	69.95	863	79.95	966
46.95	1114	59.95	741	71.20	53	80.90	3365
47.95	651	61.00	3995	71.90	497	81.90	822
48.95	3377	62.00	4259	73.00	3760	82.95	135
50.00	16367	62.95	3086	74.00	14470	86.95	3033
51.00	4844	64.10	386	75.00	39427	87.90	2708

Average of 12.823 to 12.835 min.: VN088101.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.80	147	111.00	85	137.20	54	172.70	145
91.00	195	114.80	105	140.90	846	172.90	268
92.00	2747	115.70	182	141.85	129	174.00	47325
93.00	3738	115.85	226	142.80	247	174.90	3492
94.00	8930	116.85	597	142.95	658	176.00	45051
95.00	69032	117.80	210	144.90	215	176.95	2918
96.00	4924	118.00	94	146.90	114	206.60	62
103.70	148	118.95	425	147.80	111	207.25	155
103.95	329	127.85	189	154.70	54	208.20	54
104.95	146	129.90	309	155.10	89	281.15	157
105.80	470	134.95	139	171.90	488		