


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103025\
Data File : BP026038.D
Acq On : 30 Oct 2025 10:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 30 11:51:34 2025

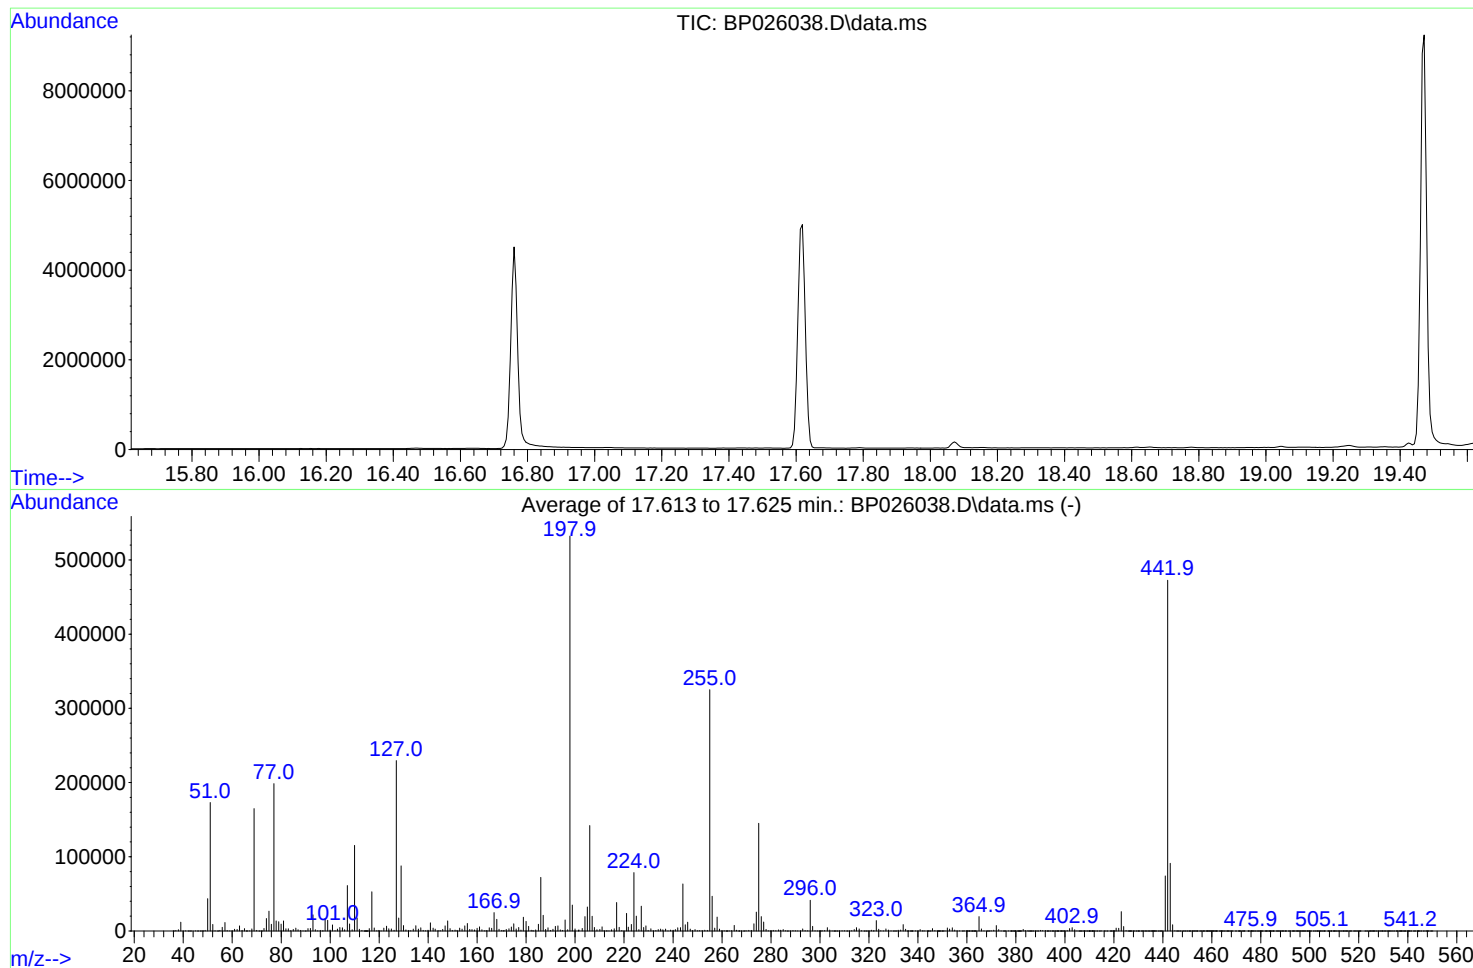

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2486

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2745	PASS
69	69	100	100	100.0	164910	PASS
70	69	0.00	2	0.6	912	PASS
197	198	0.00	2	0.3	1808	PASS
198	198	100	100	100.0	532011	PASS
199	198	5	9	6.6	34927	PASS
365	198	1	100	3.7	19451	PASS
441	443	0.01	150	81.2	74093	PASS
442	442	100	100	100.0	472508	PASS
443	442	15	24	19.3	91243	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/30/2025	BNA_P	<u>BP026038.D</u>
Compound Name	Response	Retention Time
DDT	1702124	20.777
DDD	17819	20.307
DDE	2173	19.866
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19992	1722116	1.16

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103025\
Data File : BP026038.D
Acq On : 30 Oct 2025 10:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 30 12:40:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

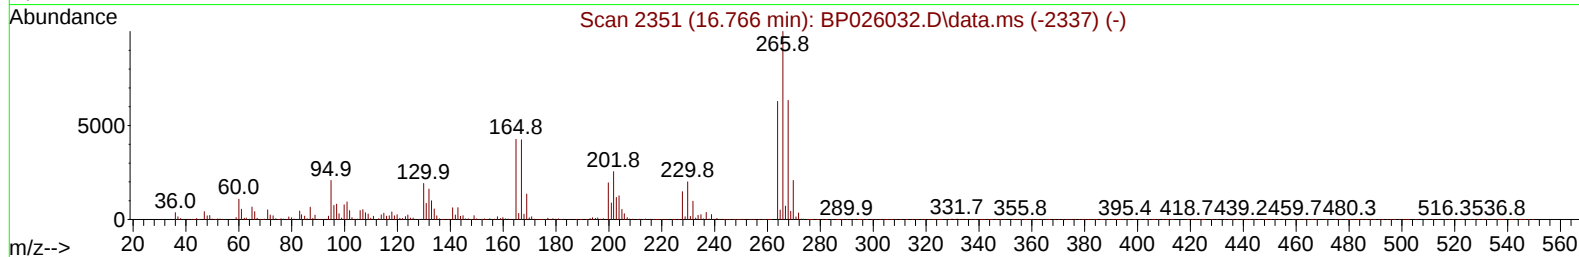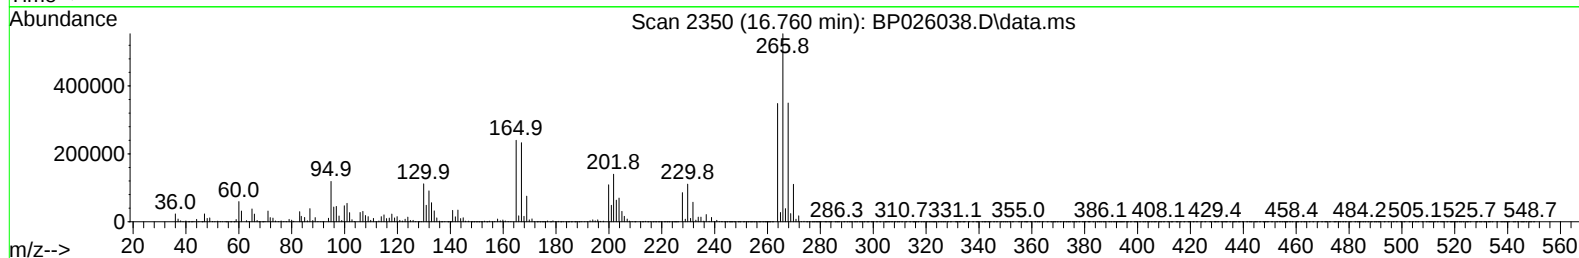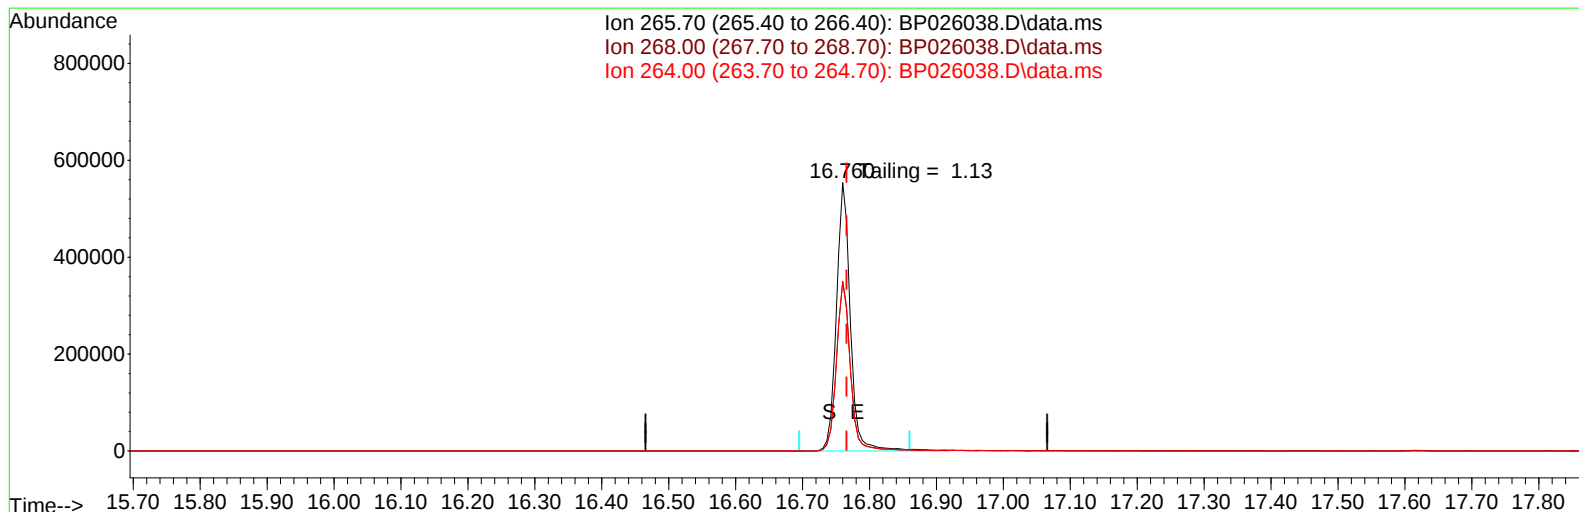

TIC: BP026038.D\data.ms

(70) Pentachlorophenol (C)

16.760min (-0.006) 1770436.21 ng m




response 805688

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.18
264.00	62.80	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103025\
Data File : BP026038.D
Acq On : 30 Oct 2025 10:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 30 12:40:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

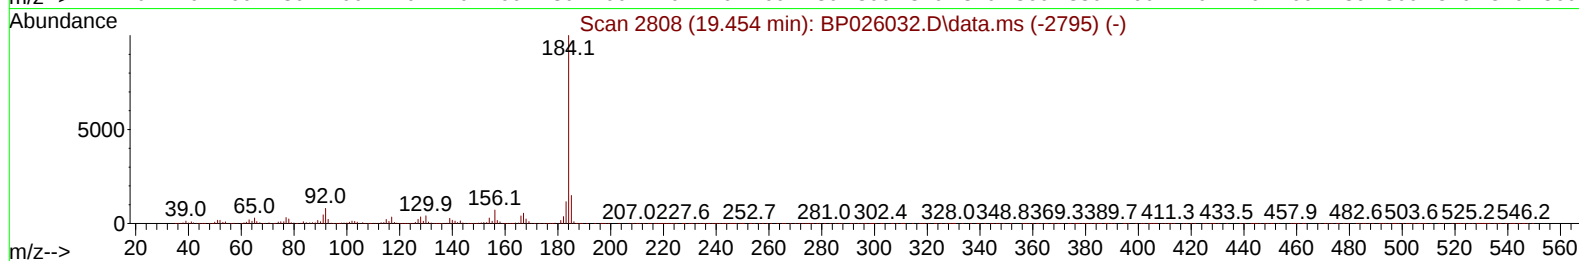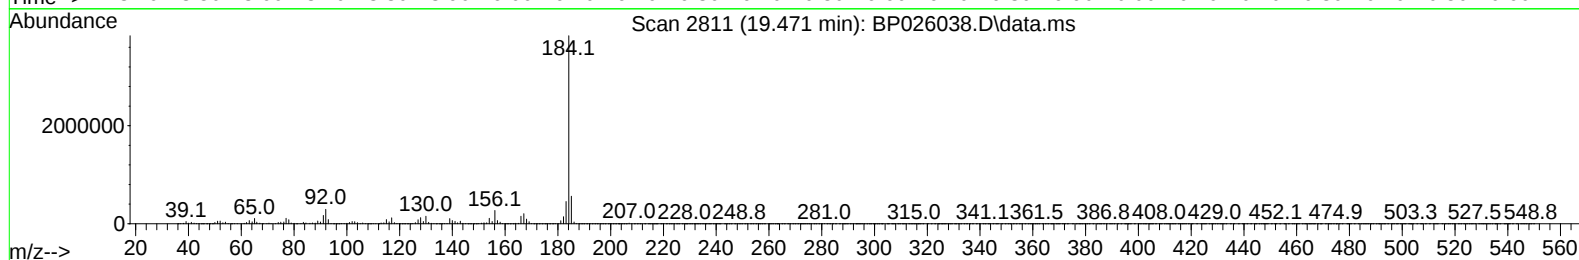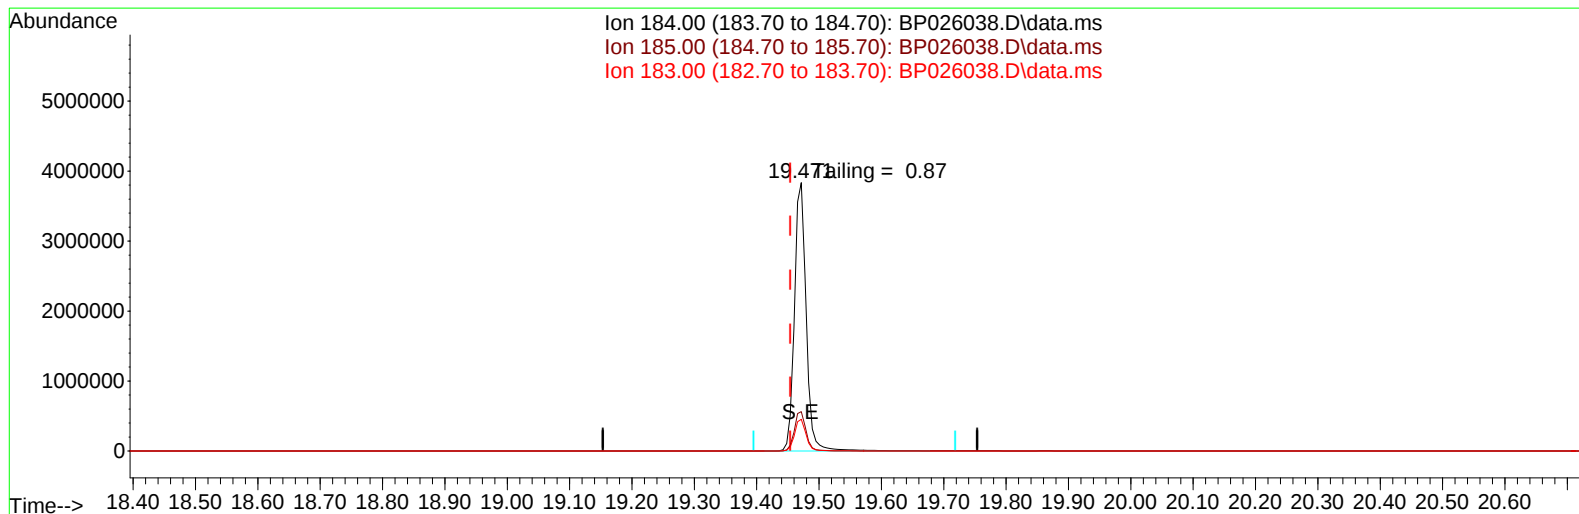

TIC: BP026038.D\data.ms

(77) Benzidine

19.471min (+ 0.018) 5475.51 ng

response 5032842

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.67
183.00	11.50	11.80
0.00	0.00	0.00