

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102725\
 Data File : VY023592.D
 Acq On : 27 Oct 2025 12:30
 Operator : SY/MD
 Sample : Q3466-04
 Misc : 4.79g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 B9-0.5-1.0-20251023

Quant Time: Oct 28 04:39:03 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	745194	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	1231218	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	979970	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	361763	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	314555	50.479	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	100.960%
35) Dibromofluoromethane	7.634	113	380851	50.342	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.680%
50) Toluene-d8	10.109	98	1364092	48.417	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.840%
62) 4-Bromofluorobenzene	12.408	95	359173	38.614	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	77.220%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102725\
Data File : VY023592.D
Acq On : 27 Oct 2025 12:30
Operator : SY/MD
Sample : Q3466-04
Misc : 4.79g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
B9-0.5-1.0-20251023

Quant Time: Oct 28 04:39:03 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration




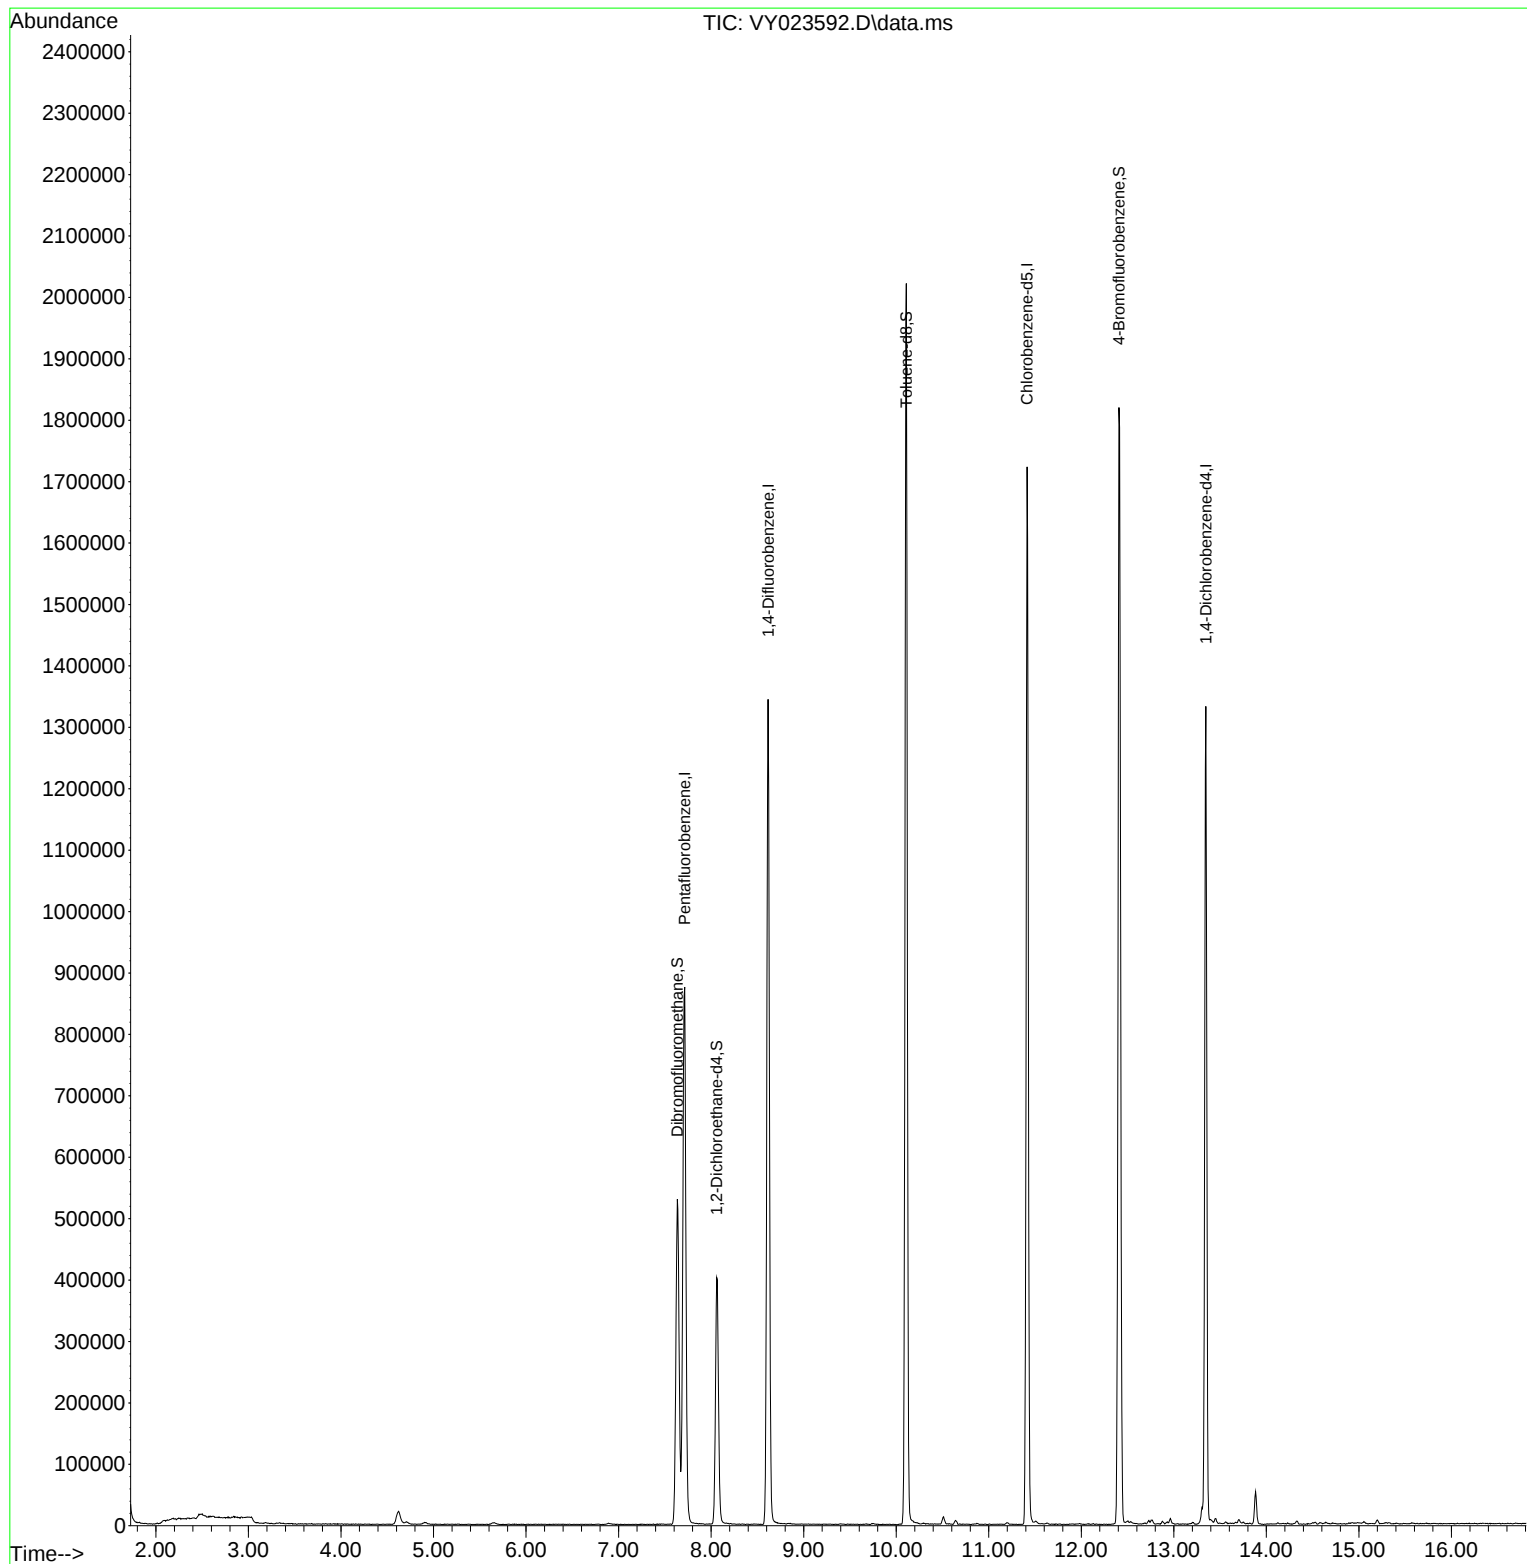




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 99
Delta R.T. 0.006 min
Lab File: VY023592.D
Acq: 27 Oct 2025 12:30




Instrument :
MSVOA_Y
ClientSampleId :
B9-0.5-1.0-20251023


Tgt Ion:168 Resp: 745194
Ion Ratio Lower Upper
168 100
99 47.6 39.7 59.5

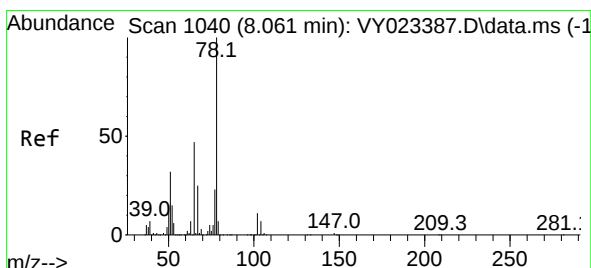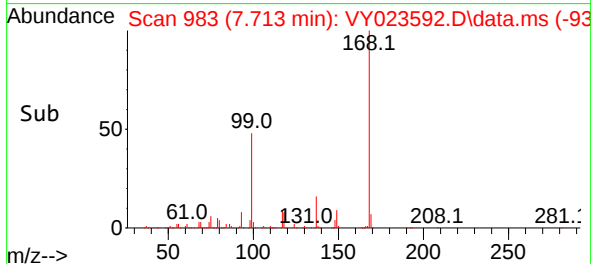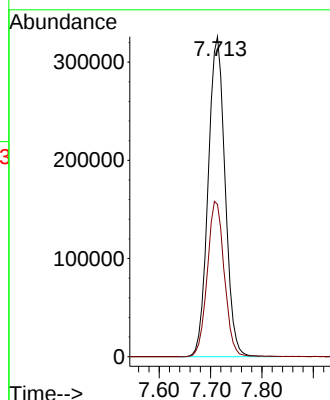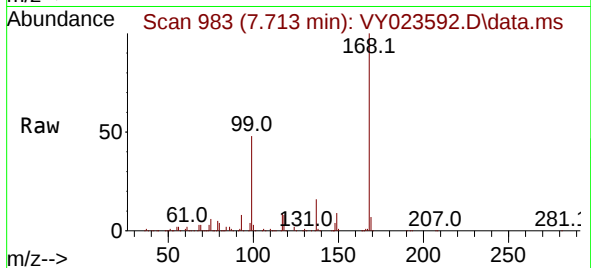

#33
1,2-Dichloroethane-d4
Concen: 50.479 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY023592.D
Acq: 27 Oct 2025 12:30

Tgt Ion: 65 Resp: 314555
Ion Ratio Lower Upper
65 100
67 53.8 0.0 105.8

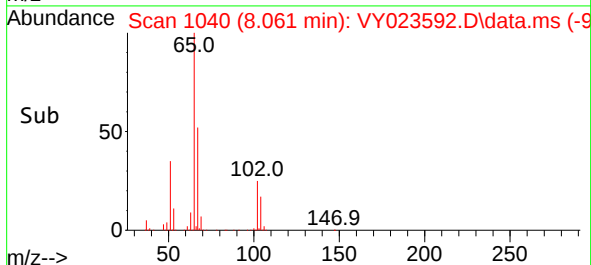
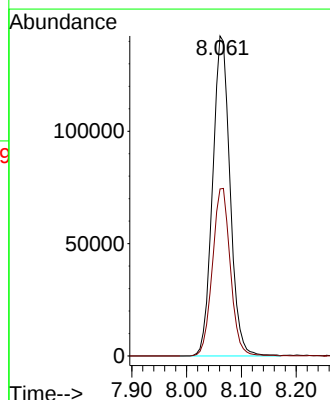
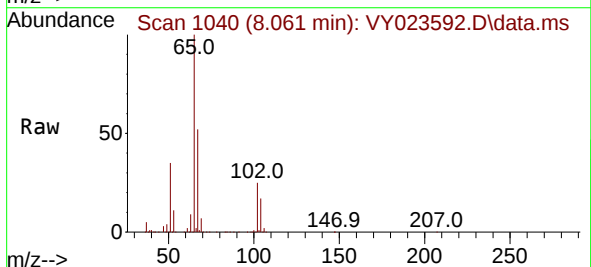


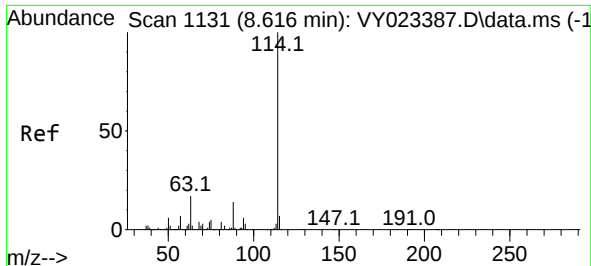

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY023592.D
Acq: 27 Oct 2025 12:30




Instrument :
MSVOA_Y
ClientSampleId :
B9-0.5-1.0-20251023


Tgt Ion:114 Resp: 1231218
Ion Ratio Lower Upper
114 100
63 17.0 0.0 34.2
88 14.3 0.0 28.4

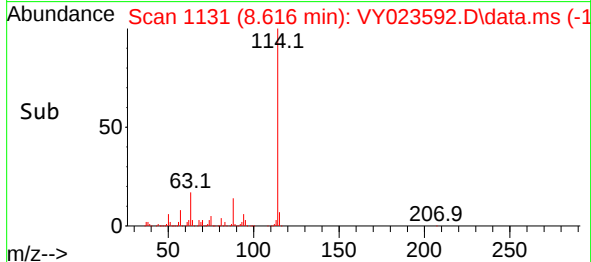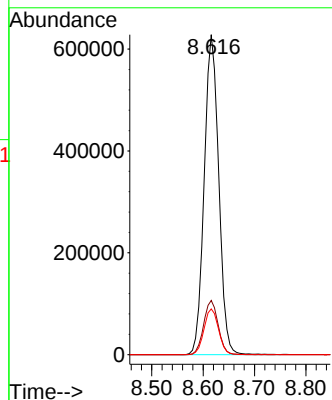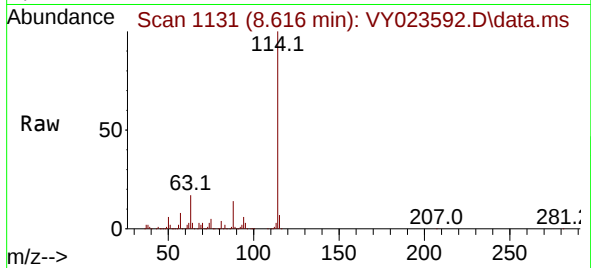

#35
Dibromofluoromethane
Concen: 50.342 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY023592.D
Acq: 27 Oct 2025 12:30

Tgt Ion:113 Resp: 380851
Ion Ratio Lower Upper
113 100
111 101.5 81.8 122.6
192 22.5 18.0 27.0


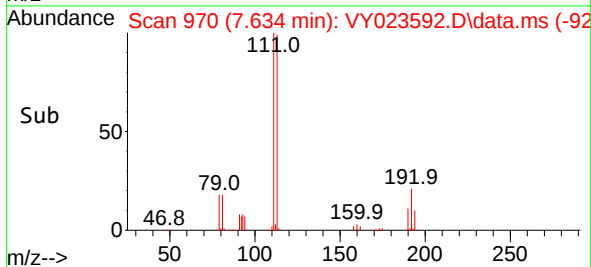
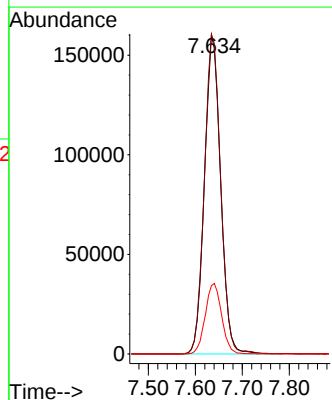
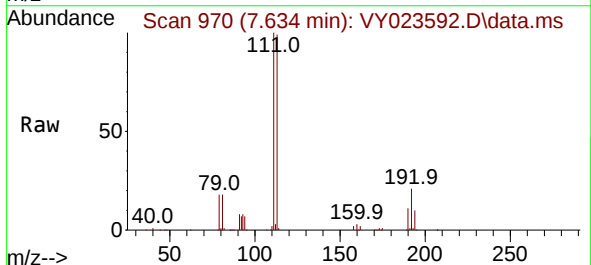


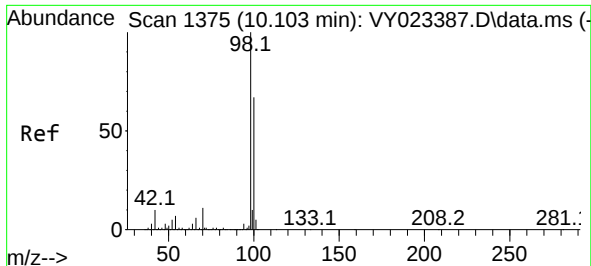

#50
Toluene-d8
Concen: 48.417 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023592.D
Acq: 27 Oct 2025 12:30




Instrument :
MSVOA_Y
ClientSampleId :
B9-0.5-1.0-20251023

Tgt Ion: 98 Resp: 1364092
Ion Ratio Lower Upper
98 100
100 65.3 53.0 79.4

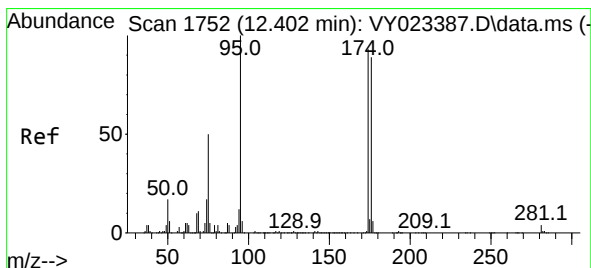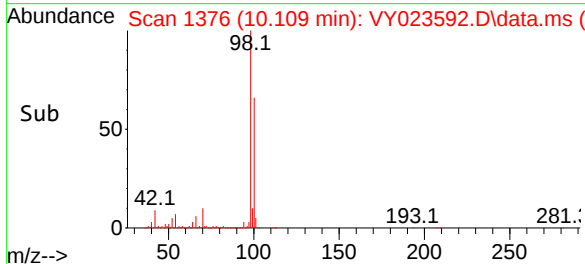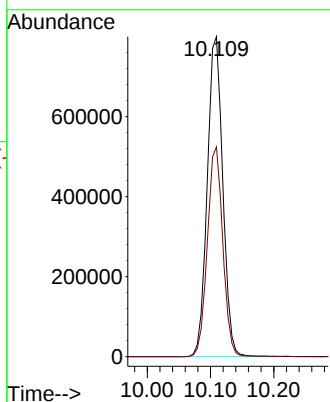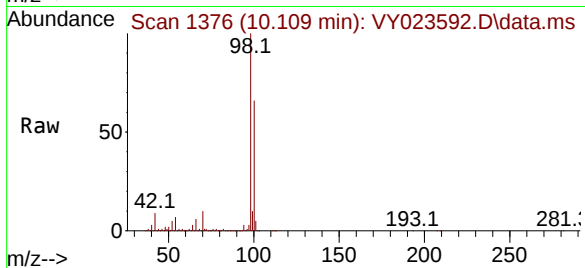

#62
4-Bromofluorobenzene
Concen: 38.614 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY023592.D
Acq: 27 Oct 2025 12:30

Tgt Ion: 95 Resp: 359173
Ion Ratio Lower Upper
95 100
174 96.5 0.0 192.8
176 94.2 0.0 187.6

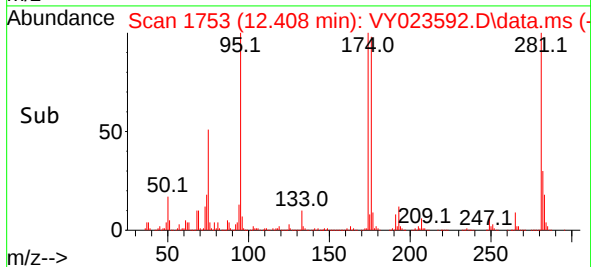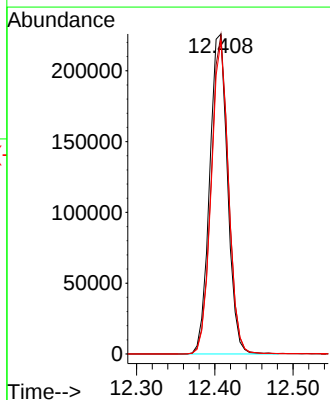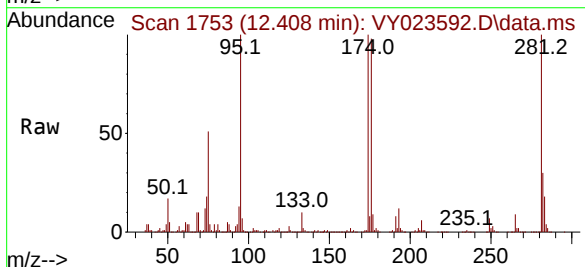



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY023592.D

Acq: 27 Oct 2025 12:30

Instrument :

MSVOA_Y

ClientSampleId :

B9-0.5-1.0-20251023





Tgt Ion:117 Resp: 979970

Ion Ratio Lower Upper

117 100

82 51.7 41.0 61.4

119 32.7 25.6 38.4

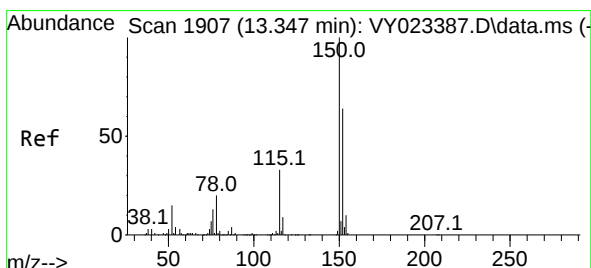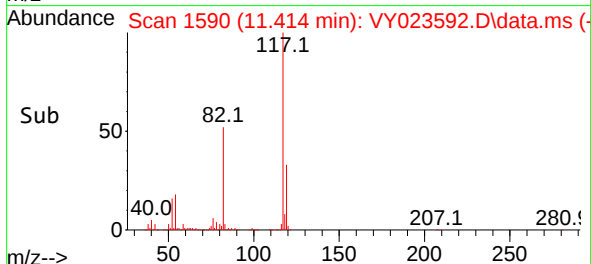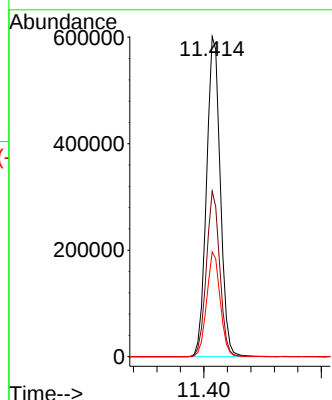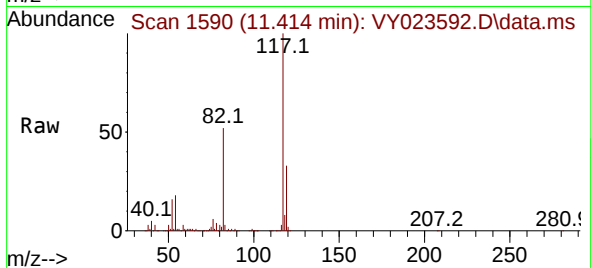

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY023592.D

Acq: 27 Oct 2025 12:30

Tgt Ion:152 Resp: 361763

Ion Ratio Lower Upper

152 100

115 54.6 27.1 81.2

150 156.6 0.0 347.4

