


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102925\  
Data File : BG064617.D  
Acq On : 29 Oct 2025 10:41  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102425.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Oct 24 16:40:26 2025

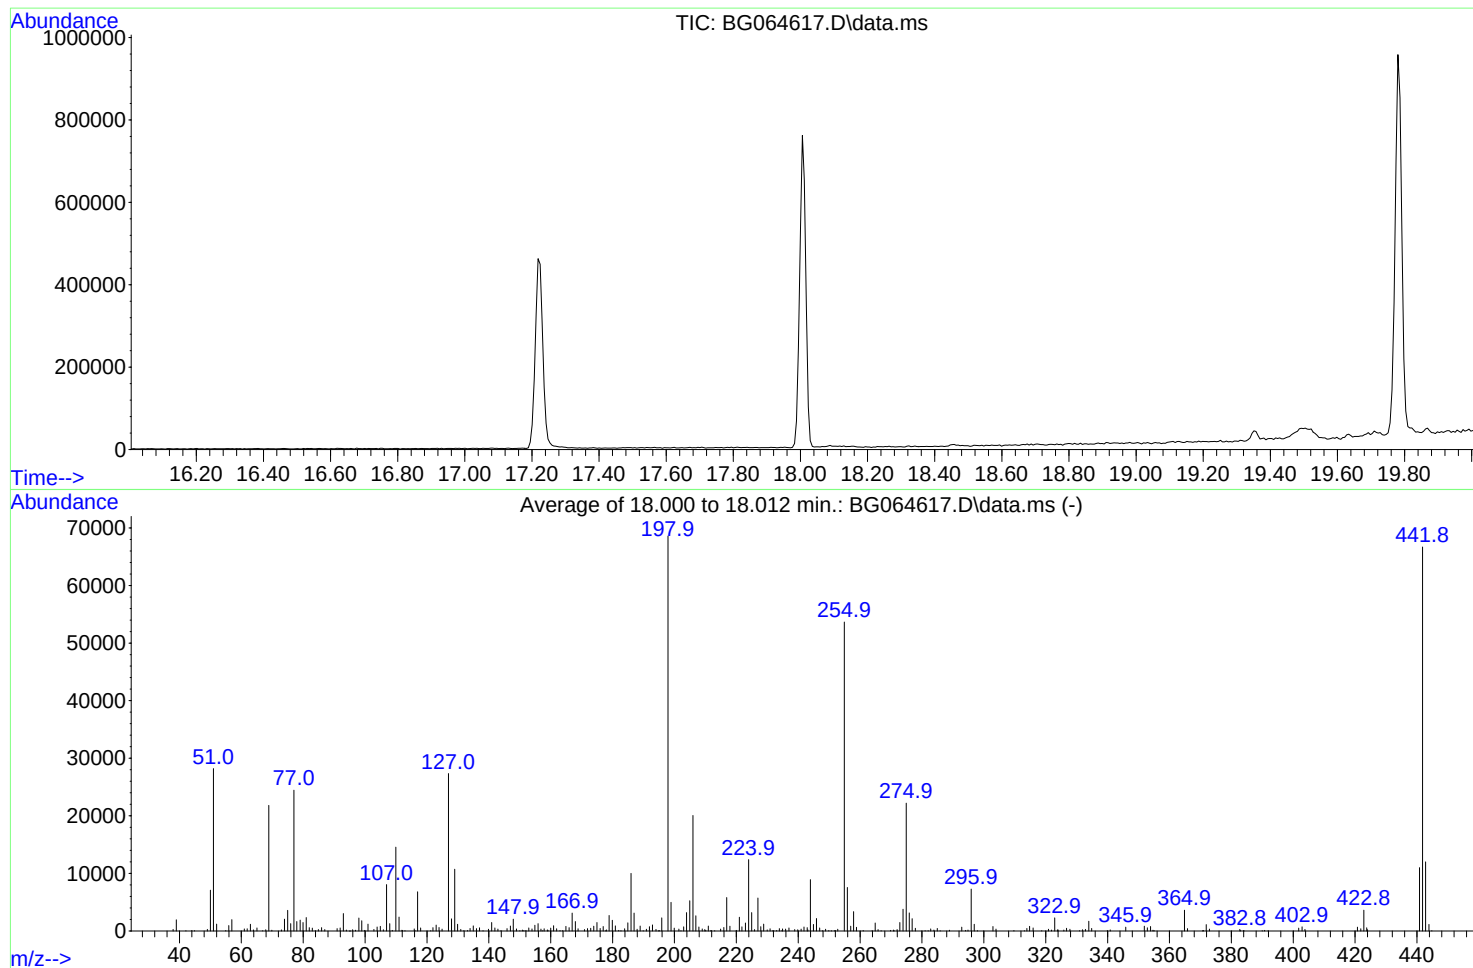

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2532

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 68          | 69           | 0.00         | 2            | 1.0       | 229     | PASS             |
| 69          | 69           | 100          | 100          | 100.0     | 21821   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 135     | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 68565   | PASS             |
| 199         | 198          | 5            | 9            | 7.3       | 4984    | PASS             |
| 365         | 198          | 1            | 100          | 5.3       | 3612    | PASS             |
| 441         | 443          | 0.01         | 150          | 91.7      | 11008   | PASS             |
| 442         | 442          | 100          | 100          | 100.0     | 66685   | PASS             |
| 443         | 442          | 15           | 24           | 18.0      | 12010   | PASS             |

# DDT Breakdown


| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/29/2025    | BNA_G            | <u>BG064617.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 244663           | 21.026             |
| DDD           | 3569             | 20.573             |
| DDE           | 0                | 19.706             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3569          | 248232           | 1.44               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102925\  
Data File : BG064617.D  
Acq On : 29 Oct 2025 10:41  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Oct 29 11:21:32 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 24 16:40:26 2025  
Response via : Initial Calibration

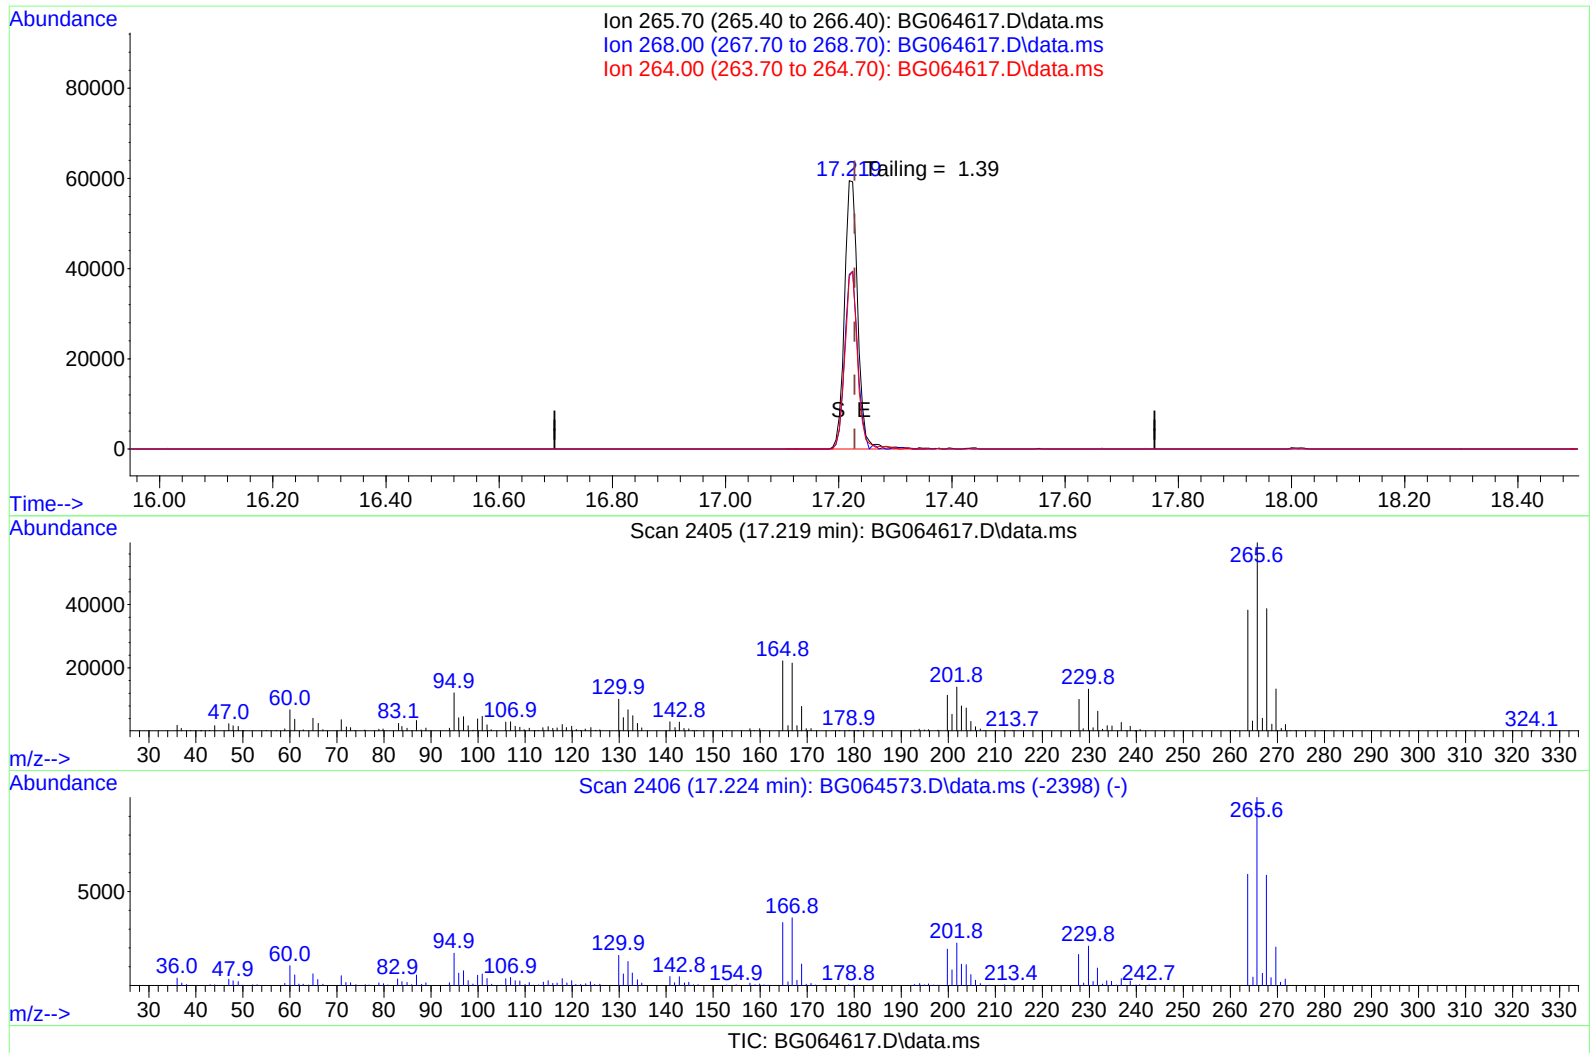

**(70) Pentachlorophenol (C)**

17.219min (-0.009) 35052.04 ng




response 97221

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.90  | 65.04  |
| 264.00 | 59.10  | 69.72  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102925\  
Data File : BG064617.D  
Acq On : 29 Oct 2025 10:41  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Oct 29 11:21:32 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 24 16:40:26 2025  
Response via : Initial Calibration

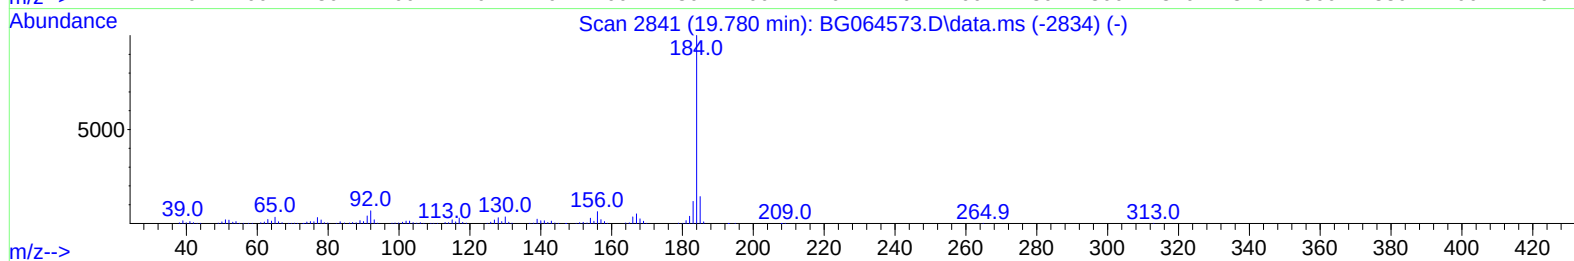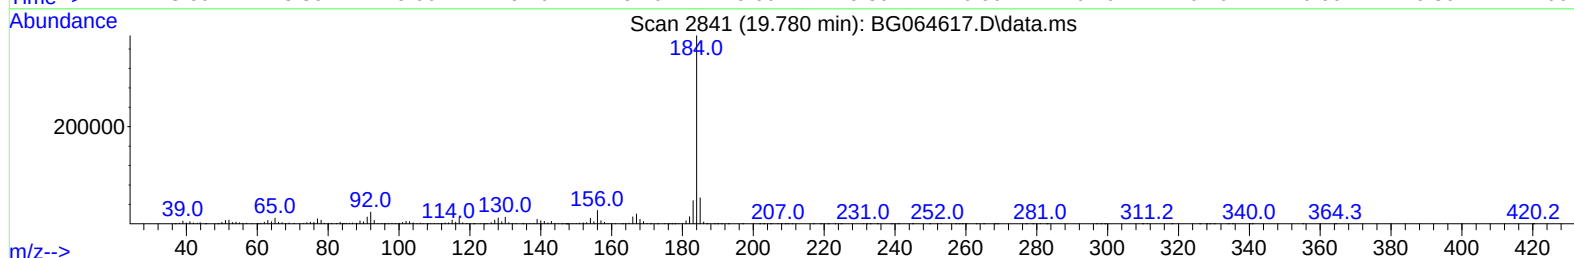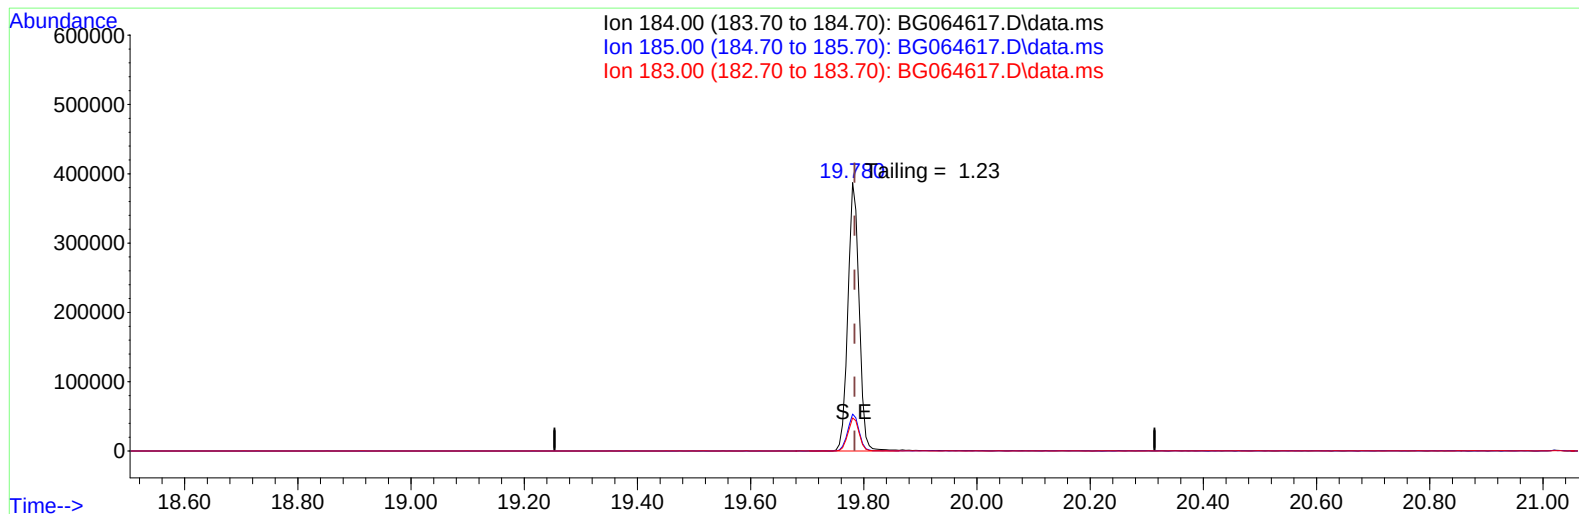

TIC: BG064617.D\data.ms

(77) Benzidine

19.780min (-0.003) 345166.57 ng

response 533588

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.30  | 13.80  |
| 183.00 | 11.80  | 12.33  |
| 0.00   | 0.00   | 0.00   |