
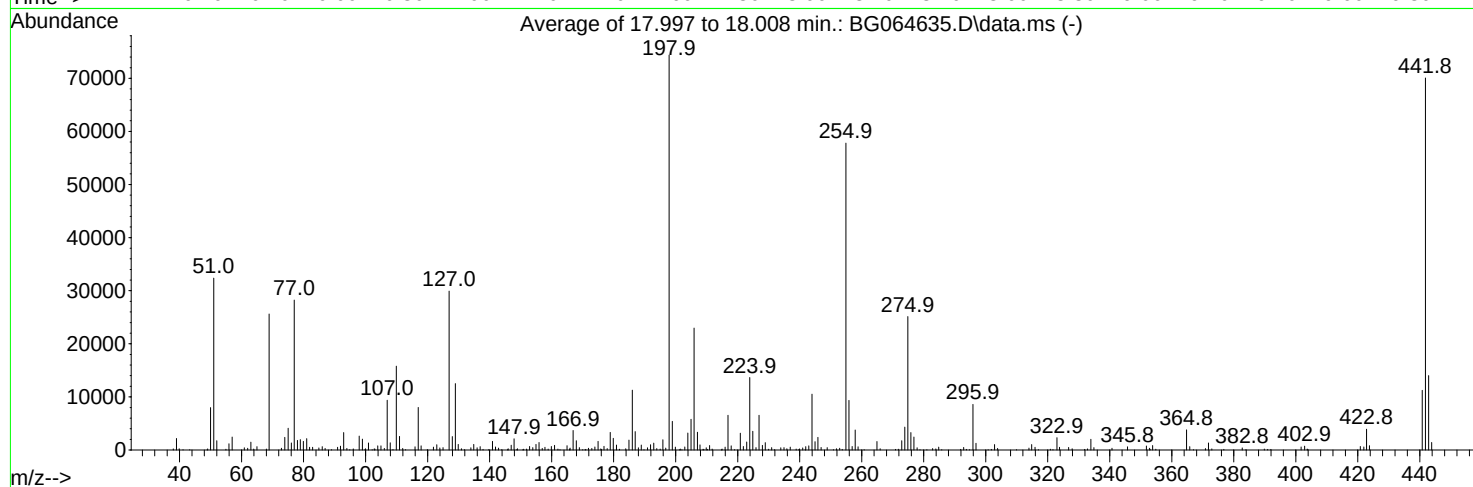


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103025\
Data File : BG064635.D
Acq On : 30 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 16:40:26 2025

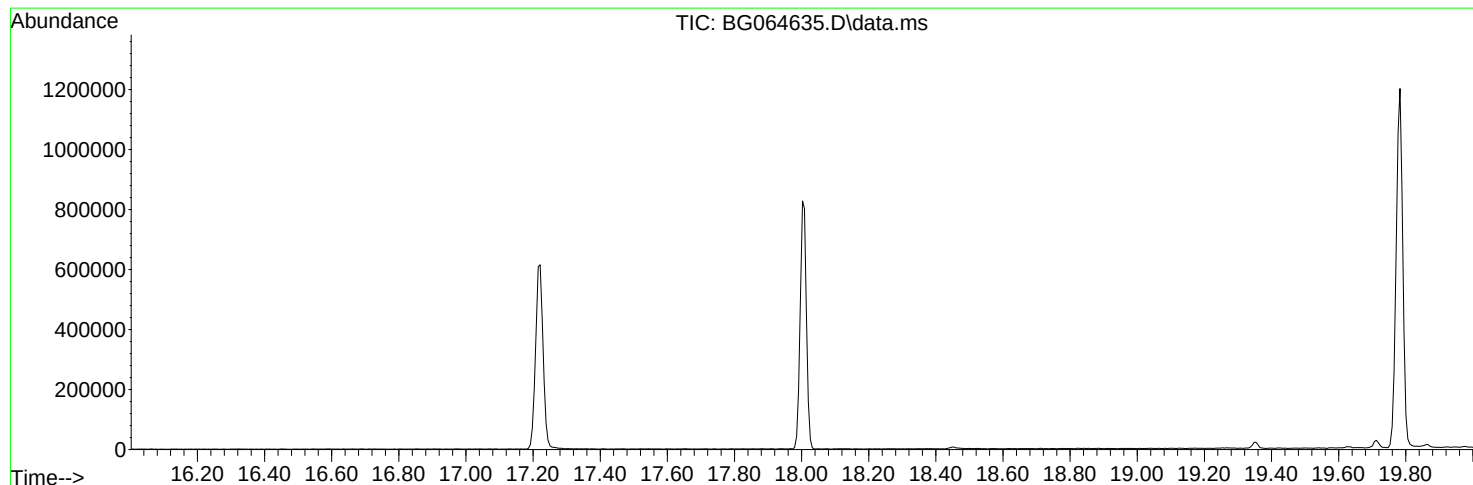




AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2531

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.7	175	PASS
69	69	100	100	100.0	25608	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.5	368	PASS
198	198	100	100	100.0	74355	PASS
199	198	5	9	7.3	5401	PASS
365	198	1	100	5.1	3813	PASS
441	443	0.01	150	80.3	11250	PASS
442	442	100	100	100.0	70075	PASS
443	442	15	24	20.0	14011	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103025\
Data File : BG064635.D
Acq On : 30 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 30 11:34:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

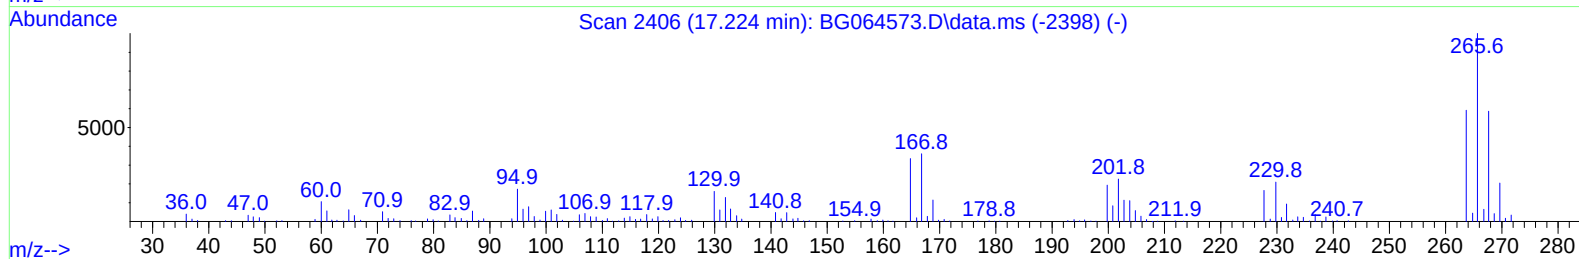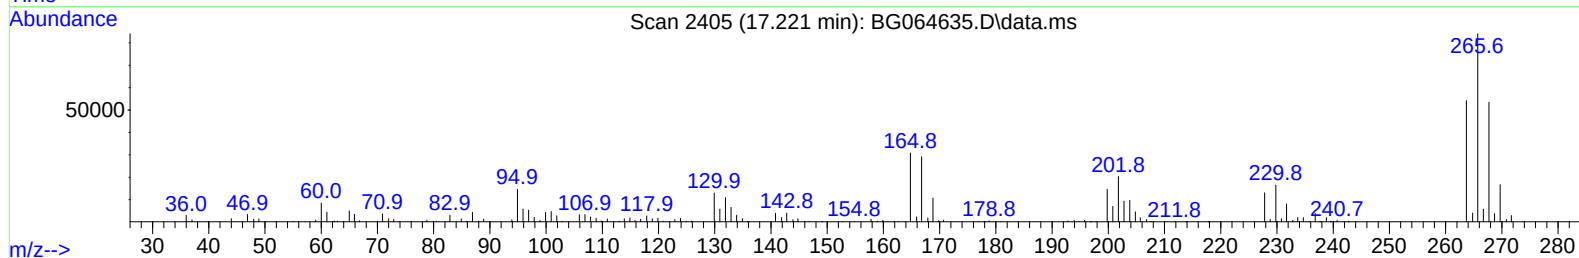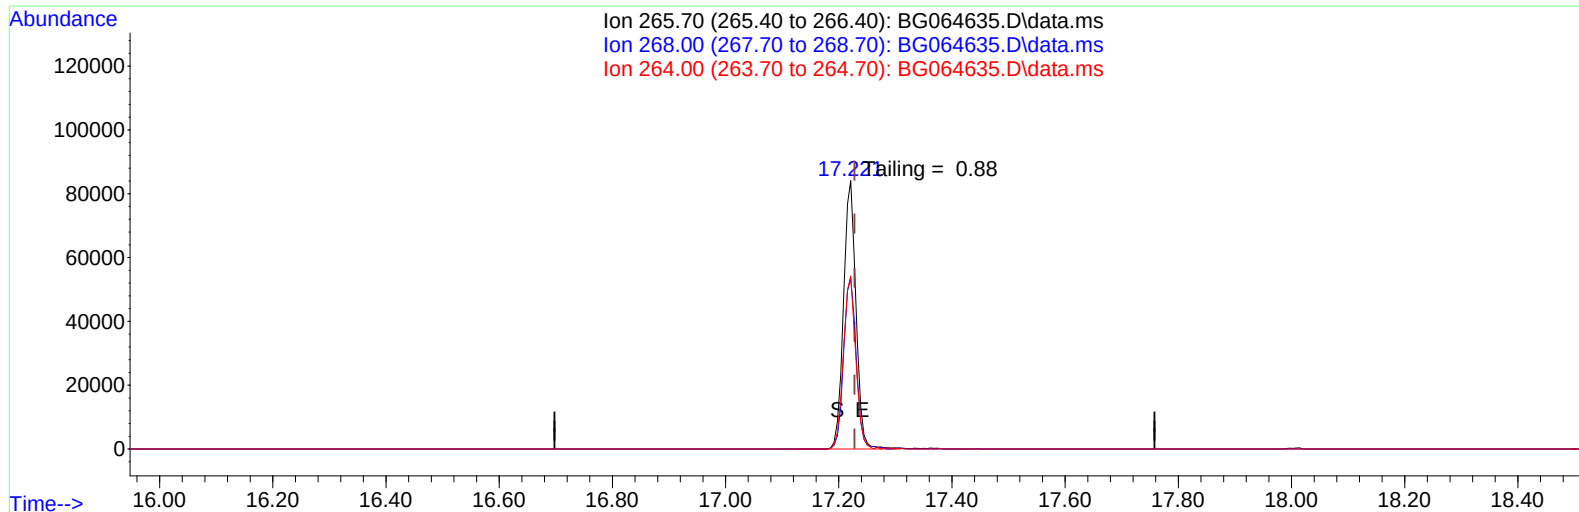

TIC: BG064635.D\data.ms

(70) Pentachlorophenol (C)

17.221min (-0.007) 25561.00 ng




response 128648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	68.13
264.00	59.10	64.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103025\
Data File : BG064635.D
Acq On : 30 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 30 11:34:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

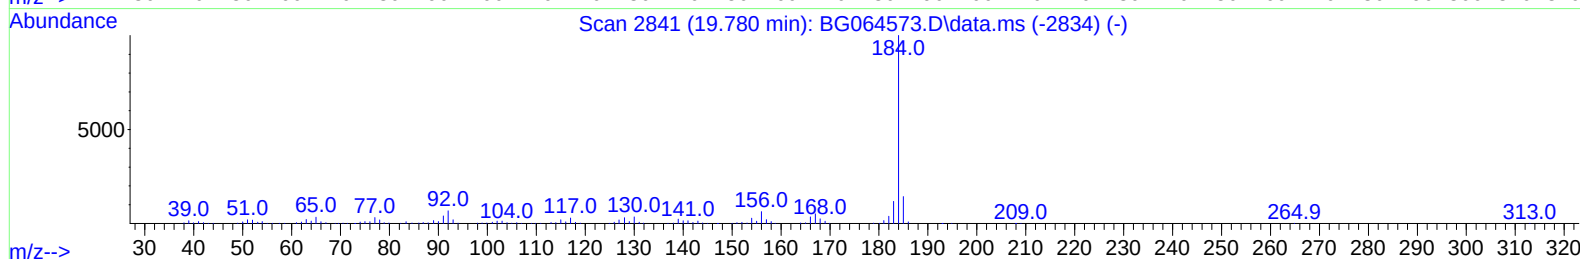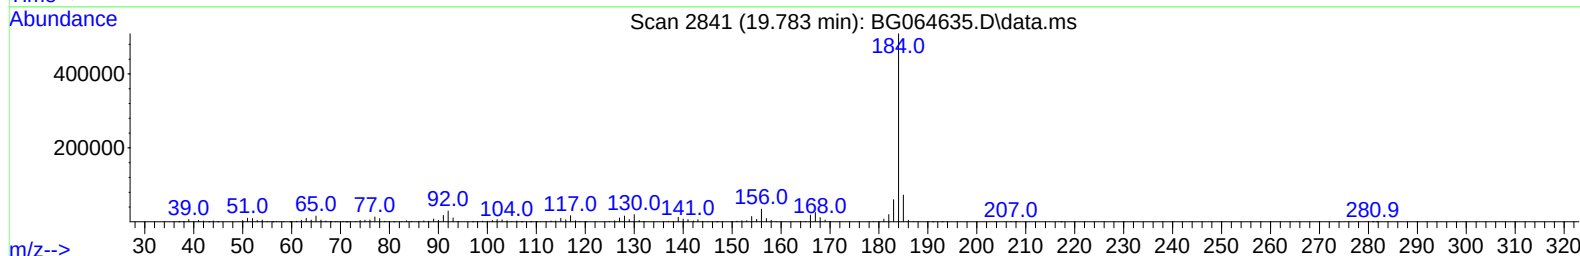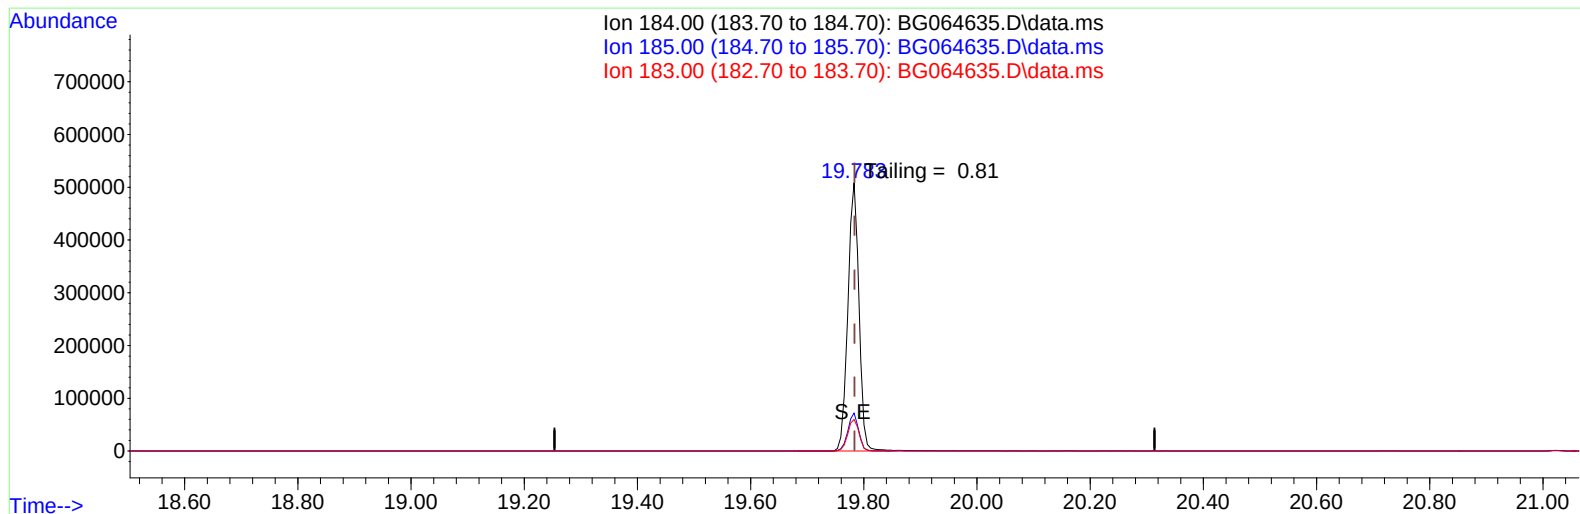

TIC: BG064635.D\data.ms

(77) Benzidine

19.783min (-0.001) 0.00 ng

response 690984

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.22
183.00	11.80	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/30/2025	BNA_G	<u>BG064635.D</u>
Compound Name	Response	Retention Time
DDT	367195	21.023
DDD	3406	20.576
DDE	398	20.077
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3804	370999	1.03

Instrument :
BNA_G
ClientSampleId :
DFTPP