


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102925\
Data File : VN088146.D
Acq On : 29 Oct 2025 09:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Title : SW846 8260
Last Update : Sat Oct 25 00:15:22 2025

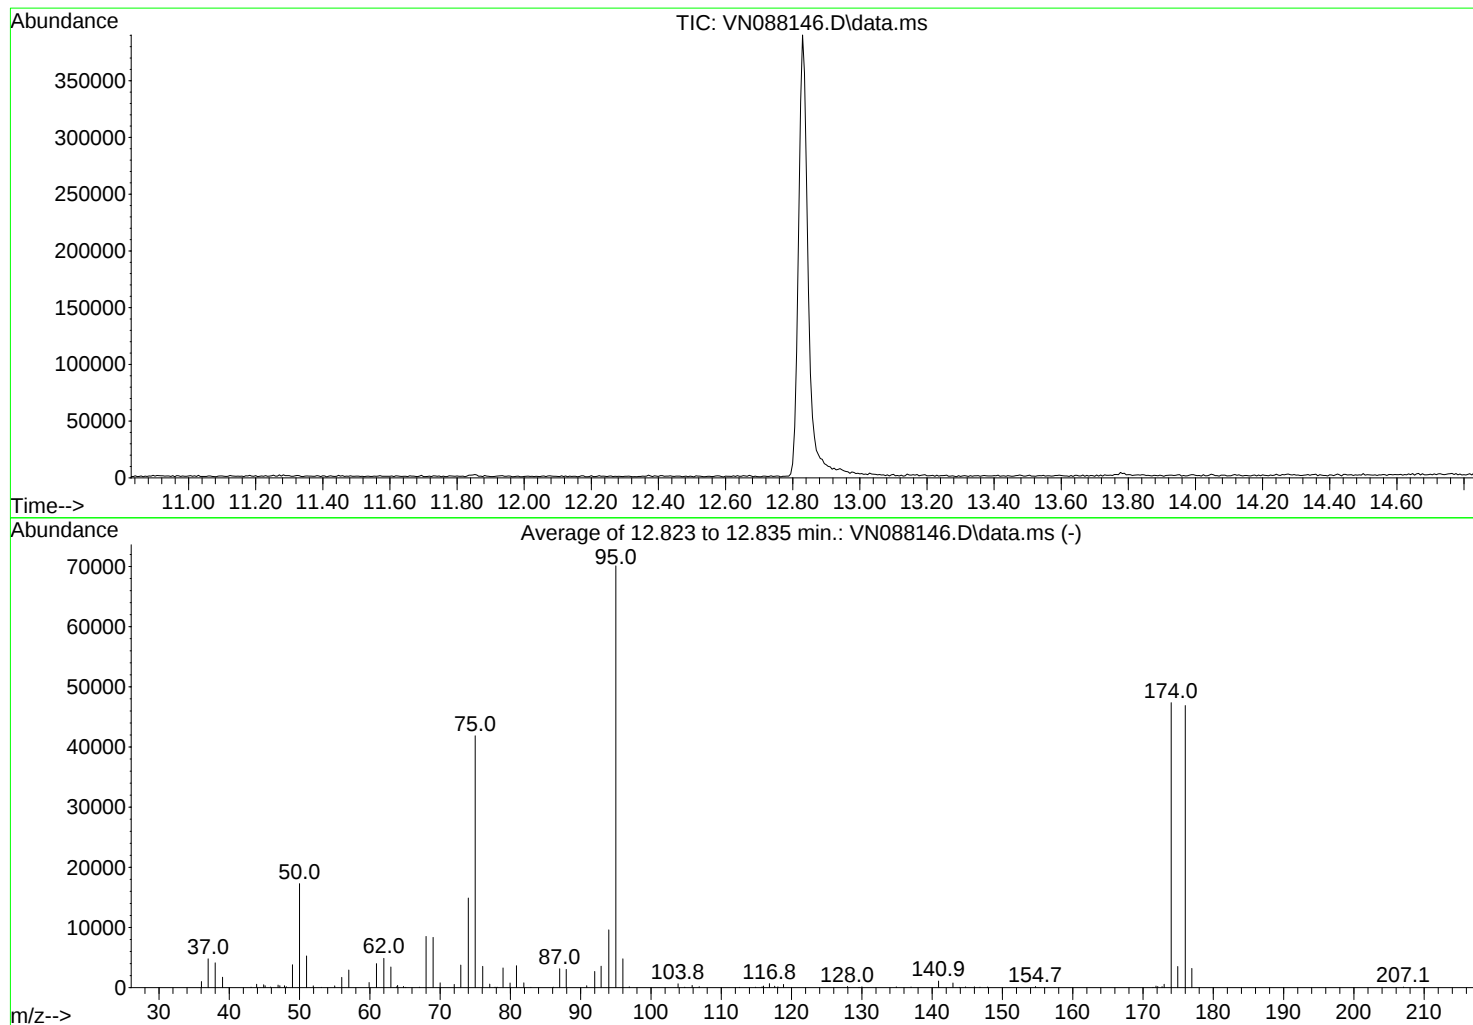

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	17300	PASS
75	95	30	60	59.7	41867	PASS
95	95	100	100	100.0	70120	PASS
96	95	5	9	6.8	4784	PASS
173	174	0.00	2	1.2	566	PASS
174	95	50	100	67.6	47387	PASS
175	174	5	9	7.4	3519	PASS
176	174	95	101	99.0	46891	PASS
177	176	5	9	6.8	3203	PASS

Average of 12.823 to 12.835 min.: VN088146.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	1020	47.85	312	60.95	3996	72.00	531
37.00	4781	48.10	150	62.00	4877	72.95	374
38.00	4116	49.00	3806	63.00	3431	74.00	1488
39.05	1737	50.00	17300	63.80	143	75.00	4186
43.10	76	51.00	5259	63.95	384	76.05	3543
43.90	565	51.95	305	64.80	195	77.05	596
44.90	479	53.10	60	65.10	58	77.80	88
45.10	322	55.00	296	67.10	89	78.10	80
45.90	97	56.00	1707	68.00	8517	78.95	3270
46.95	433	57.00	2920	69.00	8349	79.95	780
47.20	334	59.90	855	70.00	800	80.85	3640

Average of 12.823 to 12.835 min.: VN088146.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	808	96.90	125	118.05	125	146.00	125
82.90	61	103.85	632	118.85	536	146.80	74
86.10	69	104.80	72	127.95	187	147.90	110
87.00	3131	105.85	370	129.60	59	154.70	192
87.95	3024	106.85	159	130.00	124	171.40	59
90.85	329	112.60	54	134.90	131	171.85	268
92.00	2697	114.90	75	137.00	116	172.10	190
92.90	3570	115.80	142	140.90	1096	172.70	150
94.00	9597	116.00	263	142.95	783	173.00	566
95.00	70120	116.85	667	143.90	62	174.00	47387
96.00	4784	117.60	237	144.75	140	174.95	3519

Average of 12.823 to 12.835 min.: VN088146.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	46891						
176.95	3203						
207.05	120						

Instrument :

MSVOA_N

ClientSampleId :

BFB