

Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO ₄	Con SO ₄	Method name	date time	Initial wt/Final Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/3/2025 15:58	10 RM/IZ
STD2	0.417	0.655	0.659	2.182	0.549	0.953	3.345	IC1-110325	11/3/2025 16:22	10 RM/IZ
STD3	0.813	1.228	1.228	4.086	1.024	2.097	6.147	IC1-110325	11/3/2025 17:04	10 RM/IZ
STD4	1.014	1.491	1.496	4.984	1.245	2.506	7.444	IC1-110325	11/3/2025 17:47	10 RM/IZ
STD5	1.966	2.918	2.907	9.724	2.426	5.166	14.580	IC1-110325	11/3/2025 18:08	10 RM/IZ
STD6	3.912	5.914	5.907	19.694	4.918	9.286	29.234	IC1-110325	11/3/2025 18:30	10 RM/IZ
STD7	5.078	7.595	7.603	25.330	6.339	12.992	37.751	IC1-110325	11/3/2025 18:51	10 RM/IZ
ICV	1.960	2.885	2.908	9.698	2.364	5.176	14.547	IC1-110325	11/3/2025 19:13	10 RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/3/2025 19:34	10 RM/IZ
CCV	2.085	3.124	3.115	10.429	2.591	5.037	15.425	IC1-110325	11/19/2025 9:10	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/19/2025 10:15	10 RM/IZ
LB137971BLS	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/19/2025 10:36	5.00g/100mL RM/IZ
LB137971BSS	2.117	3.175	3.149	10.487	2.608	5.251	15.498	IC1-110325	11/19/2025 10:58	5.00g/100mL RM/IZ
Q3483-01	3.592	53.138	0.000	3.092	20.802	7.417	78.254	IC1-110325	11/19/2025 11:19	5.00g/100mL RM/IZ
Q3483-25	0.000	0.091	7.592	0.000	0.000	0.000	0.510	IC1-110325	11/19/2025 12:02	5.00g/100mL RM/IZ
Q3483-01DLX10	0.389	4.458	0.000	0.506	1.859	0.833	7.418	IC1-110325	11/19/2025 12:24	5.00g/100mL RM/IZ
Q3483-25DLX2	0.000	0.092	3.700	0.000	0.000	0.000	0.519	IC1-110325	11/19/2025 13:29	5.00g/100mL RM/IZ
CCV	2.088	3.130	3.124	10.468	2.592	5.132	15.498	IC1-110325	11/19/2025 13:50	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/19/2025 14:12	10 RM/IZ

Clear table


Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A										
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-110325	11/3/2025 15:58	10 RM/IZ
STD2	0.4170	0.6550	0.6590	2.1820	0.5490	0.9530	3.3450	IC1-110325	11/3/2025 16:22	10 RM/IZ
STD3	0.8130	1.2280	1.2280	4.0860	1.0240	2.0970	6.1470	IC1-110325	11/3/2025 17:04	10 RM/IZ
STD4	1.0140	1.4910	1.4960	4.9840	1.2450	2.5060	7.4440	IC1-110325	11/3/2025 17:47	10 RM/IZ
STD5	1.9660	2.9180	2.9070	9.7240	2.4260	5.1660	14.5800	IC1-110325	11/3/2025 18:08	10 RM/IZ
STD6	3.9120	5.9140	5.9070	19.6940	4.9180	9.2860	29.2340	IC1-110325	11/3/2025 18:30	10 RM/IZ
STD7	5.0780	7.5950	7.6030	25.3300	6.3390	12.9920	37.7510	IC1-110325	11/3/2025 18:51	10 RM/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	4.2500	9.1667	9.8333	9.1000	9.8000	-4.7000	11.5000
STD3	1.6250	2.3333	2.3333	2.1500	2.4000	4.8500	2.4500
STD4	1.4000	-0.6000	-0.2667	-0.3200	-0.4000	0.2400	-0.7467
STD5	-1.7000	-2.7333	-3.1000	-2.7600	-2.9600	3.3200	-2.8000
STD6	-2.2000	-1.4333	-1.5500	-1.5300	-1.6400	-7.1400	-2.5533
STD7	1.5600	1.2667	1.3733	1.3200	1.4240	3.9360	2.0297

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

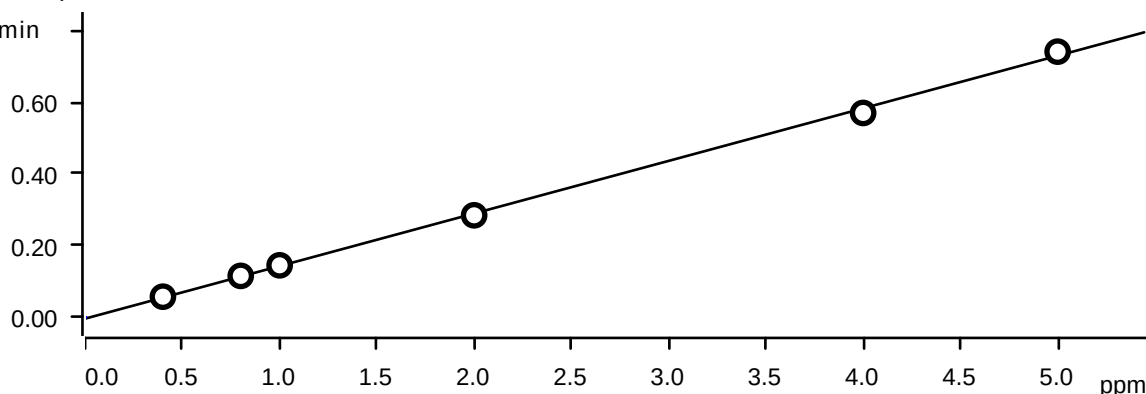

Function: $A = -3.63197E-3 + 0.0146595 \times Q$


Relative standard deviation: 2.880512 %

Correlation coefficient: 0.999558

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.116	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.145	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.285	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.570	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.741	STD7	2025-11-03 18:51:52 UTC-5	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

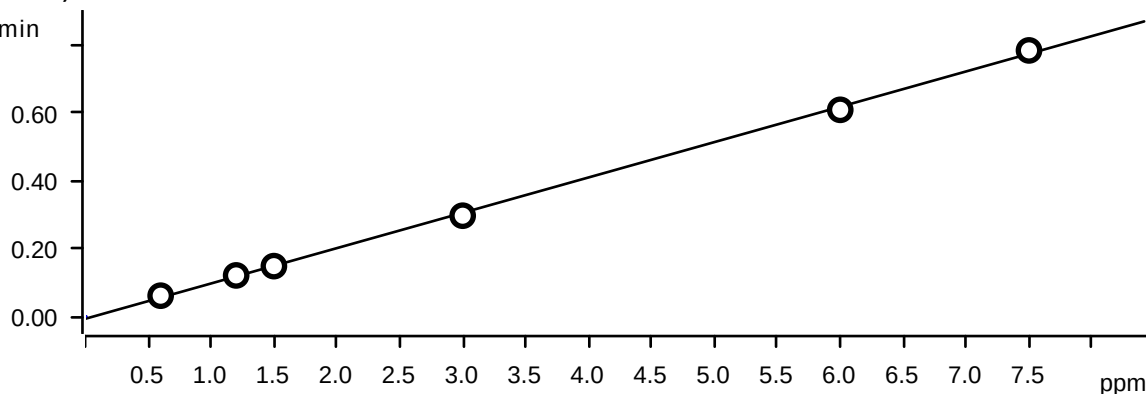


Function: $A = -7.14286E-3 + 0.0104011 \times Q$

Relative standard deviation 2.544562 %

Correlation coefficient 0.999662

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.061	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.121	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.148	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.296	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.608	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.783	STD7	2025-11-03 18:51:52 UTC-5	used

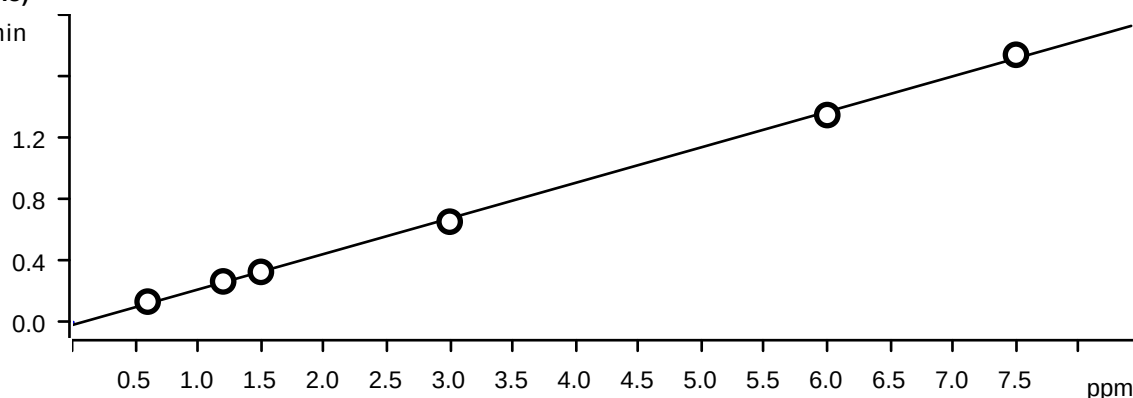Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0188106 + 0.0231263 \times Q$


Relative standard deviation 2.785229 %

Correlation coefficient 0.999598

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.134	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.265	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.654	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.347	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.740	STD7	2025-11-03 18:51:52 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

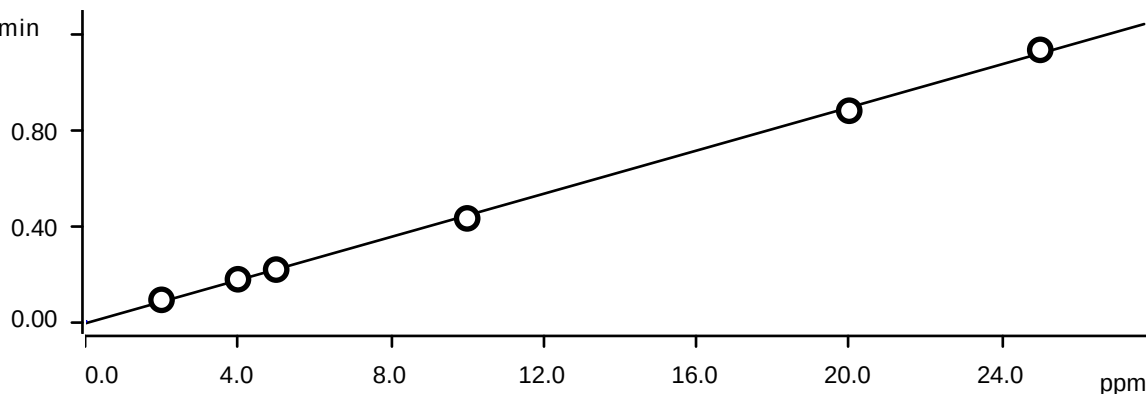

Function: $A = -8.73633E-3 + 4.51609E-3 \times Q$


Relative standard deviation: 2.618377 %

Correlation coefficient: 0.999640

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.090	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.176	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.216	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.430	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.881	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.135	STD7	2025-11-03 18:51:52 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

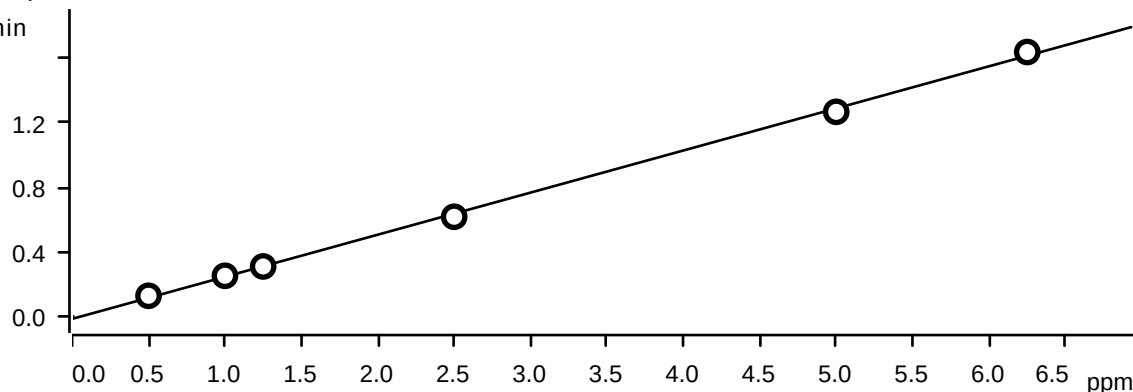


Function: $A = -0.0164240 + 0.0260850 \times Q$

Relative standard deviation: 2.824357 %

Correlation coefficient 0.999585

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.127	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.251	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.308	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.616	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.266	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.637	STD7	2025-11-03 18:51:52 UTC-5	used

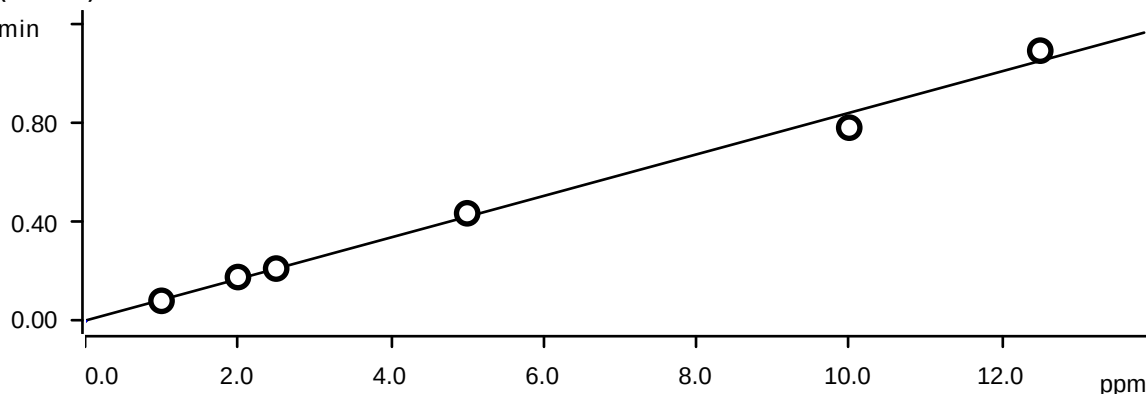
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = 1.95294E-3 + 8.36815E-3 \times Q$

Relative standard deviation 8.053642 %

Correlation coefficient 0.996454

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.177	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.212	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.434	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.779	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.089	STD7	2025-11-03 18:51:52 UTC-5	used

Sulfate (Anions)

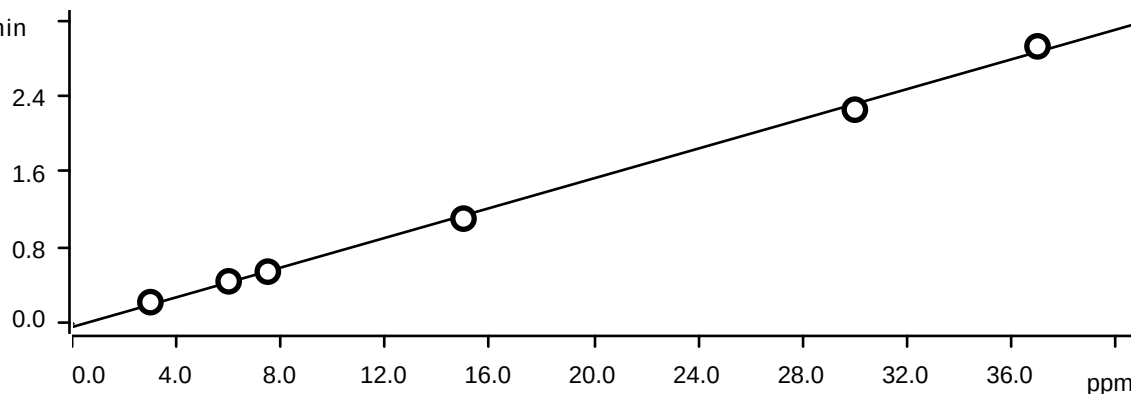 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0341972 + 7.83080E-3 \times Q$

Relative standard deviation 3.795793 %

Correlation coefficient 0.999249


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.228	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.447	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.549	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.108	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.255	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.922	STD7	2025-11-03 18:51:52 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-11-03 15:58:57 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

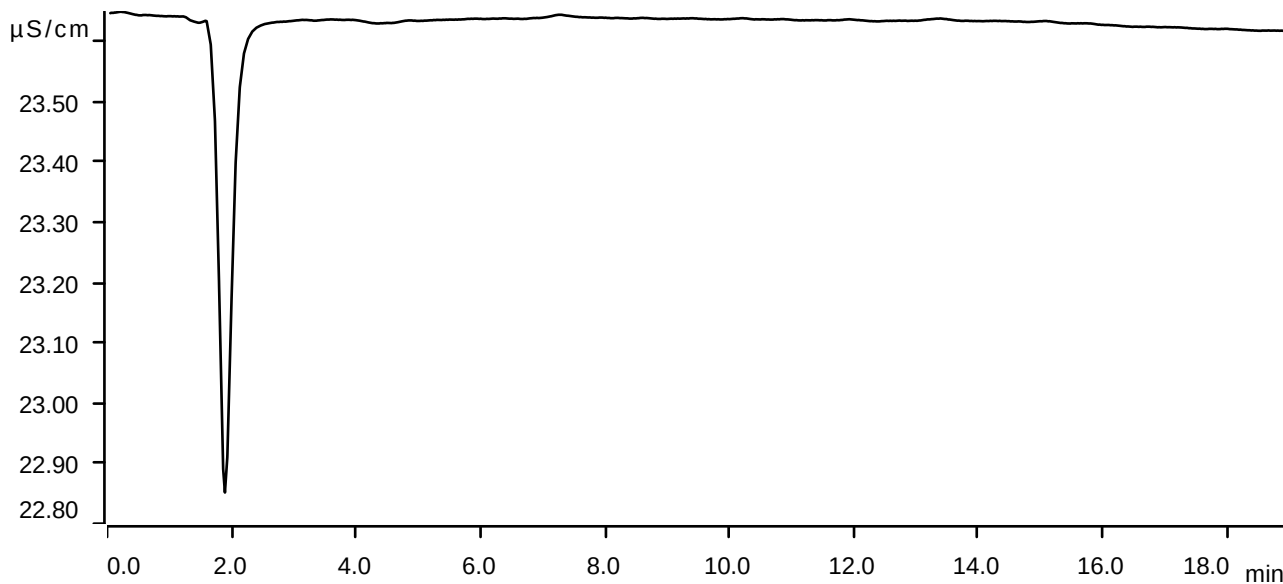Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-11-03 16:22:03 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

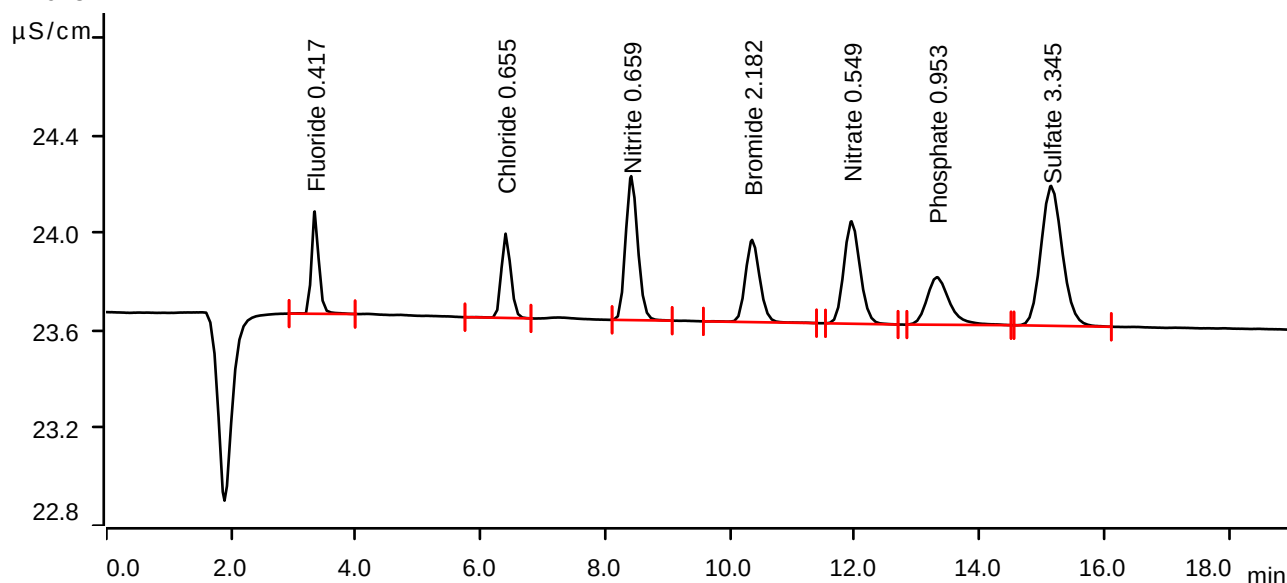

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.340	0.0576	0.420	0.417	Fluoride
2	6.402	0.0609	0.345	0.655	Chloride
3	8.415	0.1336	0.590	0.659	Nitrite
4	10.353	0.0898	0.337	2.182	Bromide
5	11.947	0.1268	0.420	0.549	Nitrate
6	13.317	0.0817	0.195	0.953	Phosphate
7	15.147	0.2277	0.574	3.345	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-11-03 17:04:52 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

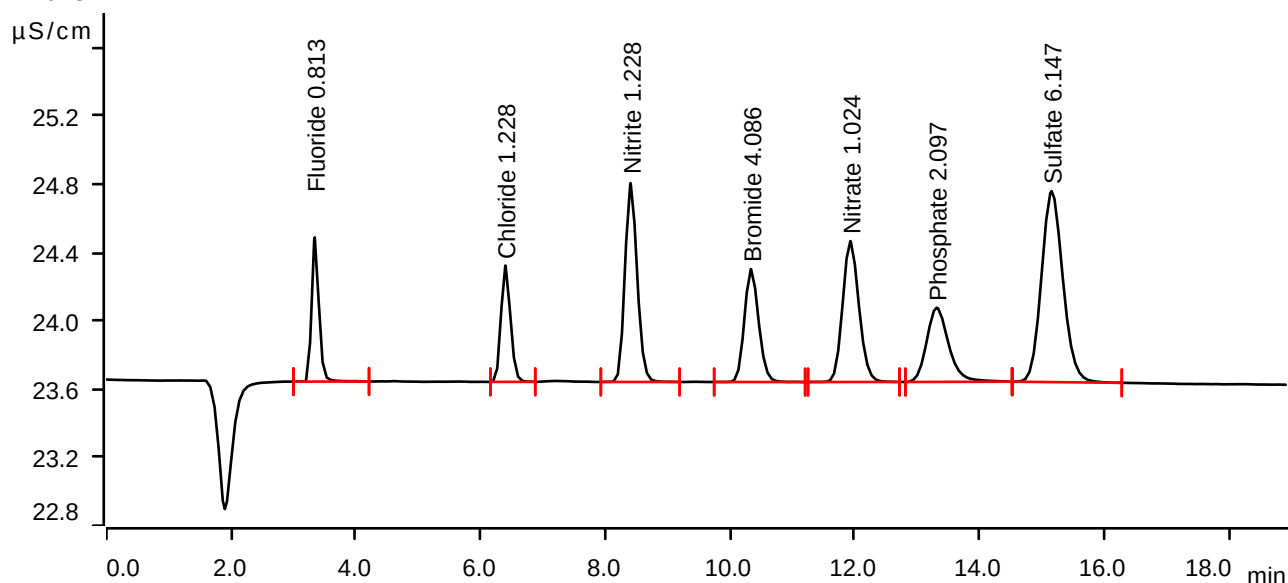

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.1156	0.844	0.813	Fluoride
2	6.397	0.1206	0.681	1.228	Chloride
3	8.407	0.2651	1.164	1.228	Nitrite
4	10.337	0.1758	0.661	4.086	Bromide
5	11.928	0.2506	0.825	1.024	Nitrate
6	13.312	0.1774	0.435	2.097	Phosphate
7	15.155	0.4471	1.119	6.147	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-11-03 17:47:32 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

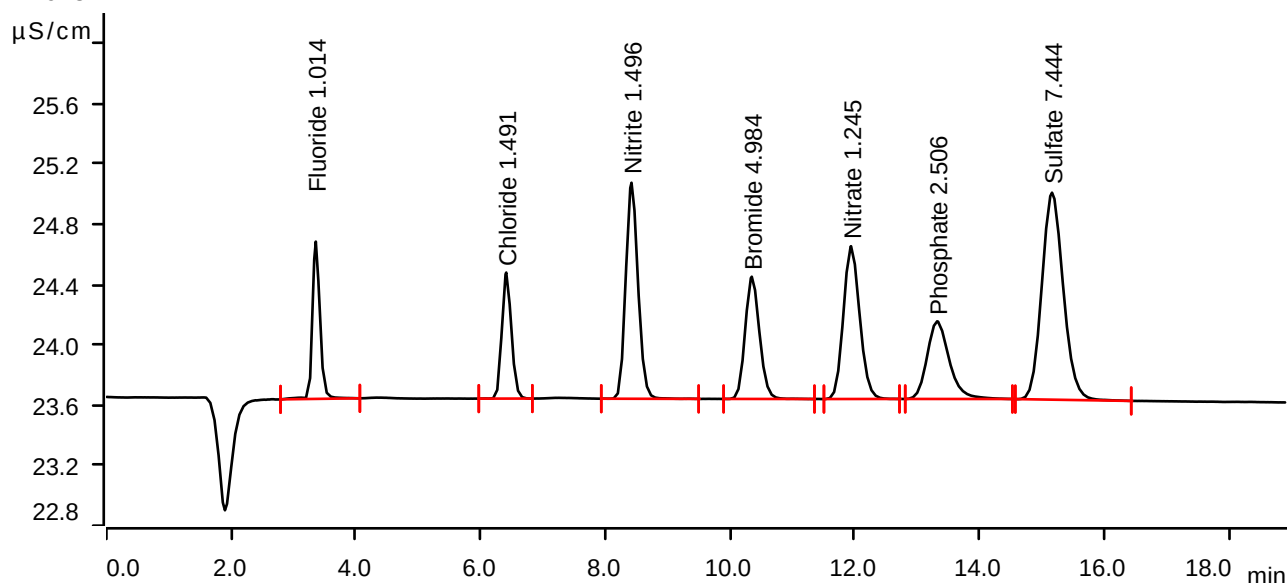

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.1450	1.044	1.014	Fluoride
2	6.412	0.1479	0.837	1.491	Chloride
3	8.420	0.3271	1.434	1.496	Nitrite
4	10.348	0.2164	0.811	4.984	Bromide
5	11.940	0.3084	1.014	1.245	Nitrate
6	13.320	0.2117	0.516	2.506	Phosphate
7	15.162	0.5487	1.374	7.444	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-11-03 18:08:59 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

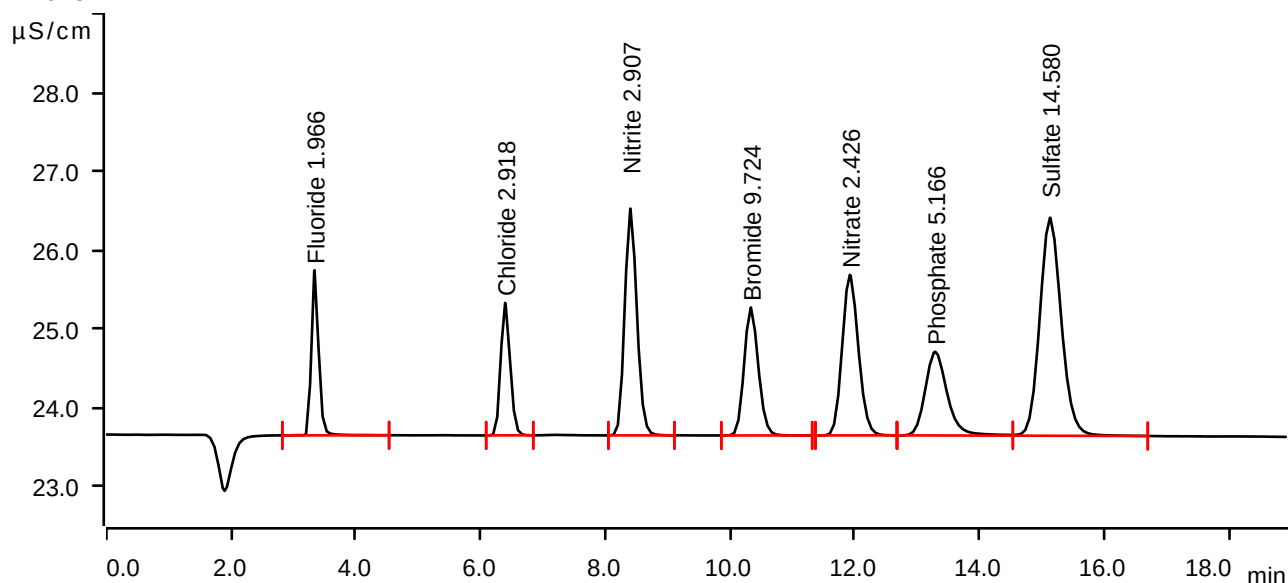

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.338	0.2845	2.095	1.966	Fluoride
2	6.393	0.2963	1.681	2.918	Chloride
3	8.403	0.6535	2.878	2.907	Nitrite
4	10.332	0.4304	1.624	9.724	Bromide
5	11.920	0.6163	2.038	2.426	Nitrate
6	13.290	0.4342	1.063	5.166	Phosphate
7	15.128	1.1075	2.767	14.580	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-11-03 18:30:25 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

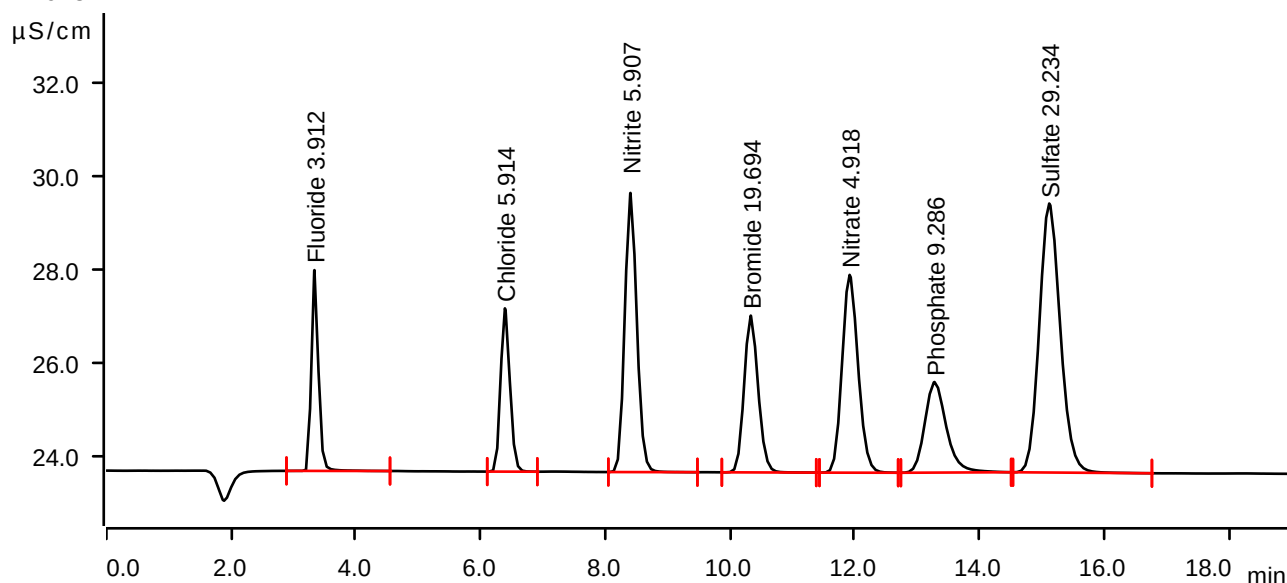

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.337	0.5698	4.312	3.912	Fluoride
2	6.390	0.6080	3.506	5.914	Chloride
3	8.403	1.3473	5.995	5.907	Nitrite
4	10.330	0.8806	3.367	19.694	Bromide
5	11.917	1.2665	4.248	4.918	Nitrate
6	13.278	0.7790	1.945	9.286	Phosphate
7	15.117	2.2550	5.777	29.234	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-11-03 18:51:52 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

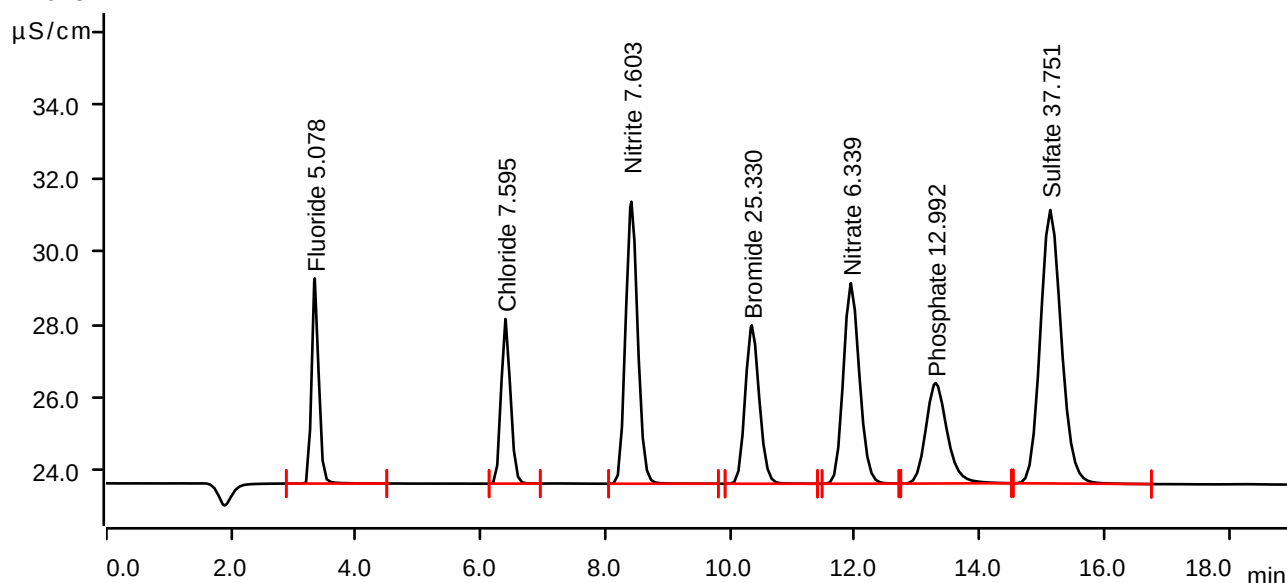


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.7408	5.606	5.078	Fluoride
2	6.398	0.7828	4.499	7.595	Chloride
3	8.418	1.7395	7.709	7.603	Nitrite
4	10.348	1.1352	4.330	25.330	Bromide
5	11.937	1.6370	5.482	6.339	Nitrate
6	13.295	1.0891	2.746	12.992	Phosphate
7	15.133	2.9220	7.473	37.751	Sulfate

Sample data

Ident ICV
 Sample type Check standard 1
 Determination start 2025-11-03 19:13:20 UTC-5
 Method IC1-110325
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.39 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

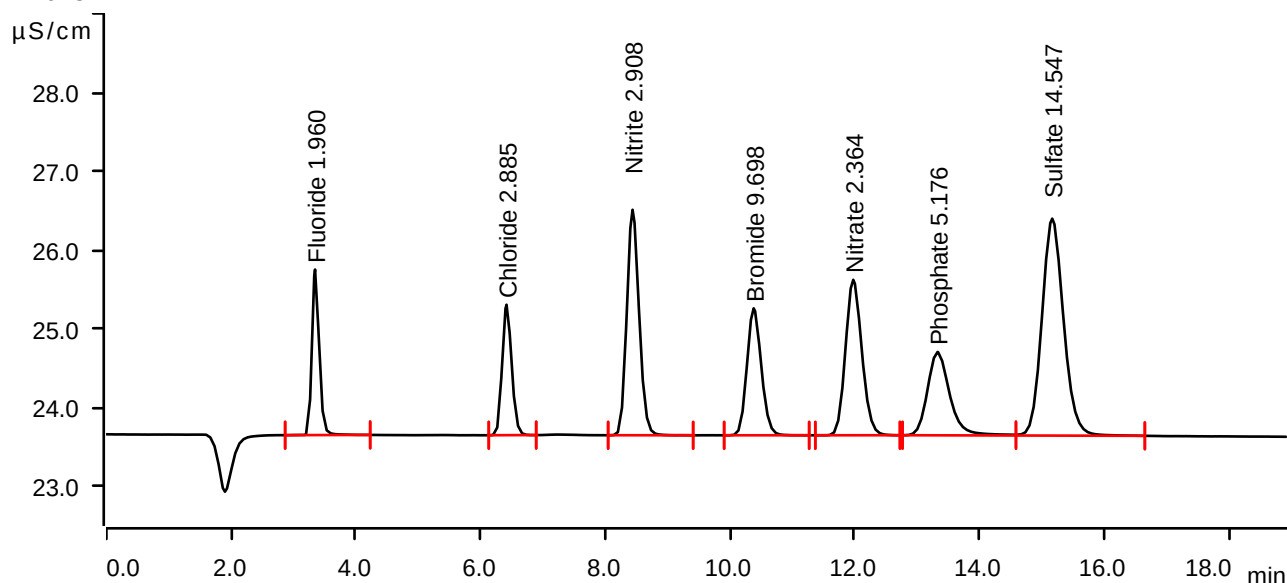Anions


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.347	0.2837	2.100	1.960	Fluoride
2	6.417	0.2929	1.656	2.885	Chloride
3	8.437	0.6536	2.862	2.908	Nitrite
4	10.378	0.4292	1.611	9.698	Bromide
5	11.975	0.6003	1.973	2.364	Nitrate
6	13.327	0.4351	1.058	5.176	Phosphate
7	15.165	1.1050	2.753	14.547	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-11-03 19:34:48 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

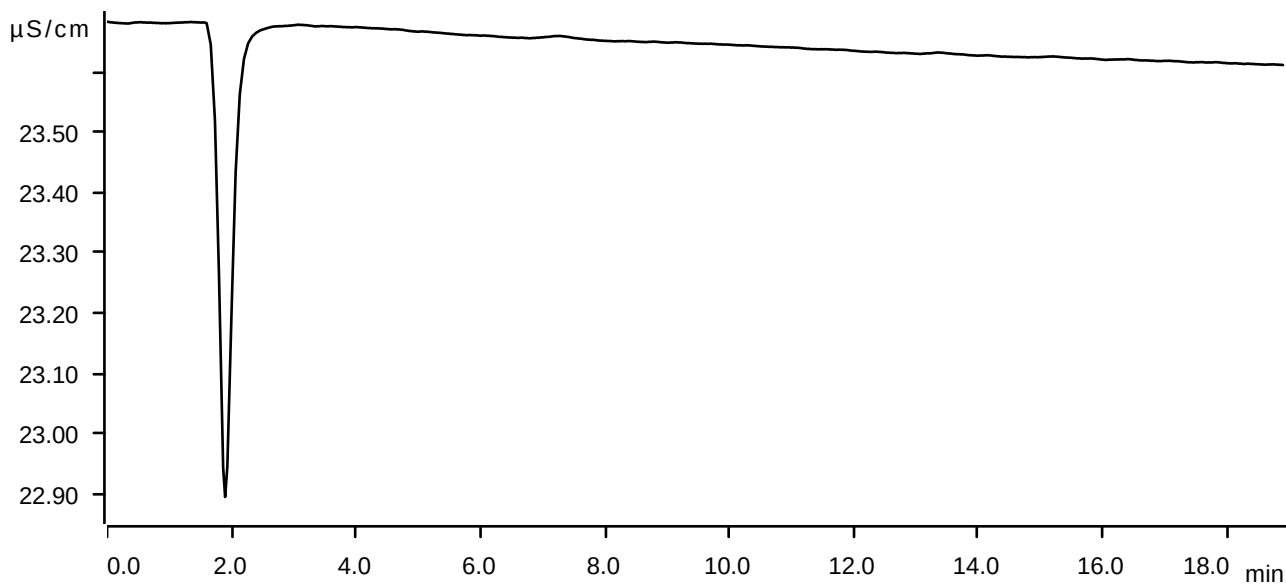Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-11-19 09:10:39 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

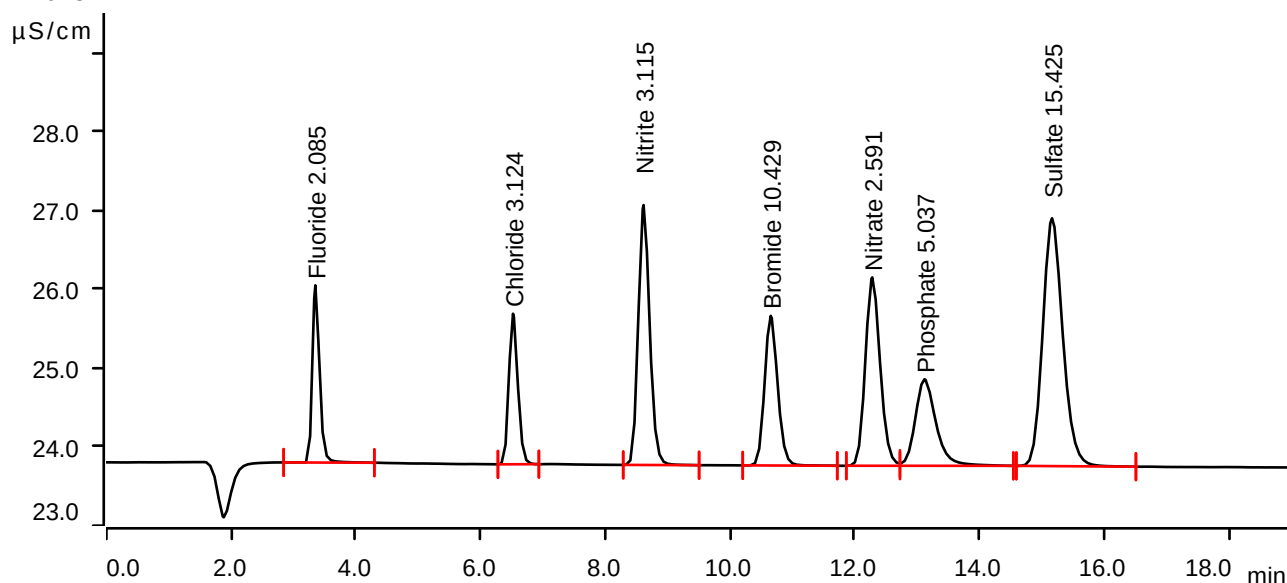


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.3020	2.248	2.085	Fluoride
2	6.520	0.3178	1.910	3.124	Chloride
3	8.613	0.7015	3.297	3.115	Nitrite
4	10.652	0.4622	1.899	10.429	Bromide
5	12.280	0.6594	2.391	2.591	Nitrate
6	13.117	0.4235	1.098	5.037	Phosphate
7	15.162	1.1737	3.145	15.425	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-11-19 10:15:12 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

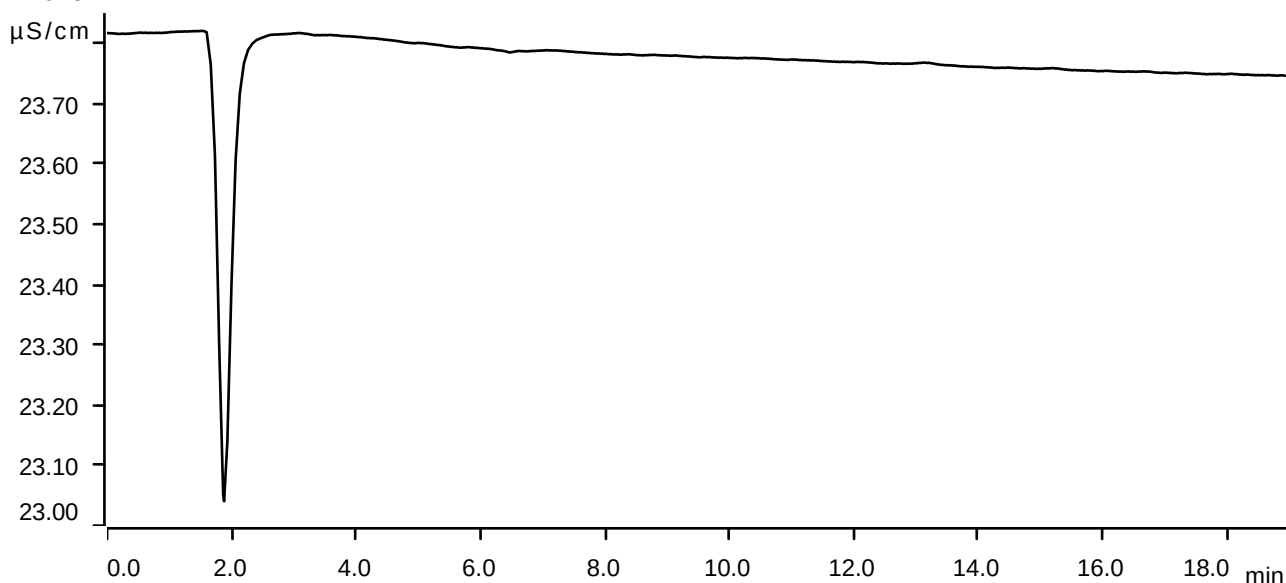
Anions

Sample data

Ident LB137971BLS
Sample type Sample
Determination start 2025-11-19 10:36:42 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

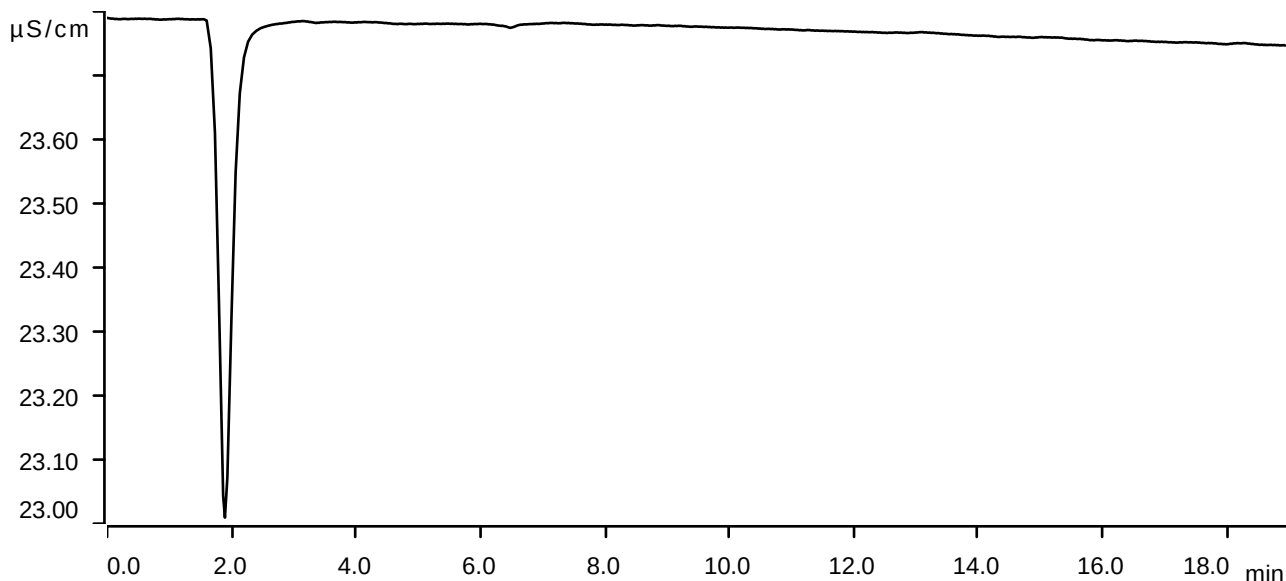Anions


Sample data

Ident LB137971BSS
Sample type Check standard 1
Determination start 2025-11-19 10:58:14 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

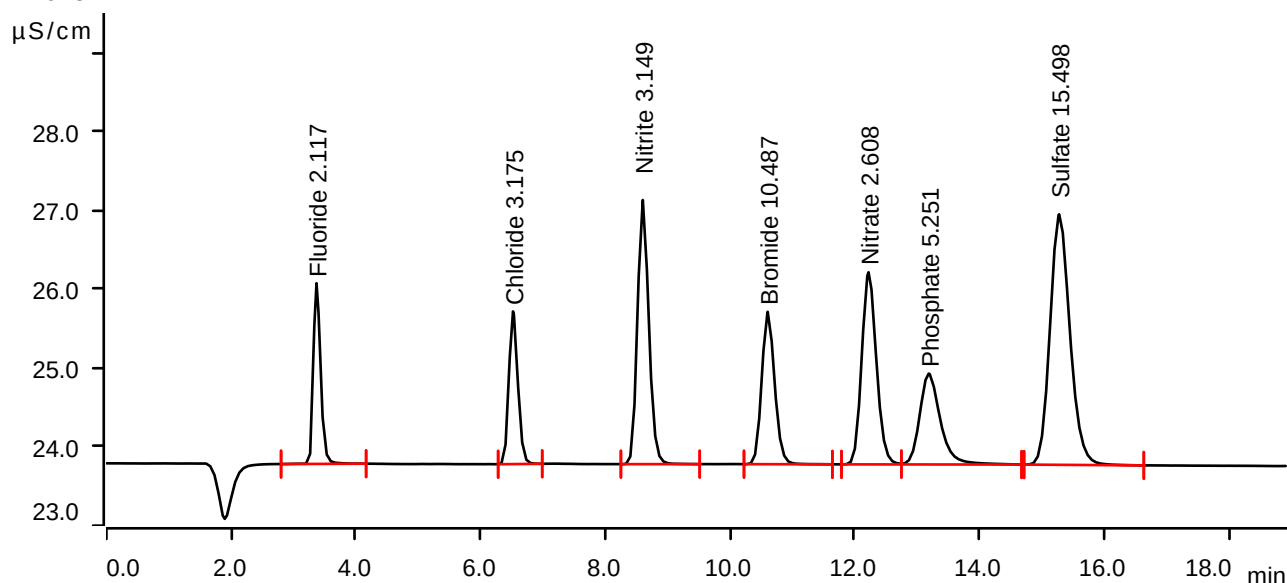

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.370	0.3068	2.293	2.117	Fluoride
2	6.520	0.3230	1.937	3.175	Chloride
3	8.600	0.7094	3.352	3.149	Nitrite
4	10.603	0.4649	1.934	10.487	Bromide
5	12.220	0.6638	2.439	2.608	Nitrate
6	13.185	0.4414	1.153	5.251	Phosphate
7	15.277	1.1795	3.179	15.498	Sulfate


Sample data

Ident Q3483-01
Sample type Sample
Determination start 2025-11-19 11:19:46 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

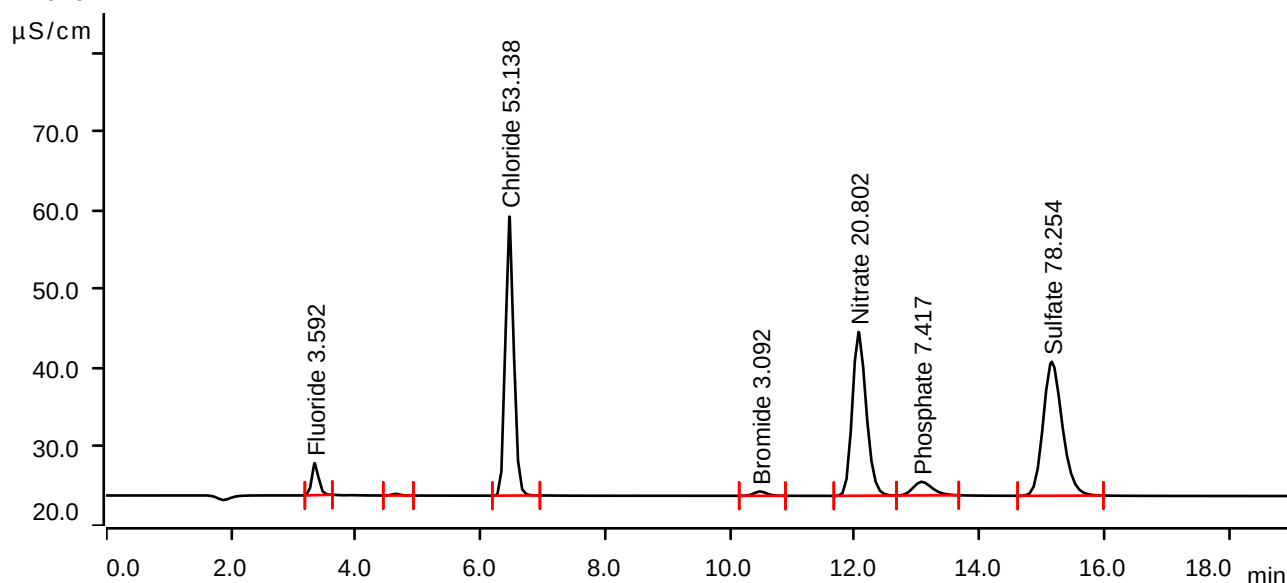

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.5229	4.082	3.592	Fluoride
2	4.637	0.0326	0.204	invalid	
3	6.462	5.5197	35.408	53.138	Chloride
4	10.480	0.1309	0.552	3.092	Bromide
5	12.060	5.4097	20.782	20.802	Nitrate
6	13.073	0.6226	1.732	7.417	Phosphate
7	15.158	6.0937	17.008	78.254	Sulfate


Sample data

Ident Q3483-25
Sample type Sample
Determination start 2025-11-19 12:02:54 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

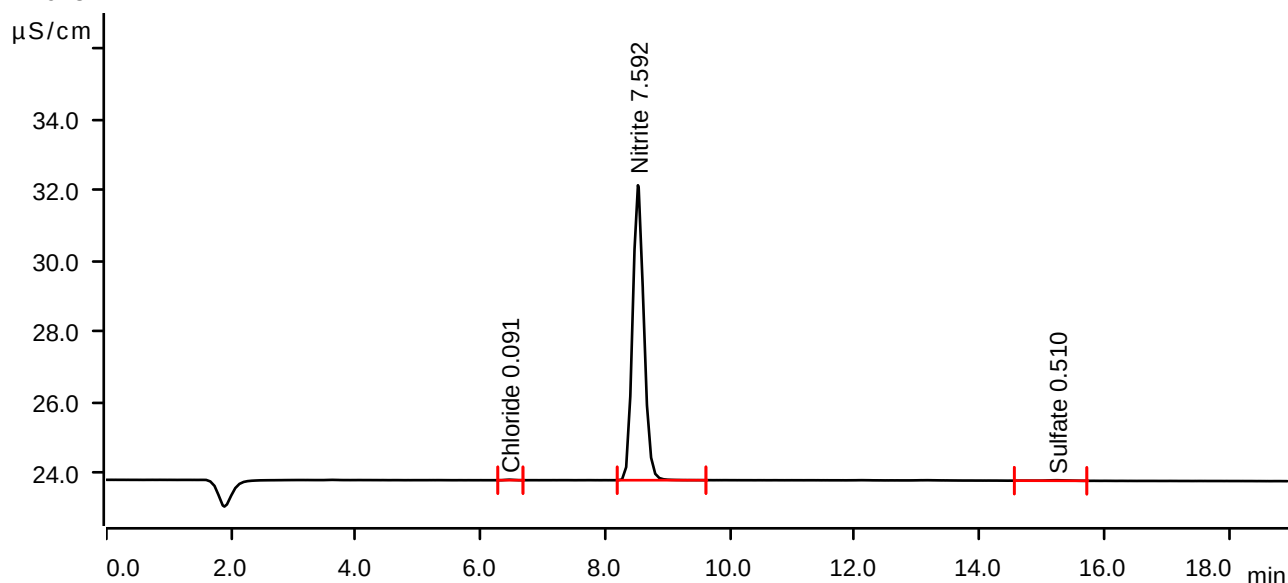

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.457	0.0024	0.015	0.091	Chloride
2	8.523	1.7371	8.349	7.592	Nitrite
3	15.237	0.0057	0.015	0.510	Sulfate


Sample data

Ident Q3483-01DLX10
Sample type Sample
Determination start 2025-11-19 12:24:28 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

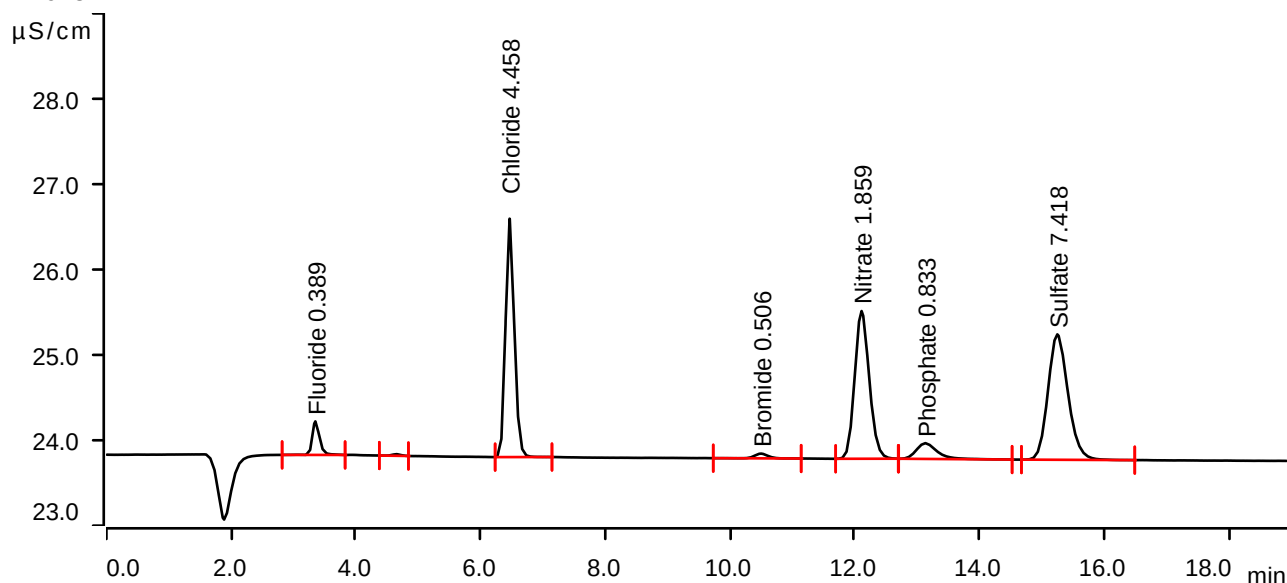

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.0535	0.393	0.389	Fluoride
2	4.652	0.0030	0.019	invalid	
3	6.465	0.4565	2.792	4.458	Chloride
4	10.500	0.0141	0.056	0.506	Bromide
5	12.108	0.4685	1.731	1.859	Nitrate
6	13.130	0.0717	0.184	0.833	Phosphate
7	15.247	0.5467	1.469	7.418	Sulfate


Sample data

Ident Q3483-25DLX2
Sample type Sample
Determination start 2025-11-19 13:29:13 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

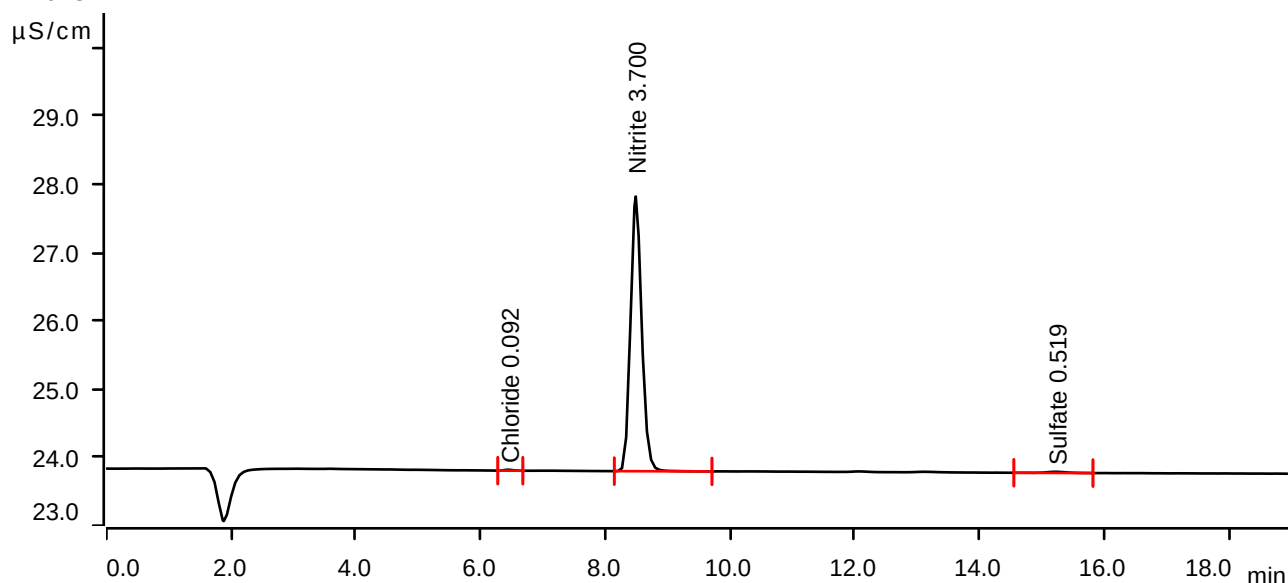

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.450	0.0024	0.015	0.092	Chloride
2	8.488	0.8368	4.022	3.700	Nitrite
3	15.232	0.0064	0.017	0.519	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-11-19 13:50:46 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

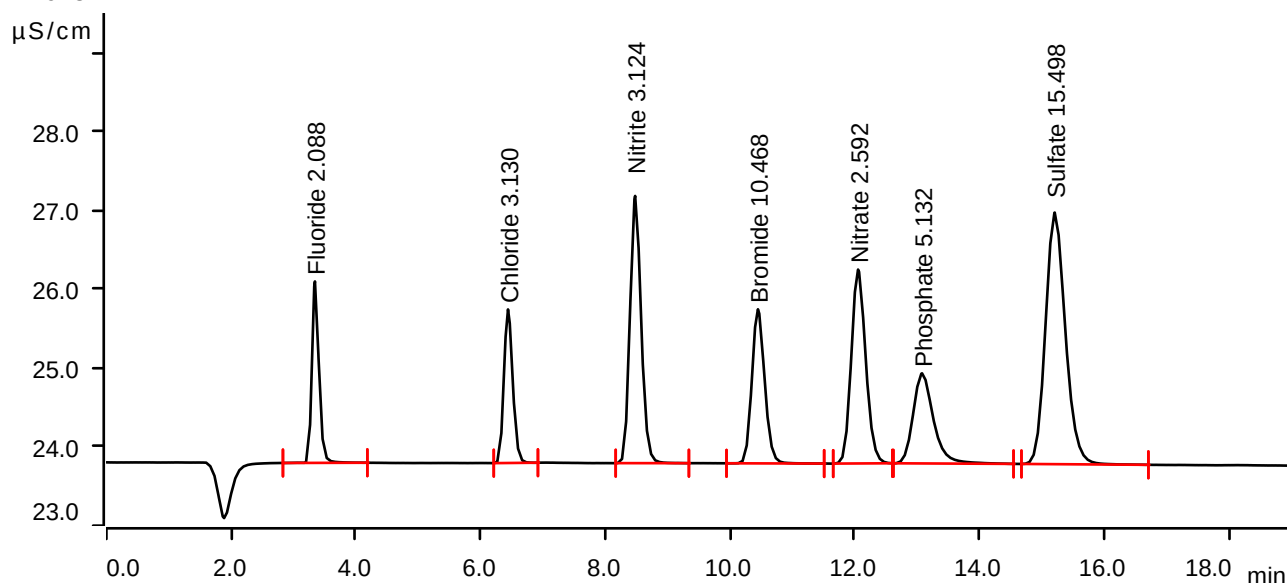


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.345	0.3025	2.302	2.088	Fluoride
2	6.440	0.3184	1.949	3.130	Chloride
3	8.478	0.7037	3.391	3.124	Nitrite
4	10.447	0.4640	1.956	10.468	Bromide
5	12.052	0.6598	2.461	2.592	Nitrate
6	13.078	0.4314	1.143	5.132	Phosphate
7	15.205	1.1794	3.193	15.498	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-11-19 14:12:16 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

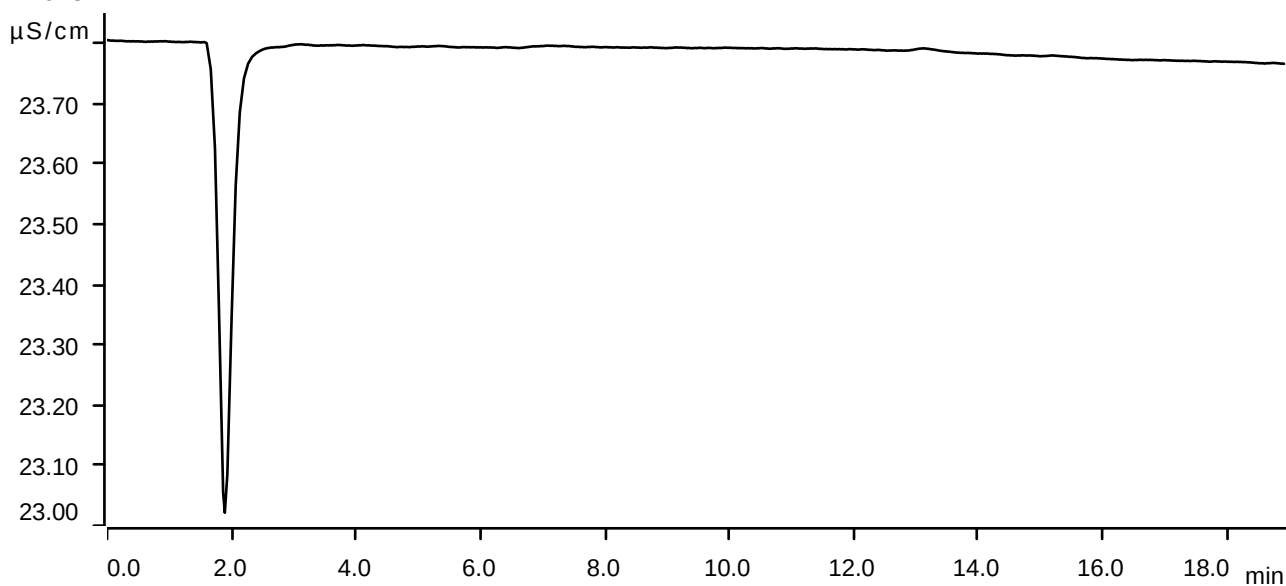Anions

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Anions-111925 WorkList ID : 193392 Department : Wet-Chemistry Date : 11-19-2025 09:18:23

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3483-01	HW1025-PT-AN-SOIL	Solid	Anions Group1	1:1 HNO3 to pH < 2	ALLI03	QA Of	10/27/2025	9056A
Q3483-25	HW1025-PT-NO2-SOIL	Solid	Anions Group2	1:1 HNO3 to pH < 2	ALLI03	QA Of	10/27/2025	9056A

Date/Time 11/19/25 09:25
 Raw Sample Received by: R (WC)
 Raw Sample Relinquished by: SL (QA-Off)

Date/Time NA
 Raw Sample Received by: "
 Raw Sample Relinquished by: (1