

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110425\
 Data File : FB032289.D
 Signal(s) : FID2B.CH
 Acq On : 4 Nov 2025 10:37
 Operator : YP/AJ
 Sample : BSF1104S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1104S2

Integration File: Calibration.e
 Quant Time: Nov 04 22:36:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	469011	23.124 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	1031208	37.642 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	1179600	38.287 ng/ml
3) t n-Heptane	7.755	388245	13.250 ng/ml
4) t Benzene	7.894	451514	13.043 ng/ml
6) t Toluene	10.624	1326087	37.061 ng/ml
7) t Ethylbenzene	13.060	394041	12.390 ng/ml
8) t m-Xylene	13.193	833832	25.038 ng/ml
9) t O-Xylene	13.920	793133	24.699 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	668532	24.161 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110425\
Data File : FB032289.D
Signal(s) : FID2B.CH
Acq On : 4 Nov 2025 10:37
Operator : YP/AJ
Sample : BSF1104S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1104S2

Integration File: Calibration.e
Quant Time: Nov 04 22:36:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

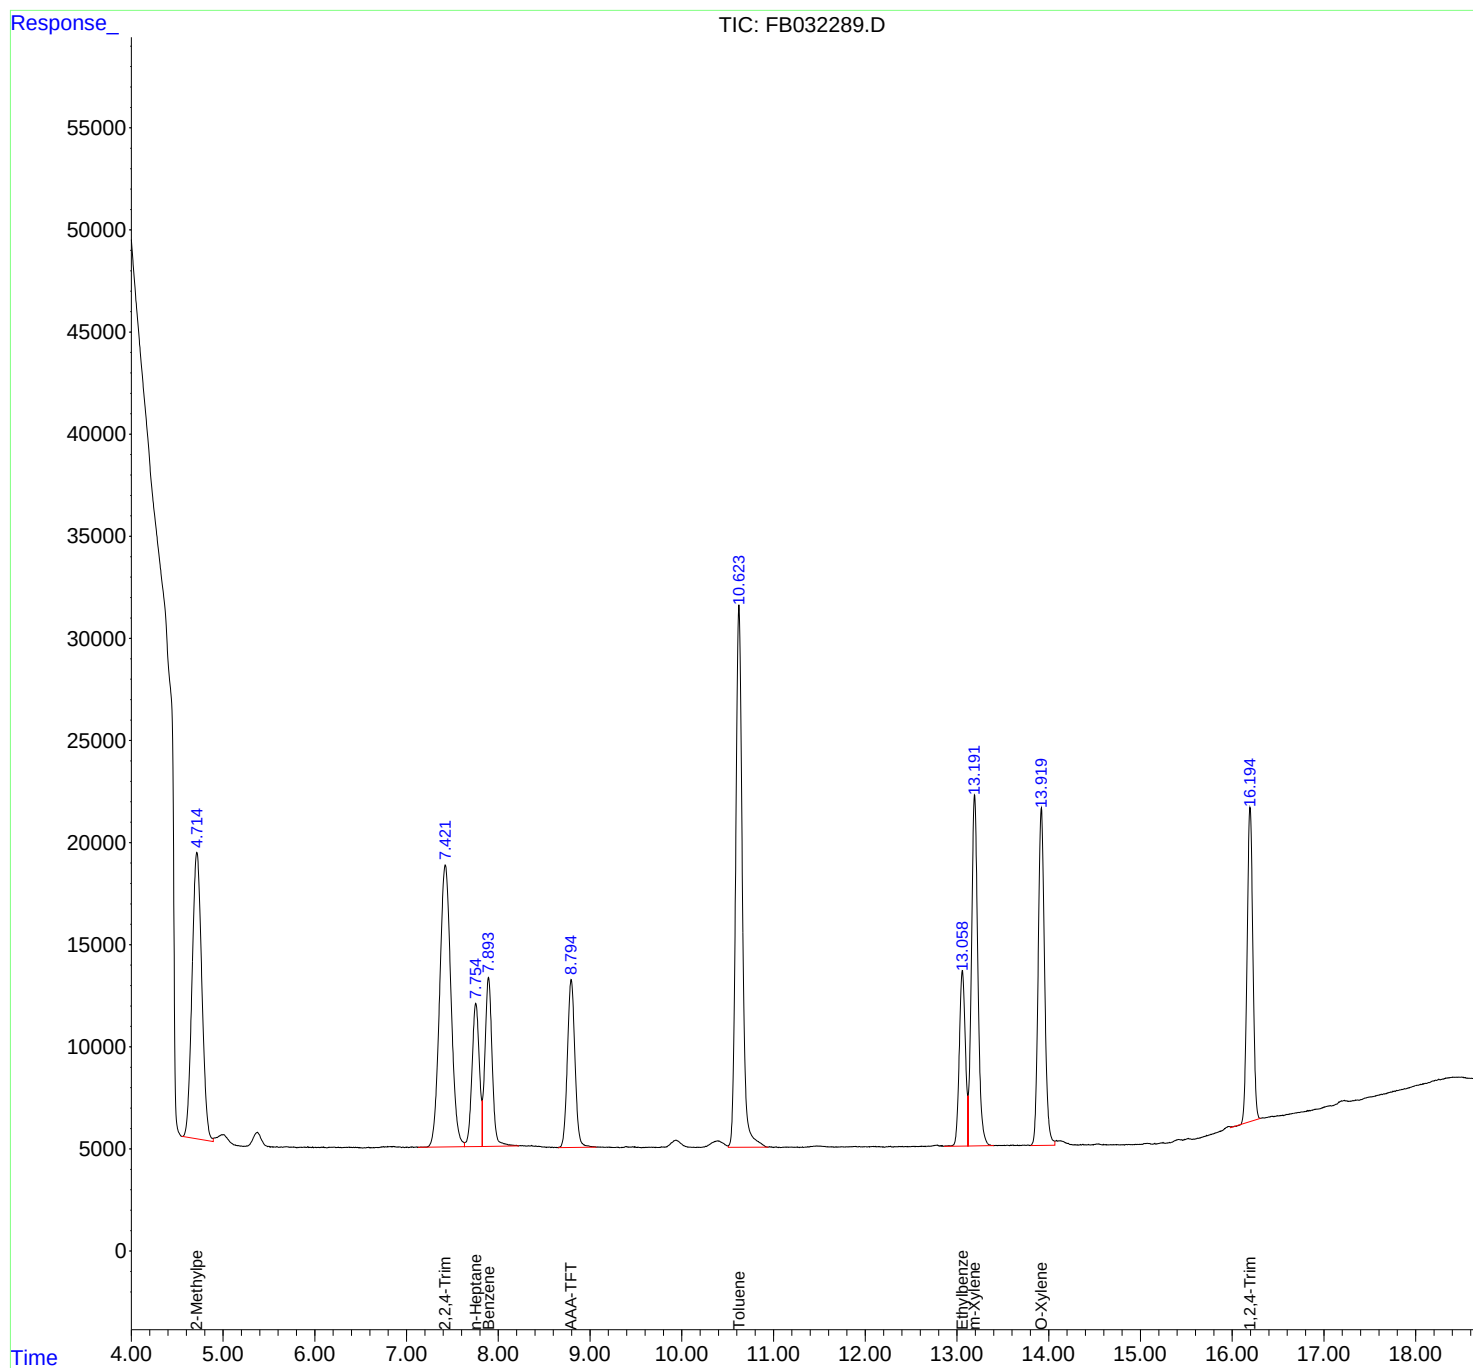


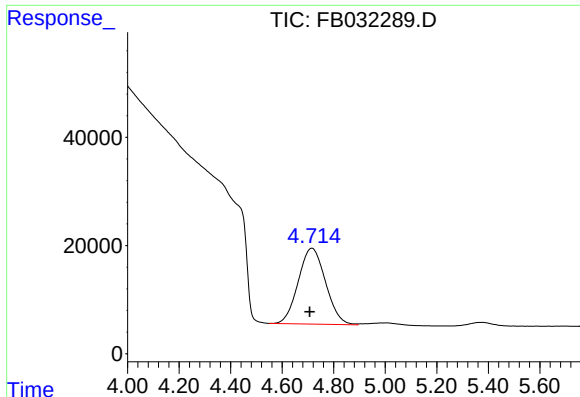

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.008 min
Response: 1031208
Conc: 37.64 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1104S2

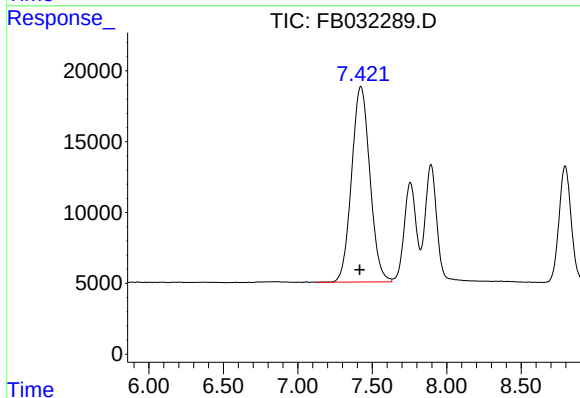


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.007 min
Response: 1179600
Conc: 38.29 ng/ml

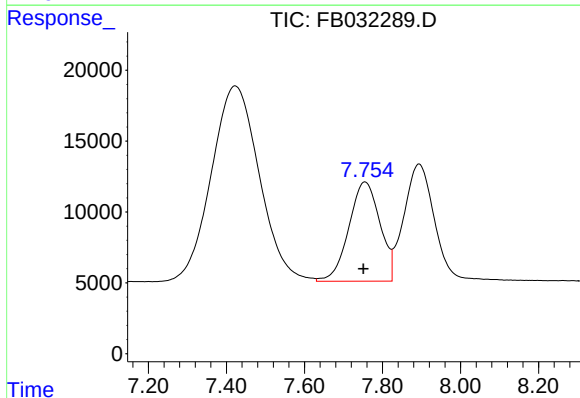


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.004 min
Response: 388245
Conc: 13.25 ng/ml

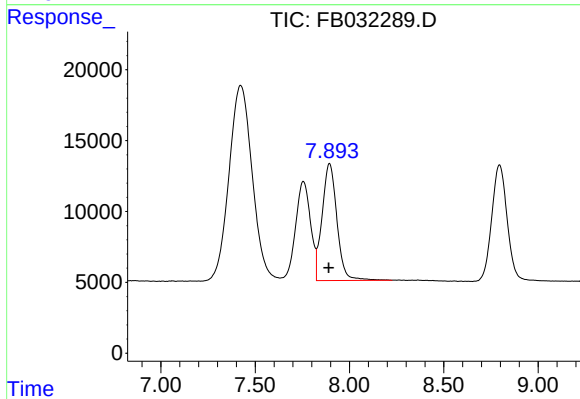

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.005 min
Response: 451514
Conc: 13.04 ng/ml

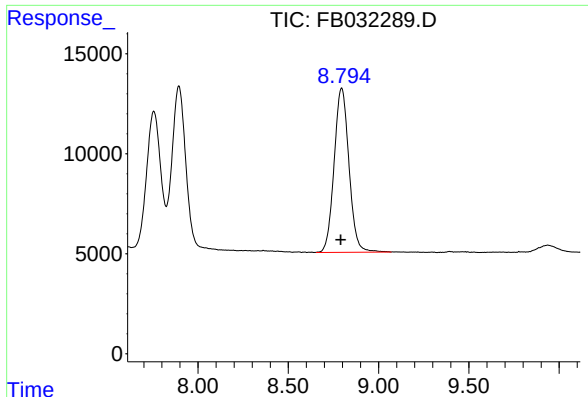

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 469011
Conc: 23.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1104S2

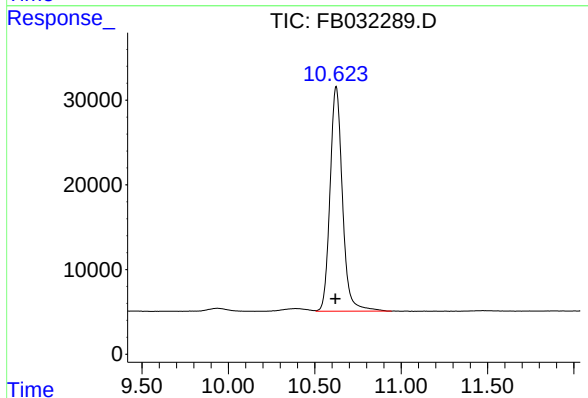


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 1326087
Conc: 37.06 ng/ml

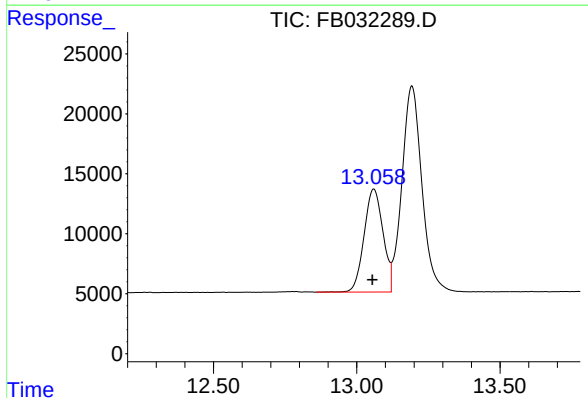


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 394041
Conc: 12.39 ng/ml

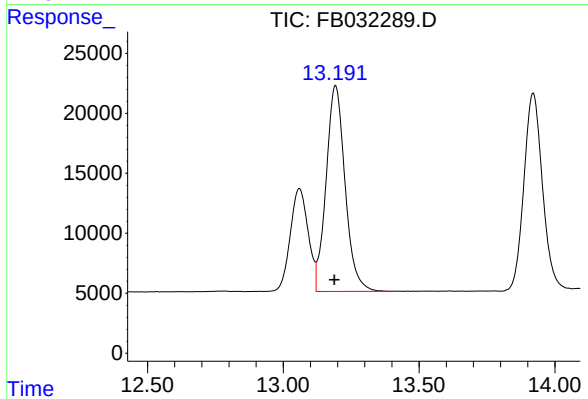

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.004 min
Response: 833832
Conc: 25.04 ng/ml

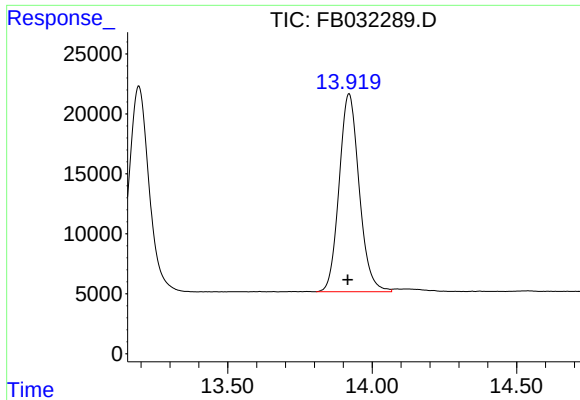

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.005 min
Response: 793133
Conc: 24.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1104S2

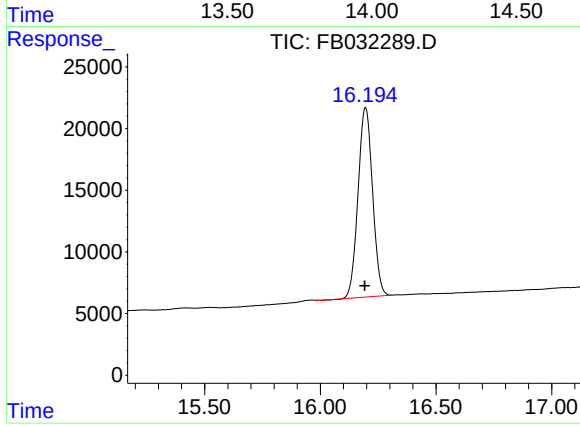

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 668532
Conc: 24.16 ng/ml