

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111525\
 Data File : PD091195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2025 20:43
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 04:48:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:46:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.874	59572378	631.9E6	17.274	17.250
28)	SA Decachlor...	9.063	8.059	86552368	667.6E6	17.373	16.869
Target Compounds							
9)	A Endosulfan I	6.067	5.235	45261732	379.7E6	7.368	7.934
10)	B gamma-Chl...	5.939	5.114	49362700	455.8E6	7.593	8.344
12)	B 4,4'-DDE	6.189	5.363	87544052	881.3E6	15.095	16.491
13)	MA Dieldrin	6.339	5.501	96362551	874.4E6	14.905	16.100
19)	B Endosulfa...	7.143	6.471	78876117	723.4E6	15.331	16.134
20)	A Methoxychlor	7.487	6.742	154.5E6	1426.0E6	71.049	71.120
21)	B Endrin ke...	7.624	6.980	80568543	766.5E6	14.302	15.043



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111525\
Data File : PD091195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2025 20:43
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 04:48:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:46:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

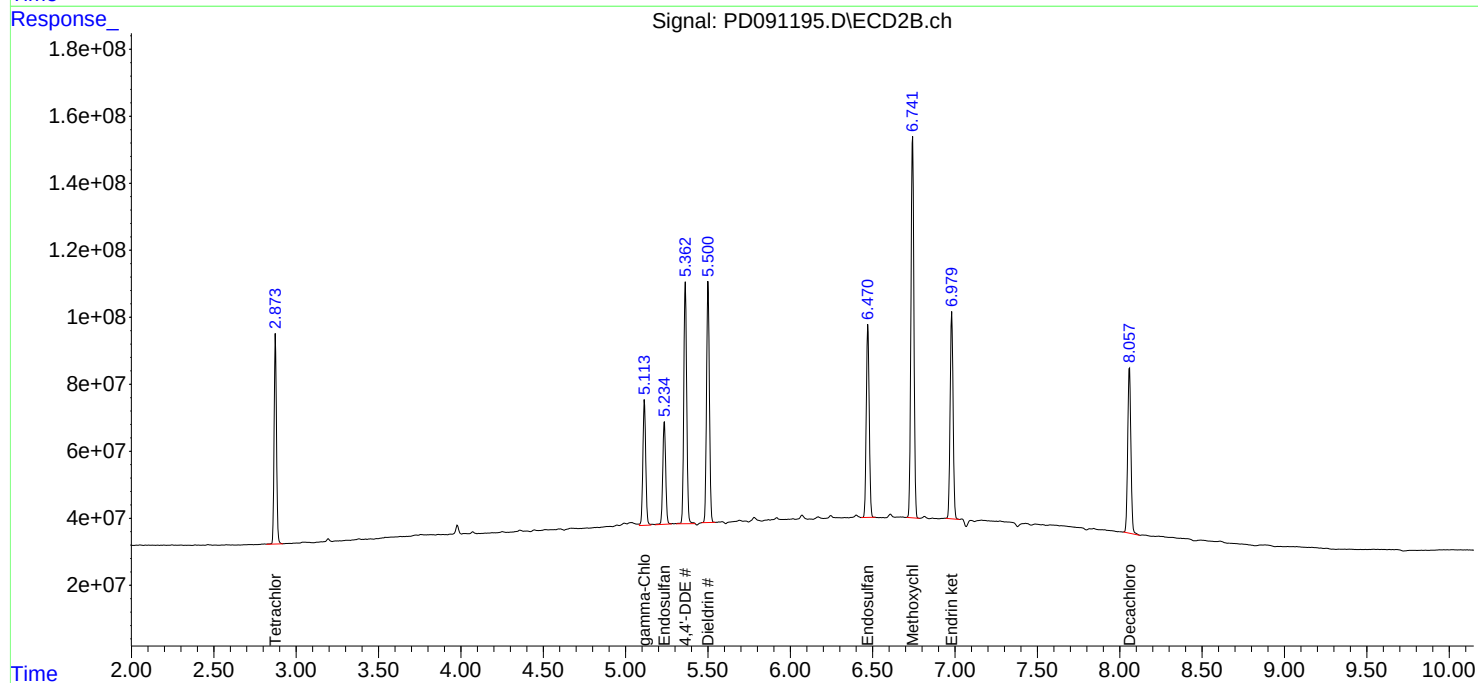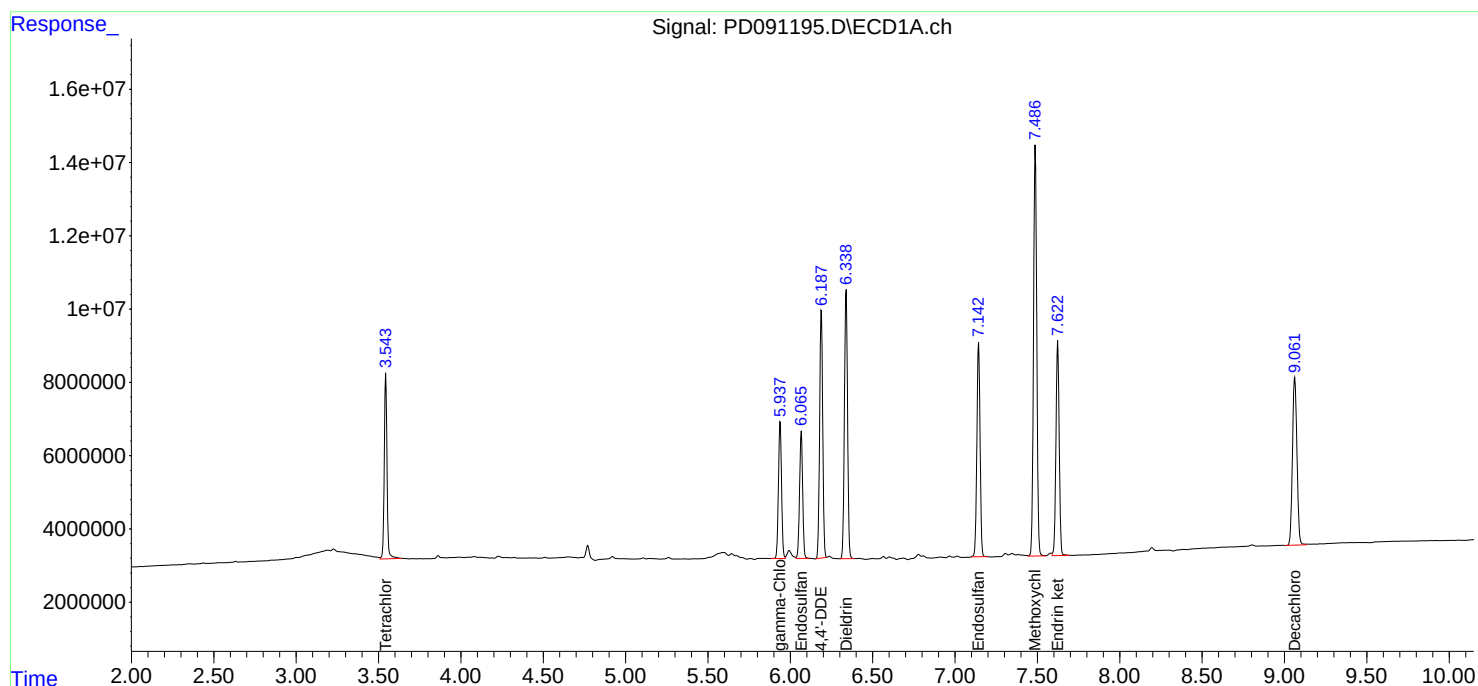


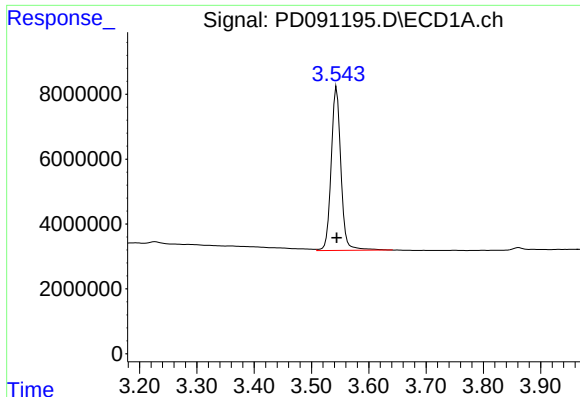

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 59572378
Conc: 17.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

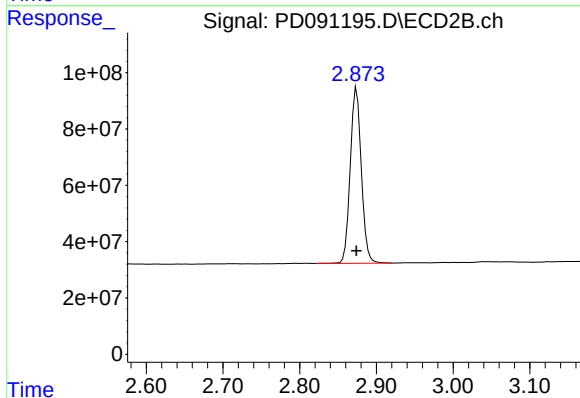


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.000 min
Response: 631860227
Conc: 17.25 ng/ml

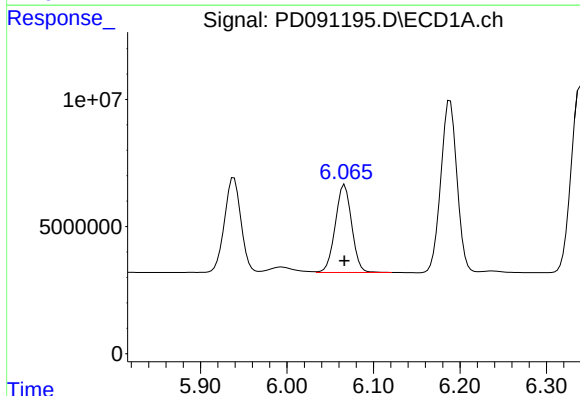


#9 Endosulfan I

R.T.: 6.067 min
Delta R.T.: 0.000 min
Response: 45261732
Conc: 7.37 ng/ml

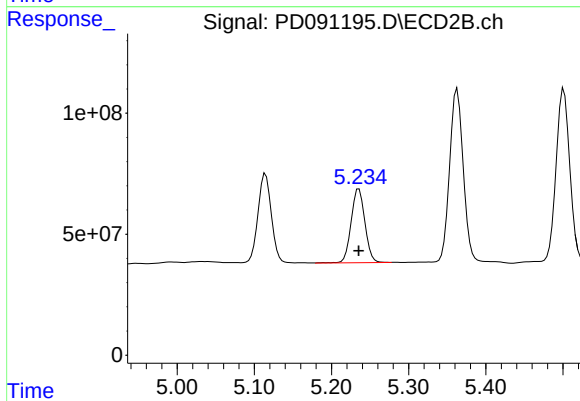

#9 Endosulfan I


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 379655336
Conc: 7.93 ng/ml

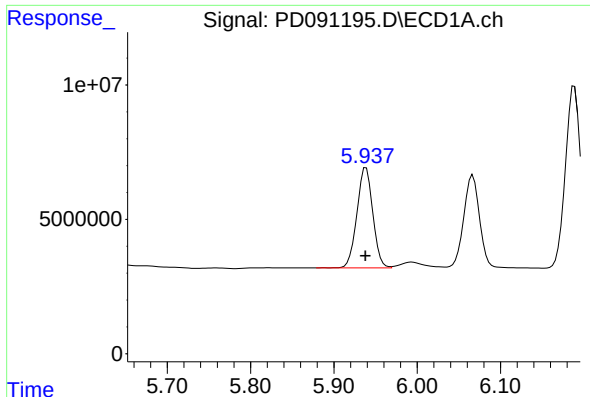

#10 gamma-Chlordane


R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 49362700
Conc: 7.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

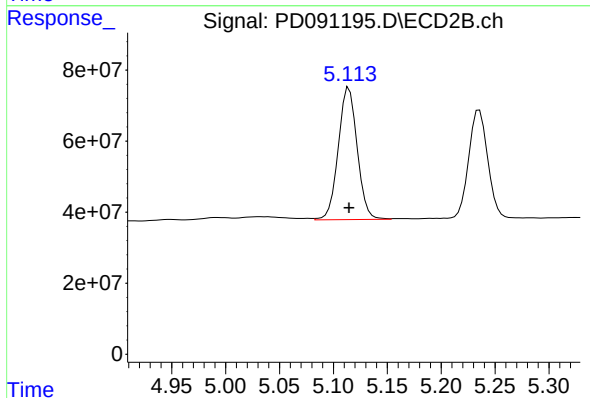


#10 gamma-Chlordane

R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 455800863
Conc: 8.34 ng/ml

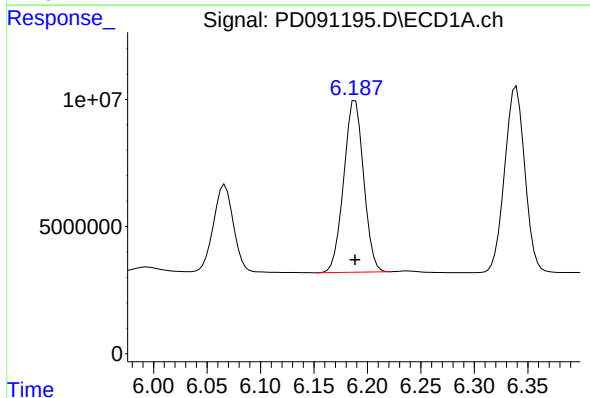


#12 4,4'-DDE

R.T.: 6.189 min
Delta R.T.: 0.000 min
Response: 87544052
Conc: 15.10 ng/ml

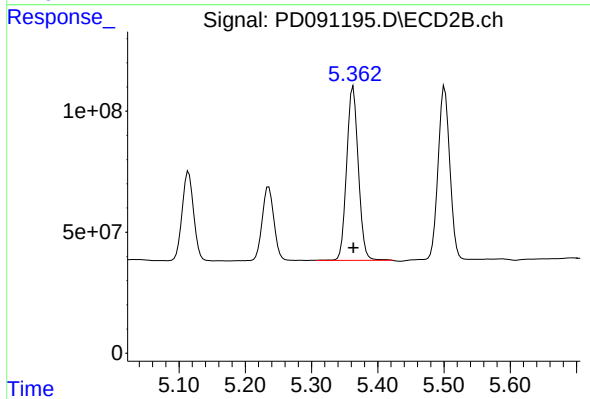

#12 4,4'-DDE


R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 881304034
Conc: 16.49 ng/ml

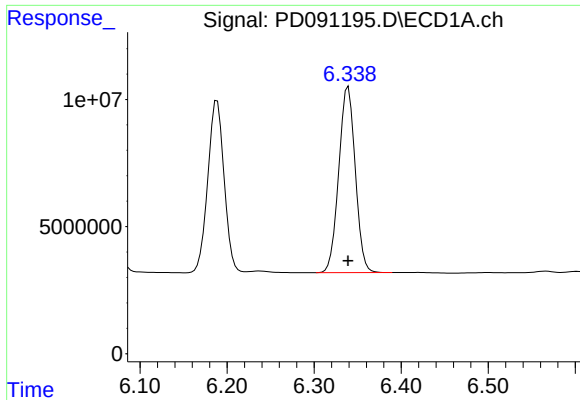

#13 Dieldrin


R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 96362551
Conc: 14.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

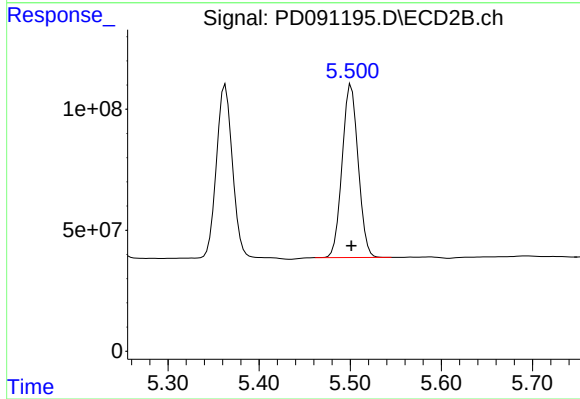


#13 Dieldrin

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 874407628
Conc: 16.10 ng/ml

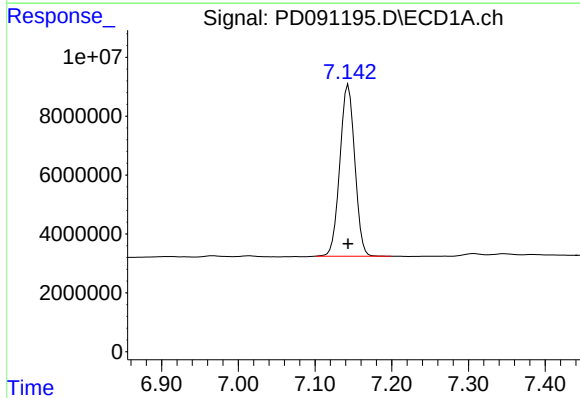


#19 Endosulfan Sulfate

R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 78876117
Conc: 15.33 ng/ml

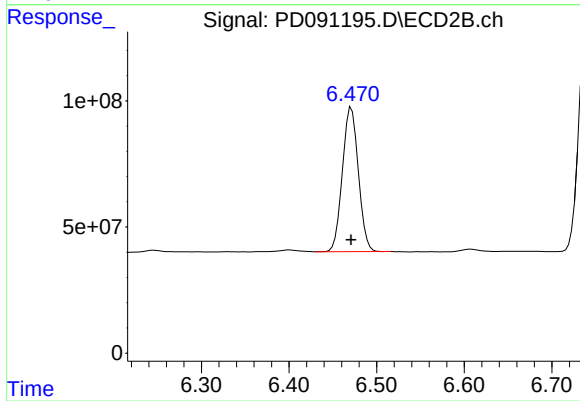

#19 Endosulfan Sulfate


R.T.: 6.471 min
Delta R.T.: 0.000 min
Response: 723362615
Conc: 16.13 ng/ml

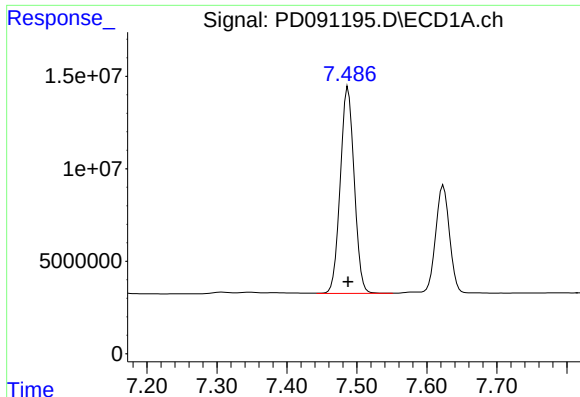

#20 Methoxychlor


R.T.: 7.487 min
Delta R.T.: 0.000 min
Response: 154485200
Conc: 71.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

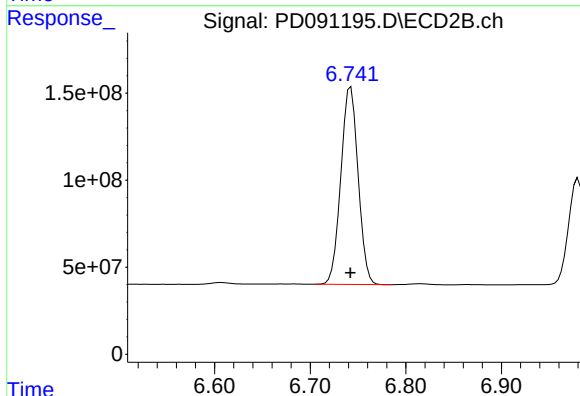


#20 Methoxychlor

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 1426049974
Conc: 71.12 ng/ml

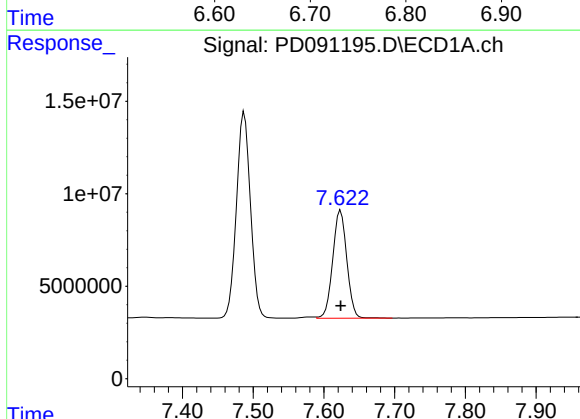


#21 Endrin ketone

R.T.: 7.624 min
Delta R.T.: 0.000 min
Response: 80568543
Conc: 14.30 ng/ml

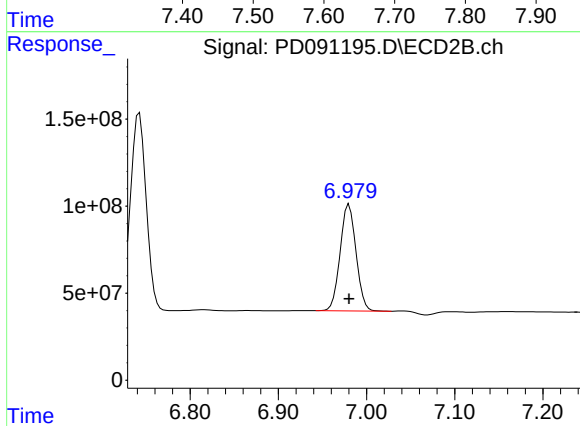

#21 Endrin ketone


R.T.: 6.980 min
Delta R.T.: 0.000 min
Response: 766525567
Conc: 15.04 ng/ml

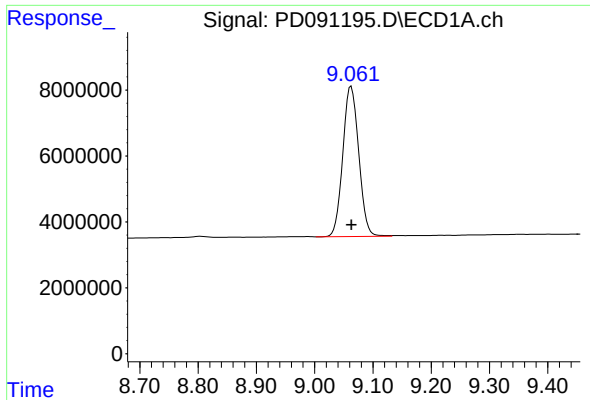

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.000 min
Response: 86552368
Conc: 17.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

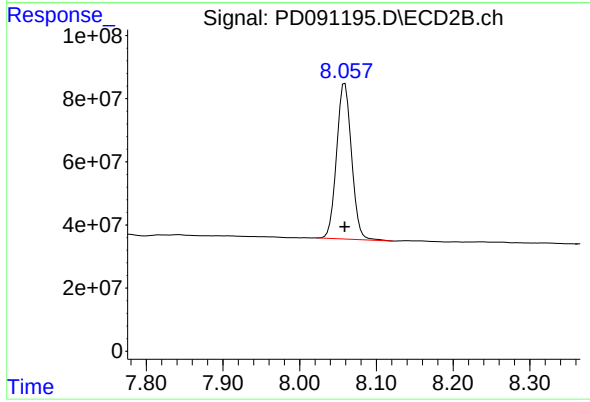

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: 0.000 min
Response: 667574884
Conc: 16.87 ng/ml