

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111525\
 Data File : PD091203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2025 22:32
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 04:29:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:28:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.873	143.9E6	1902.7E6	50.000	50.000
28)	SA Decachlor...	9.063	8.058	209.3E6	1703.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.707	3.896	113.3E6	788.6E6	500.000	500.000
24)	Chlordane-2	5.233	4.476	110.4E6	798.4E6	500.000	500.000
25)	Chlordane-3	5.939	5.114	448.7E6	2625.7E6	500.000	500.000
26)	Chlordane-4	6.024	5.178	539.1E6	2177.3E6	500.000	500.000
27)	Chlordane-5	6.864	6.078	88781325	938.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111525\
Data File : PD091203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2025 22:32
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 04:29:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:28:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

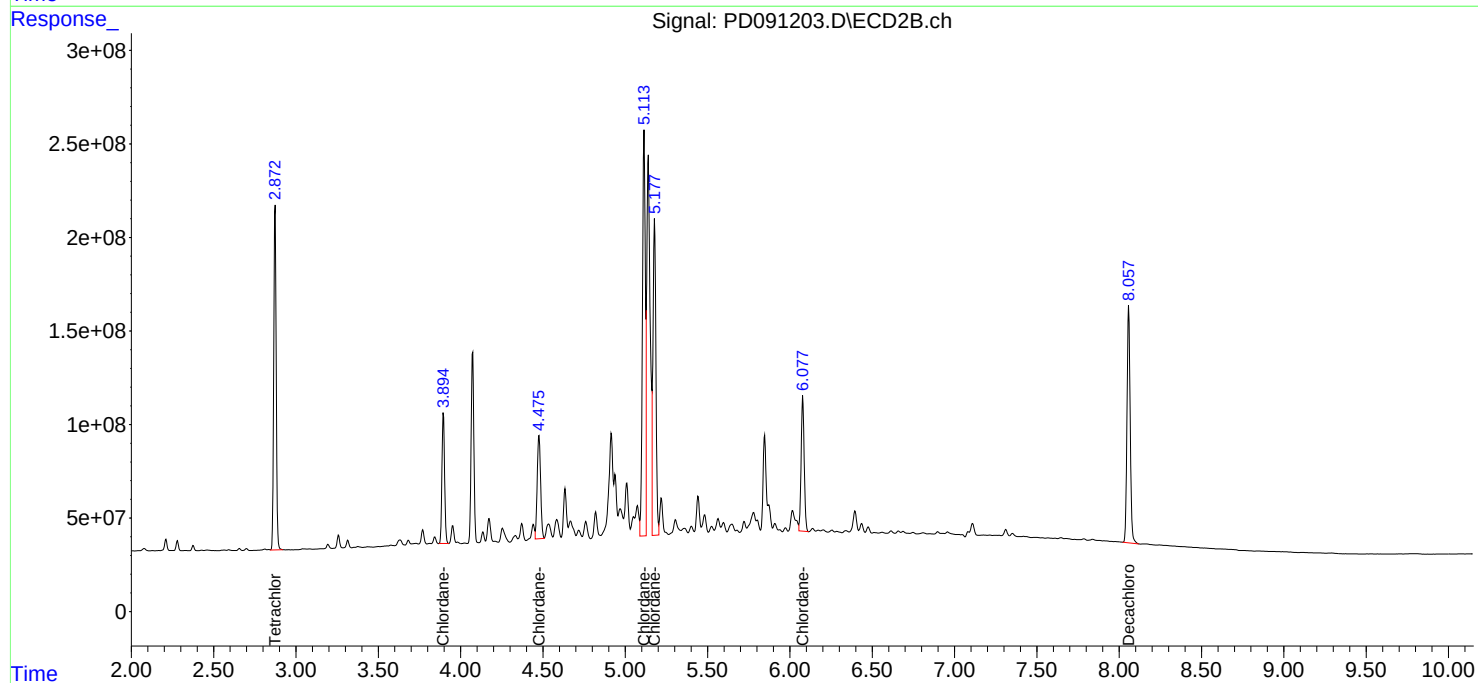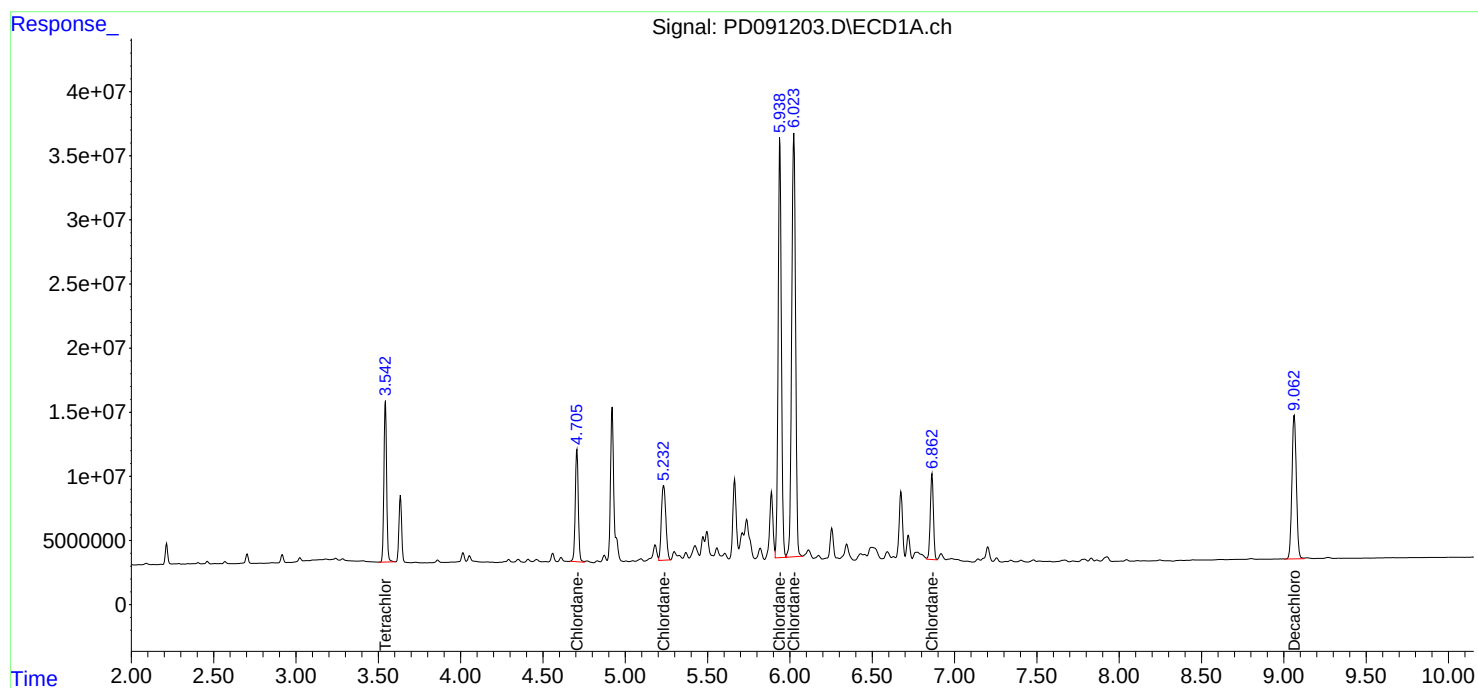


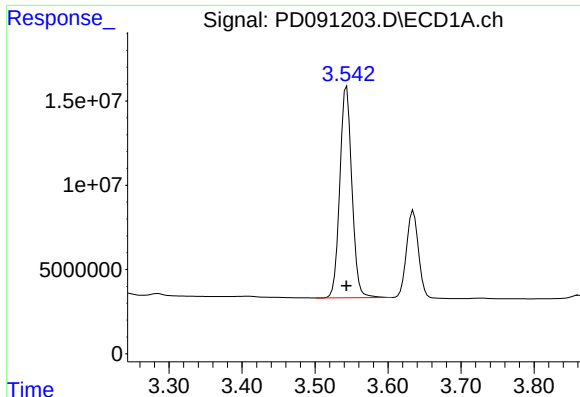

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 143891190
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

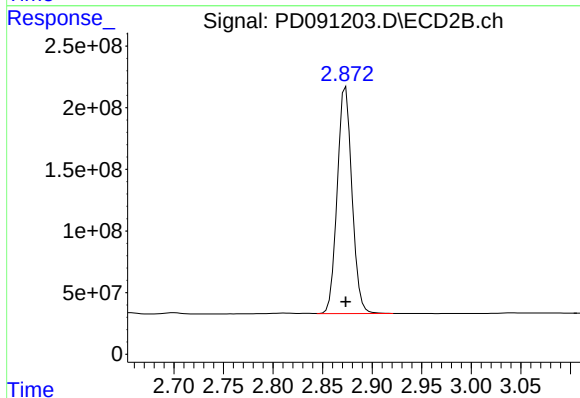


#1 Tetrachloro-m-xylene

R.T.: 2.873 min
Delta R.T.: 0.000 min
Response: 1902723643
Conc: 50.00 ng/ml

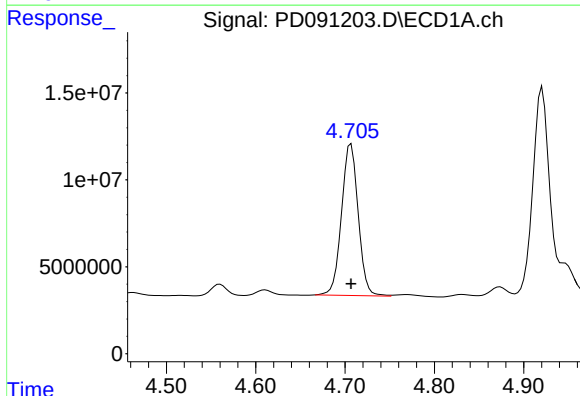


#23 Chlordane-1

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 113279394
Conc: 500.00 ng/ml

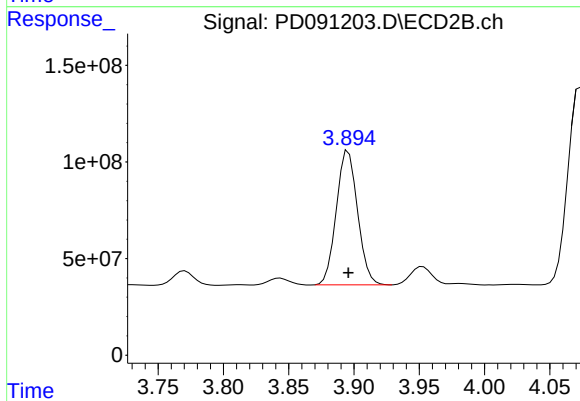

#23 Chlordane-1


R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 788566505
Conc: 500.00 ng/ml

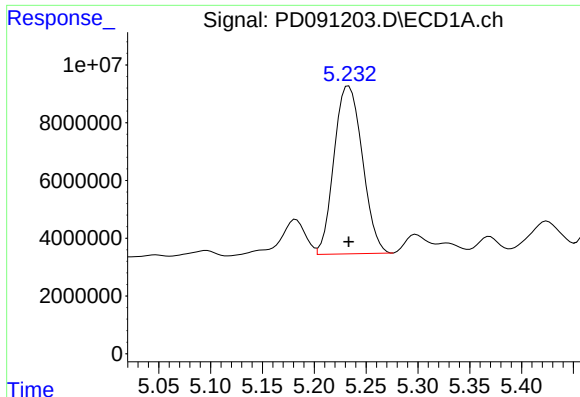

#24 Chlordane-2


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 110418770
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

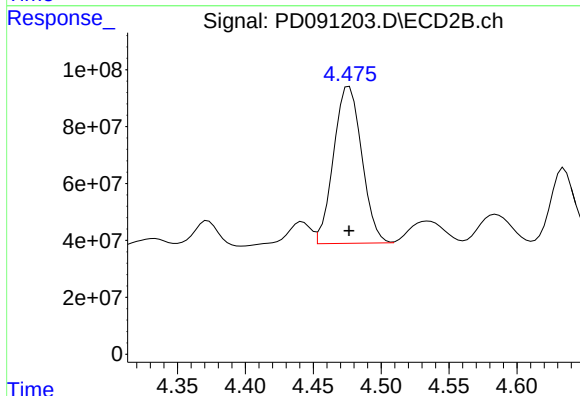


#24 Chlordane-2

R.T.: 4.476 min
Delta R.T.: 0.000 min
Response: 798417588
Conc: 500.00 ng/ml

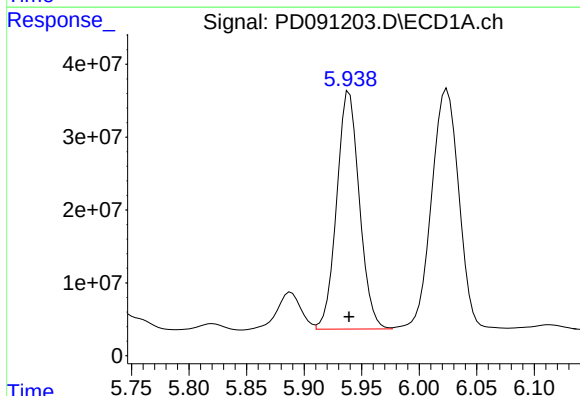


#25 Chlordane-3

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 448703112
Conc: 500.00 ng/ml

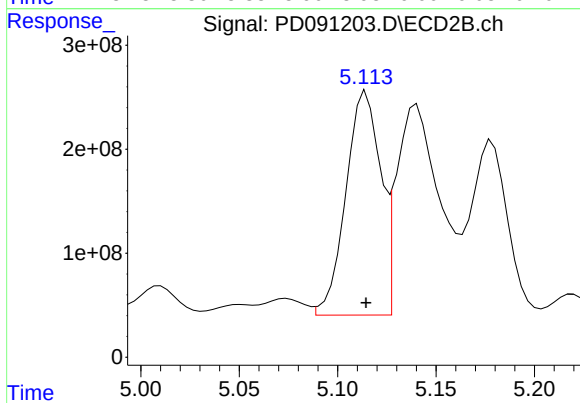

#25 Chlordane-3


R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 2625722277
Conc: 500.00 ng/ml

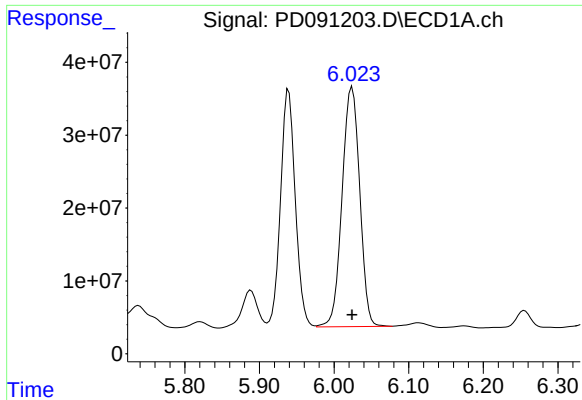

#26 Chlordane-4


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 539101822
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

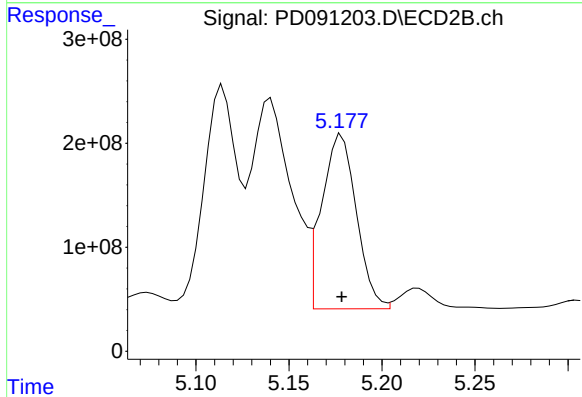


#26 Chlordane-4

R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 2177257914
Conc: 500.00 ng/ml

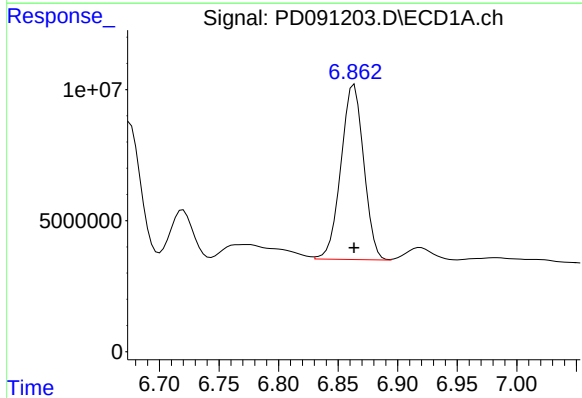


#27 Chlordane-5

R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 88781325
Conc: 500.00 ng/ml

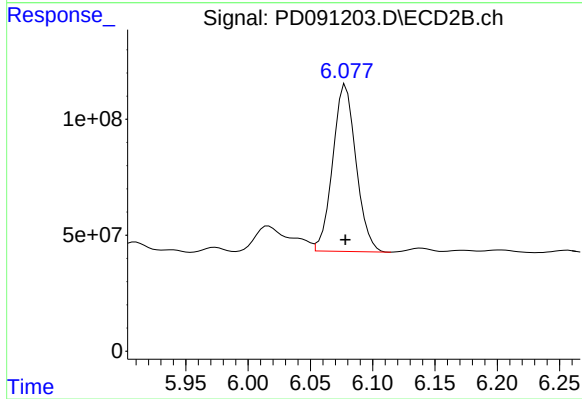

#27 Chlordane-5

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 938395073
Conc: 500.00 ng/ml

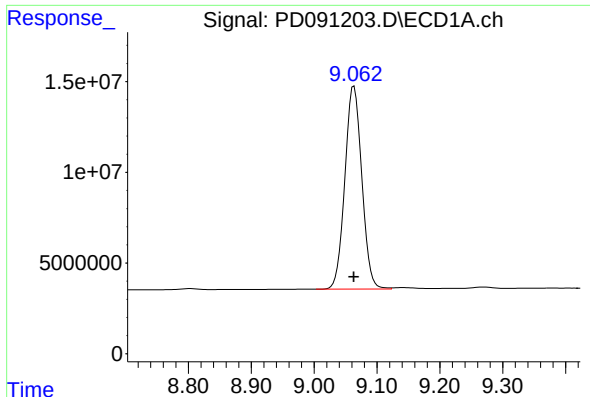

#28 Decachlorobiphenyl


R.T.: 9.063 min

Delta R.T.: 0.000 min

Response: 209287182

Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

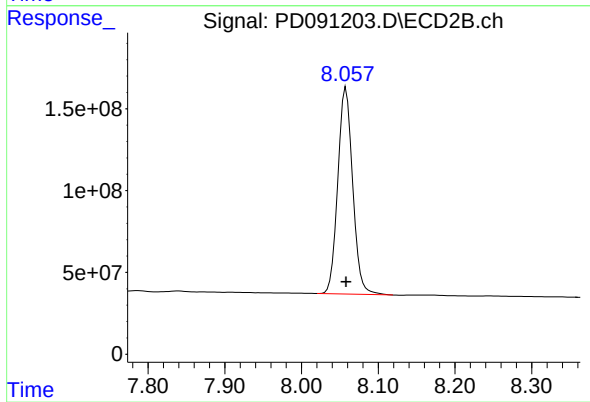

#28 Decachlorobiphenyl

R.T.: 8.058 min

Delta R.T.: 0.000 min

Response: 1703523968

Conc: 50.00 ng/ml