

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112025\
 Data File : PD091303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2025 11:26
 Operator : AR\AJ
 Sample : PB170629BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB170629BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 22:44:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:46:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.870	61683845	836.8E6	17.886	22.844 #
28)	SA Decachlor...	9.068	8.057	92274331	772.5E6	18.522	19.519
Target Compounds							
23)	Chlordane-1	4.711	3.893	47149781	350.9E6	191.621	203.962
24)	Chlordane-2	5.238	4.474	51853893	359.7E6	209.994	205.395
25)	Chlordane-3	5.943	5.112	182.7E6	1213.5E6	189.389	210.911
26)	Chlordane-4	6.028	5.177	223.1E6	1038.8E6	185.730	217.166
27)	Chlordane-5	6.868	6.076	35958475	474.5E6	182.002	233.836 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112025\
Data File : PD091303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2025 11:26
Operator : AR\AJ
Sample : PB170629BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB170629BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 22:44:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:46:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

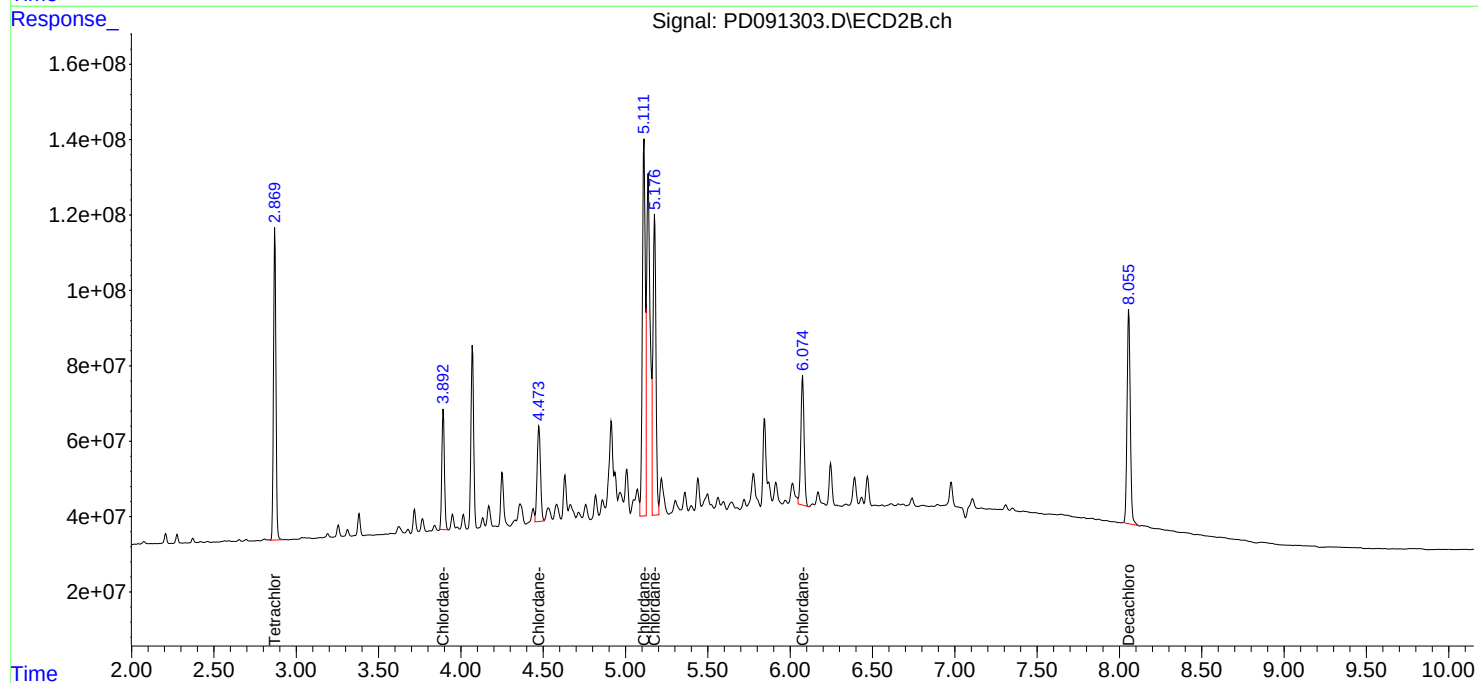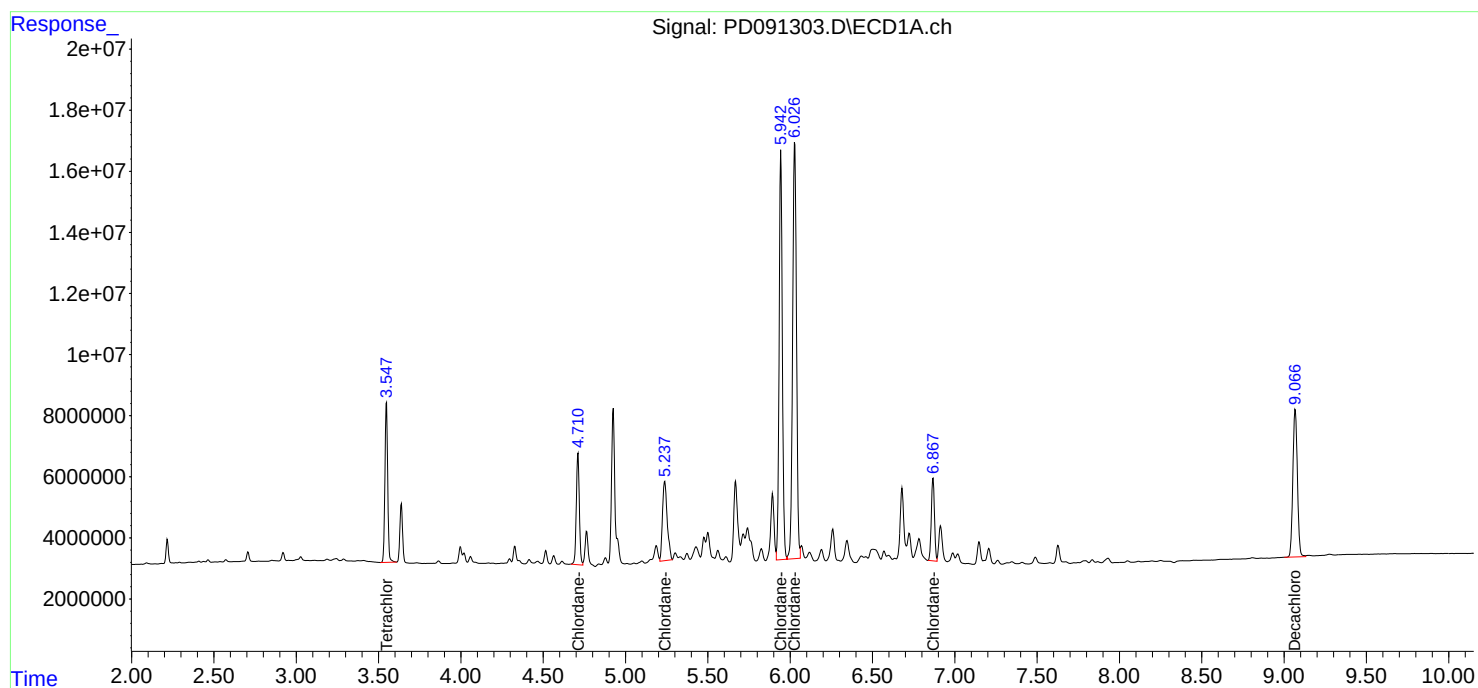


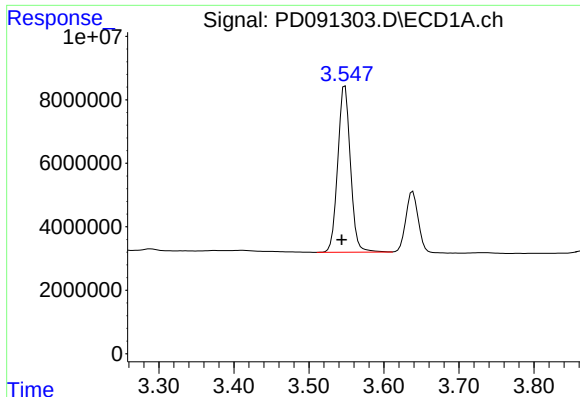

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.004 min
Response: 61683845
Conc: 17.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB170629BS

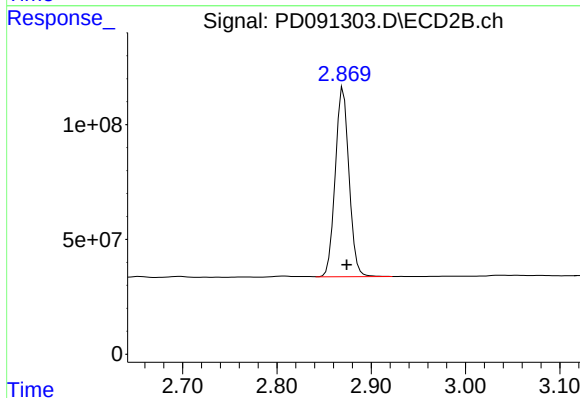


#1 Tetrachloro-m-xylene

R.T.: 2.870 min
Delta R.T.: -0.004 min
Response: 836763826
Conc: 22.84 ng/ml

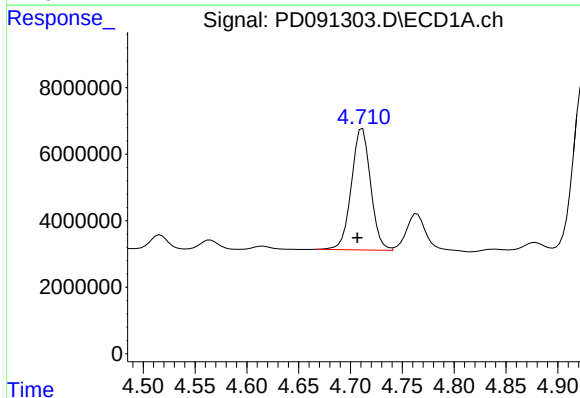


#23 Chlordane-1

R.T.: 4.711 min
Delta R.T.: 0.005 min
Response: 47149781
Conc: 191.62 ng/ml

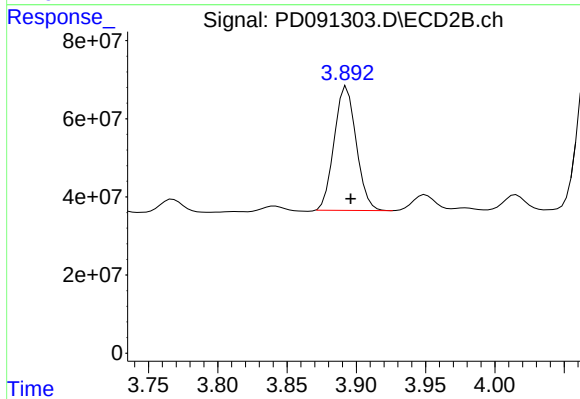

#23 Chlordane-1


R.T.: 3.893 min
Delta R.T.: -0.003 min
Response: 350874722
Conc: 203.96 ng/ml

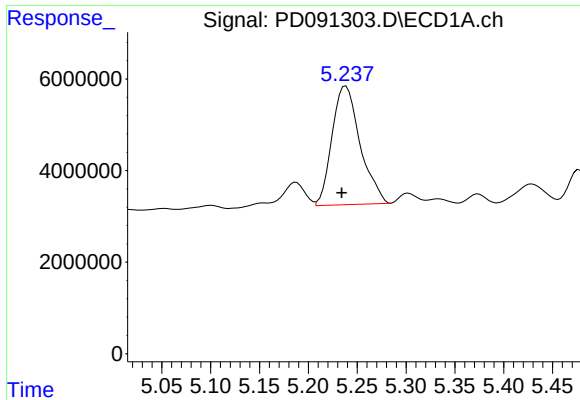

#24 Chlordane-2


R.T.: 5.238 min
Delta R.T.: 0.004 min
Response: 51853893
Conc: 209.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB170629BS

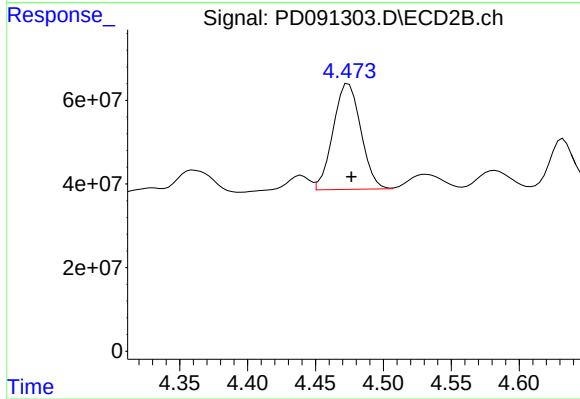


#24 Chlordane-2

R.T.: 4.474 min
Delta R.T.: -0.002 min
Response: 359654147
Conc: 205.40 ng/ml

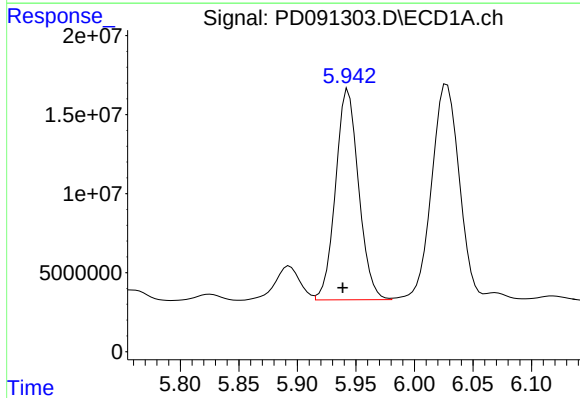


#25 Chlordane-3

R.T.: 5.943 min
Delta R.T.: 0.005 min
Response: 182730744
Conc: 189.39 ng/ml

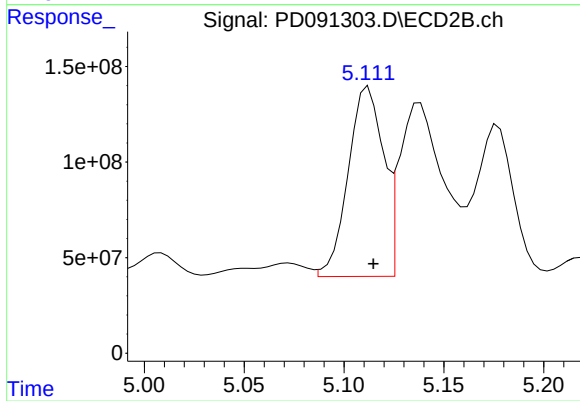

#25 Chlordane-3


R.T.: 5.112 min
Delta R.T.: -0.003 min
Response: 1213494313
Conc: 210.91 ng/ml

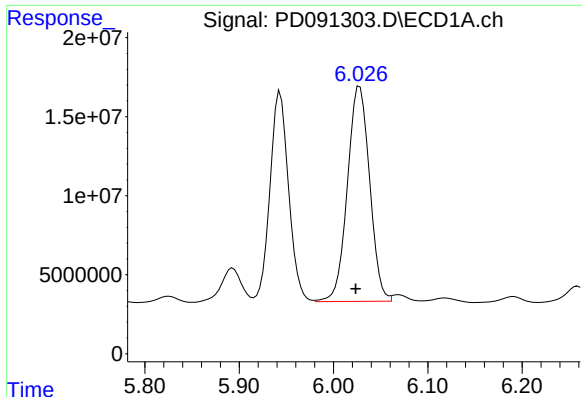

#26 Chlordane-4


R.T.: 6.028 min
Delta R.T.: 0.004 min
Response: 223099648
Conc: 185.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB170629BS

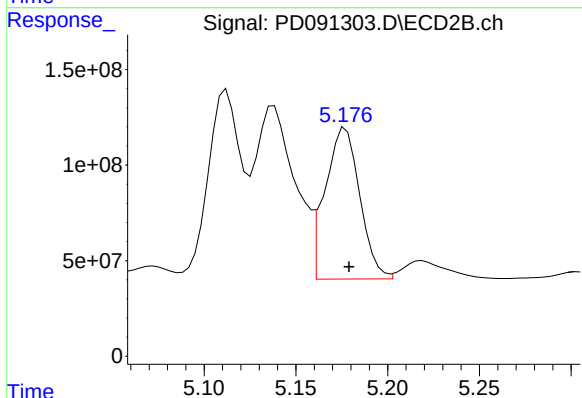


#26 Chlordane-4

R.T.: 5.177 min
Delta R.T.: -0.002 min
Response: 1038829484
Conc: 217.17 ng/ml

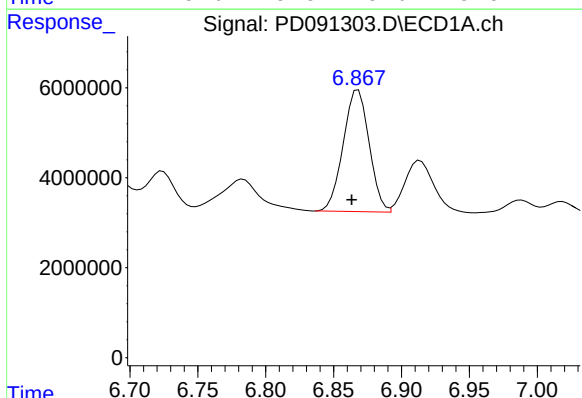


#27 Chlordane-5

R.T.: 6.868 min
Delta R.T.: 0.005 min
Response: 35958475
Conc: 182.00 ng/ml

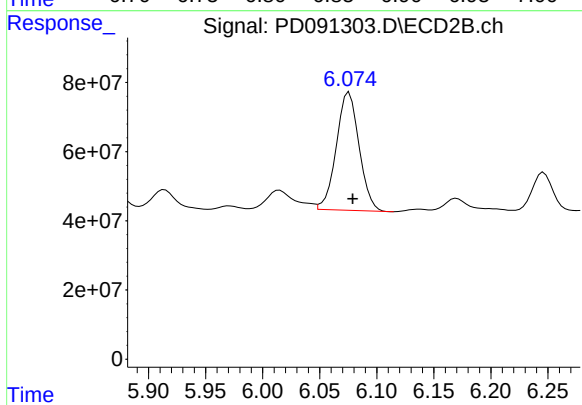

#27 Chlordane-5


R.T.: 6.076 min
Delta R.T.: -0.003 min
Response: 474500704
Conc: 233.84 ng/ml

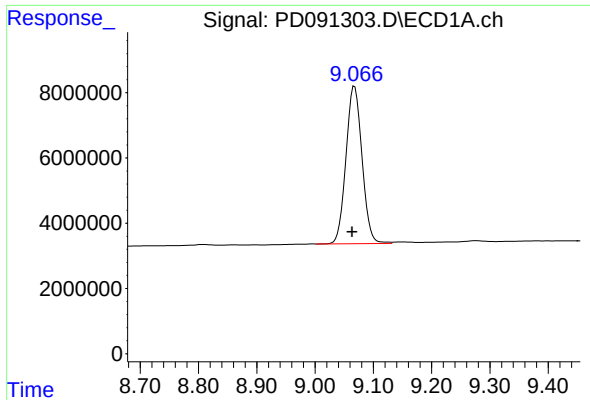

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: 0.004 min
Response: 92274331
Conc: 18.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB170629BS

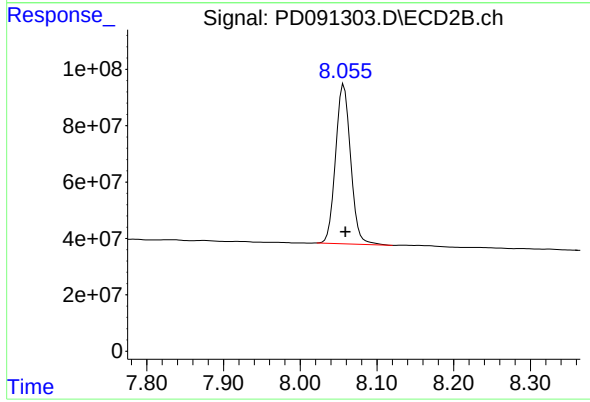

#28 Decachlorobiphenyl

R.T.: 8.057 min
Delta R.T.: -0.002 min
Response: 772466342
Conc: 19.52 ng/ml