


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
Data File : BG064798.D
Acq On : 18 Nov 2025 11:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

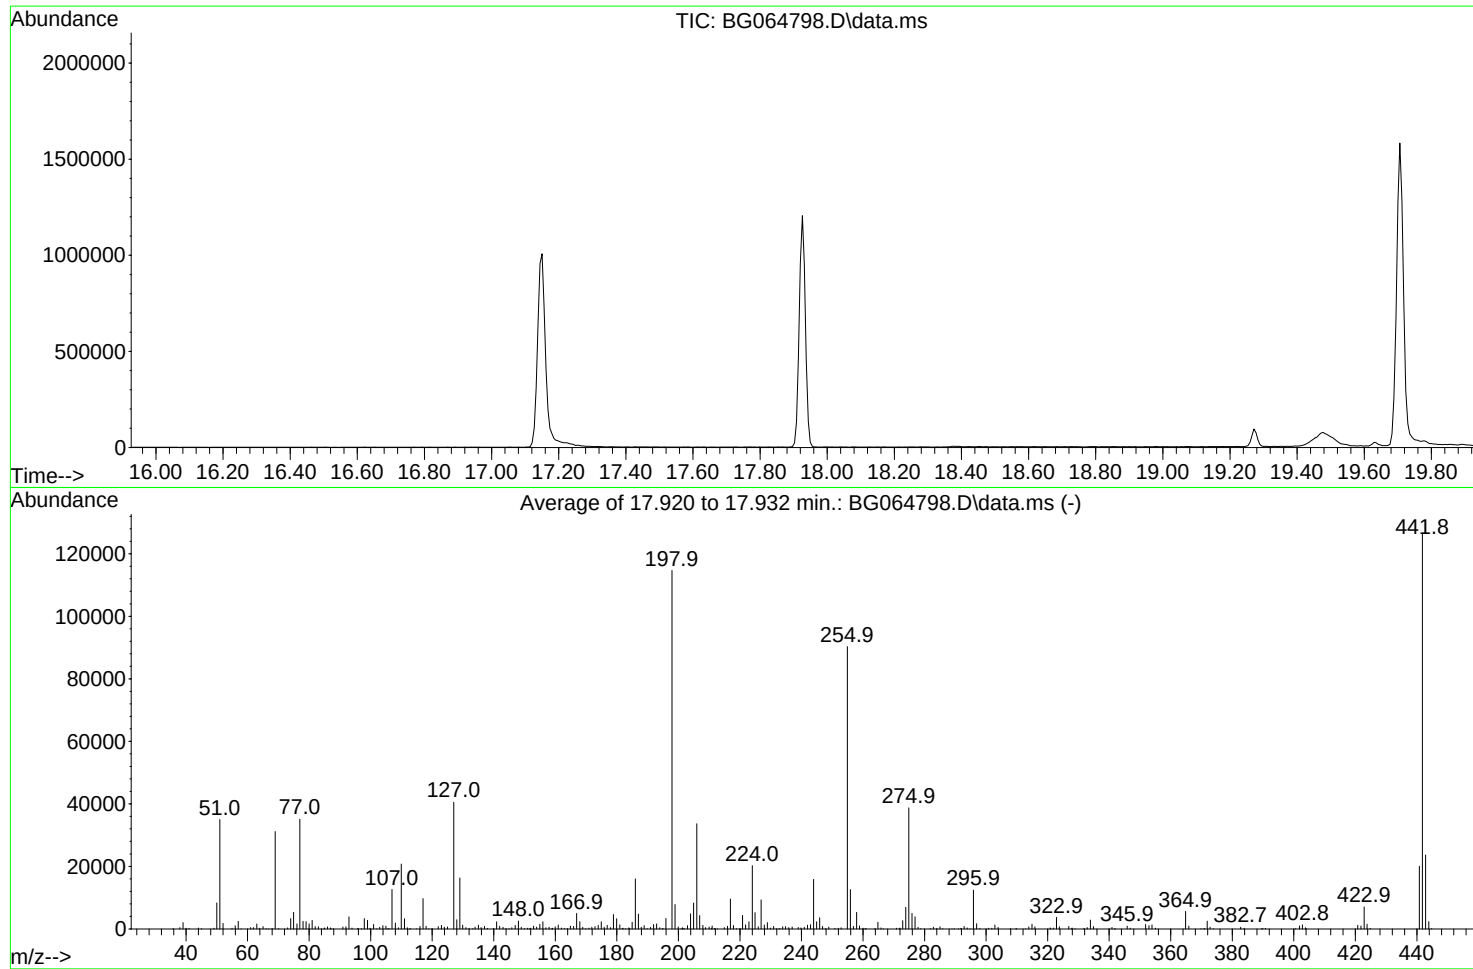




AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.6	179	PASS
69	69	100	100	100.0	31136	PASS
70	69	0.00	2	0.3	106	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	114677	PASS
199	198	5	9	6.8	7801	PASS
365	198	1	100	4.9	5614	PASS
441	443	0.01	150	84.8	20020	PASS
442	442	100	100	100.0	126304	PASS
443	442	15	24	18.7	23621	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
Data File : BG064798.D
Acq On : 18 Nov 2025 11:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 18 12:05:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

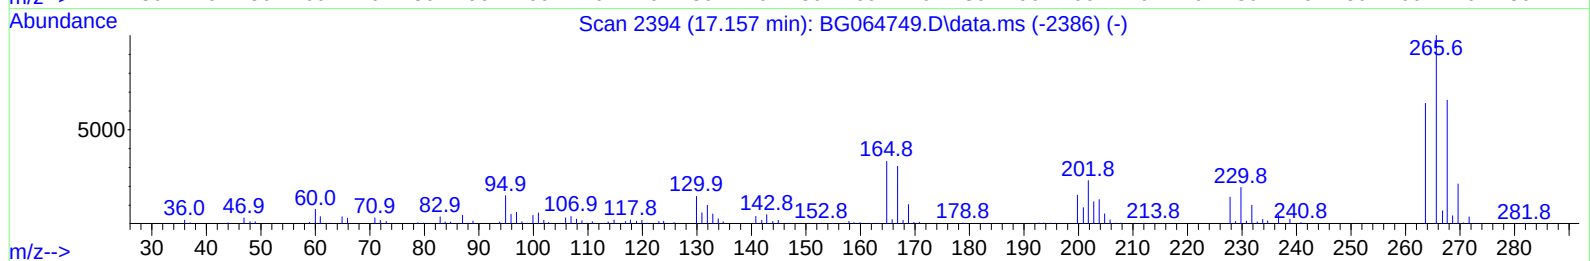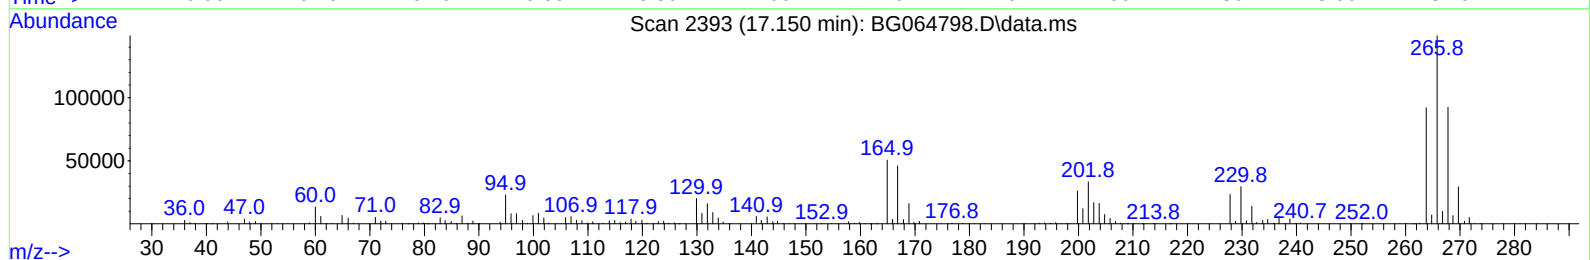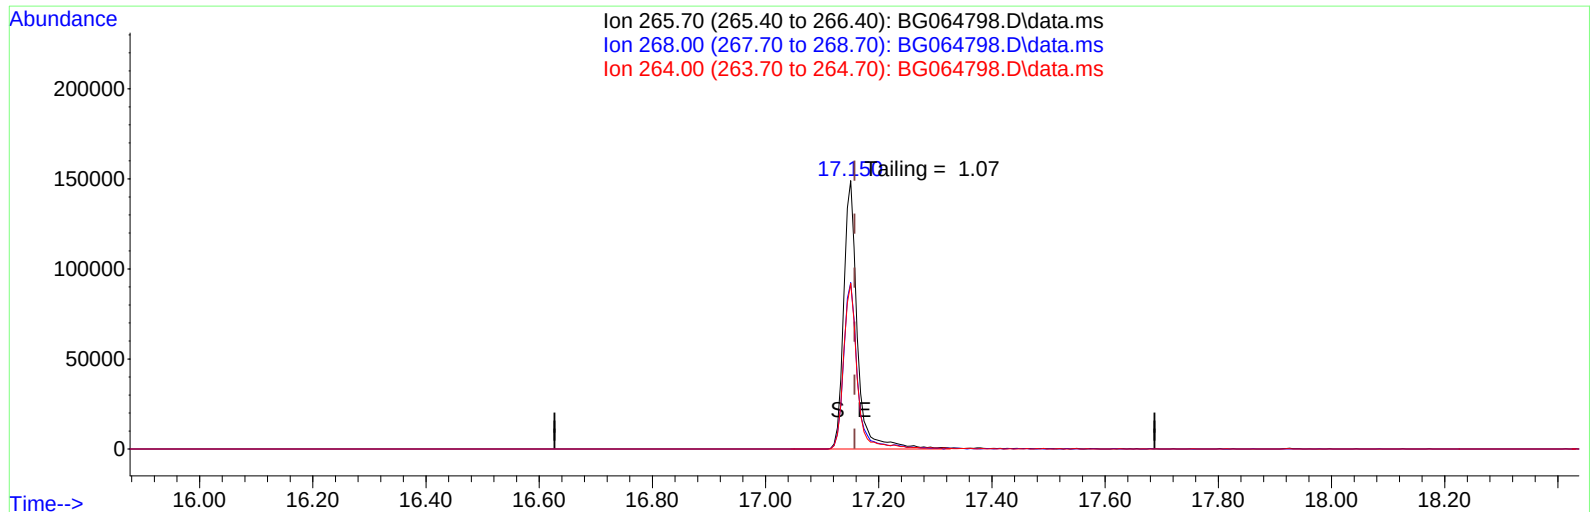

TIC: BG064798.D\data.ms

(70) Pentachlorophenol (C)

17.150min (-0.007) 33926.00 ng




response 250451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	66.50
264.00	64.00	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
Data File : BG064798.D
Acq On : 18 Nov 2025 11:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 18 12:05:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

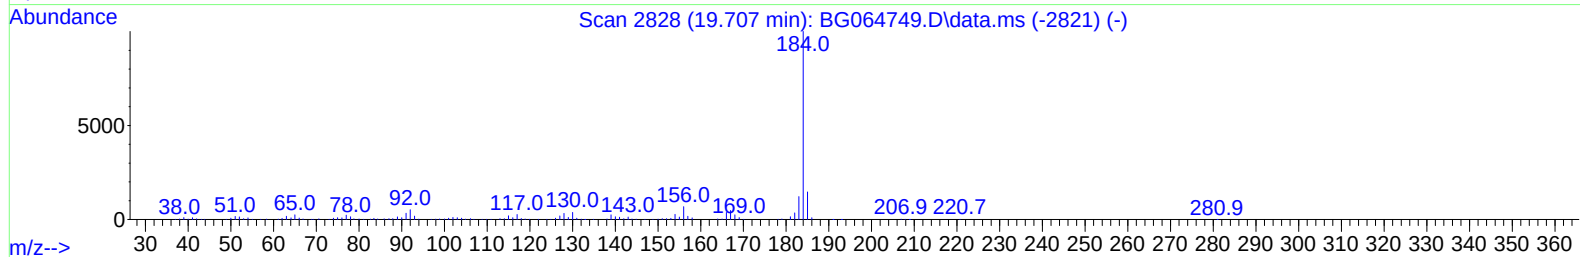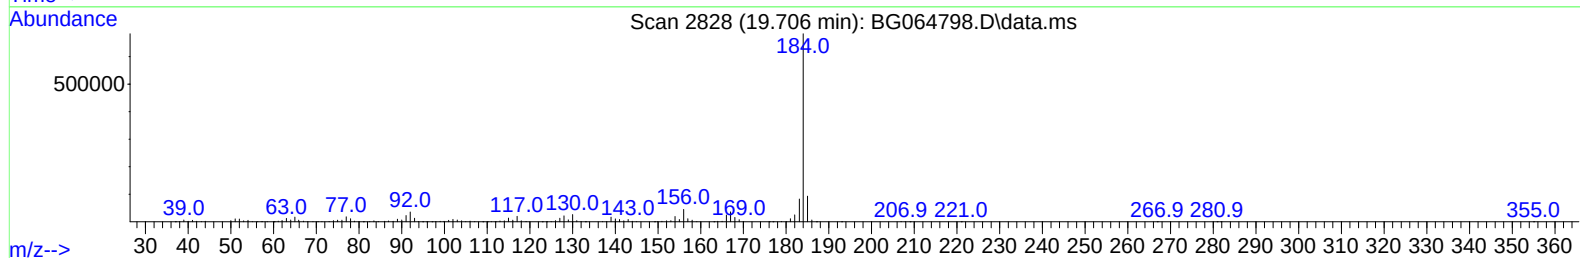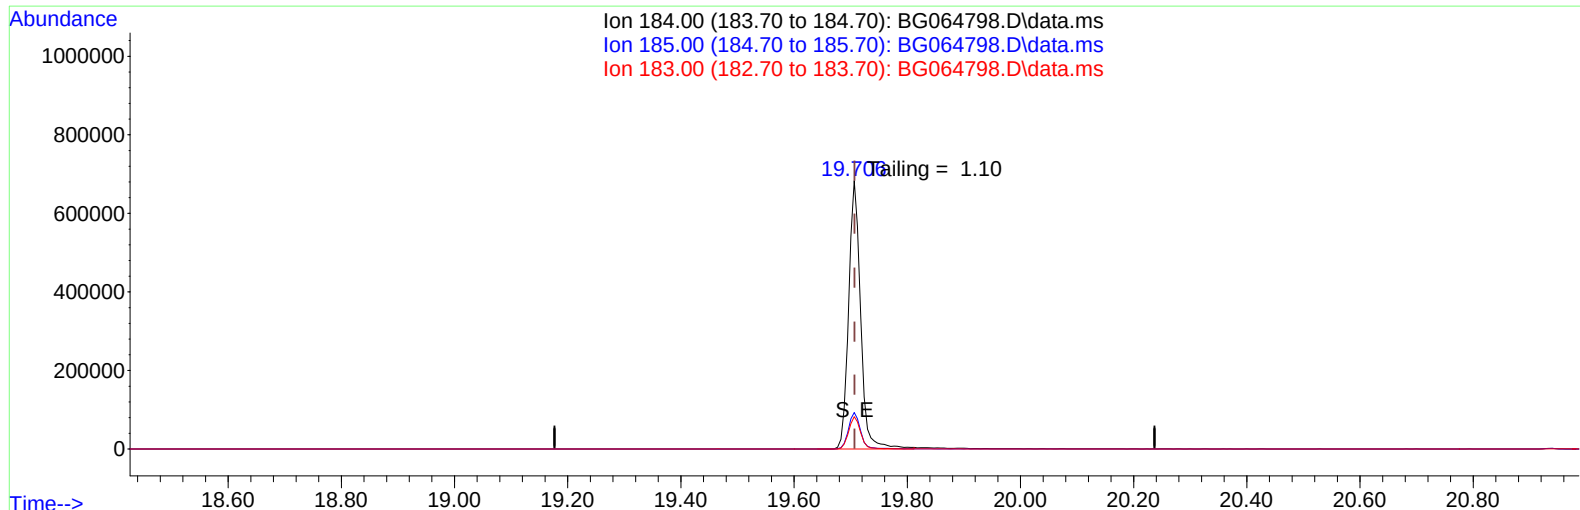

TIC: BG064798.D\data.ms

(77) Benzidine

19.706min (-0.000) 549166.45 ng

response 1019693

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.63
183.00	12.20	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/18/2025	BNA_G	<u>BG064798.D</u>
Compound Name	Response	Retention Time
DDT	621626	20.934
DDD	16049	20.494
DDE	1419	19.994
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17468	639094	2.73

Instrument :
BNA_G
ClientSampleId :
DFTPP