


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111825\
Data File : BP026142.D
Acq On : 18 Nov 2025 13:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

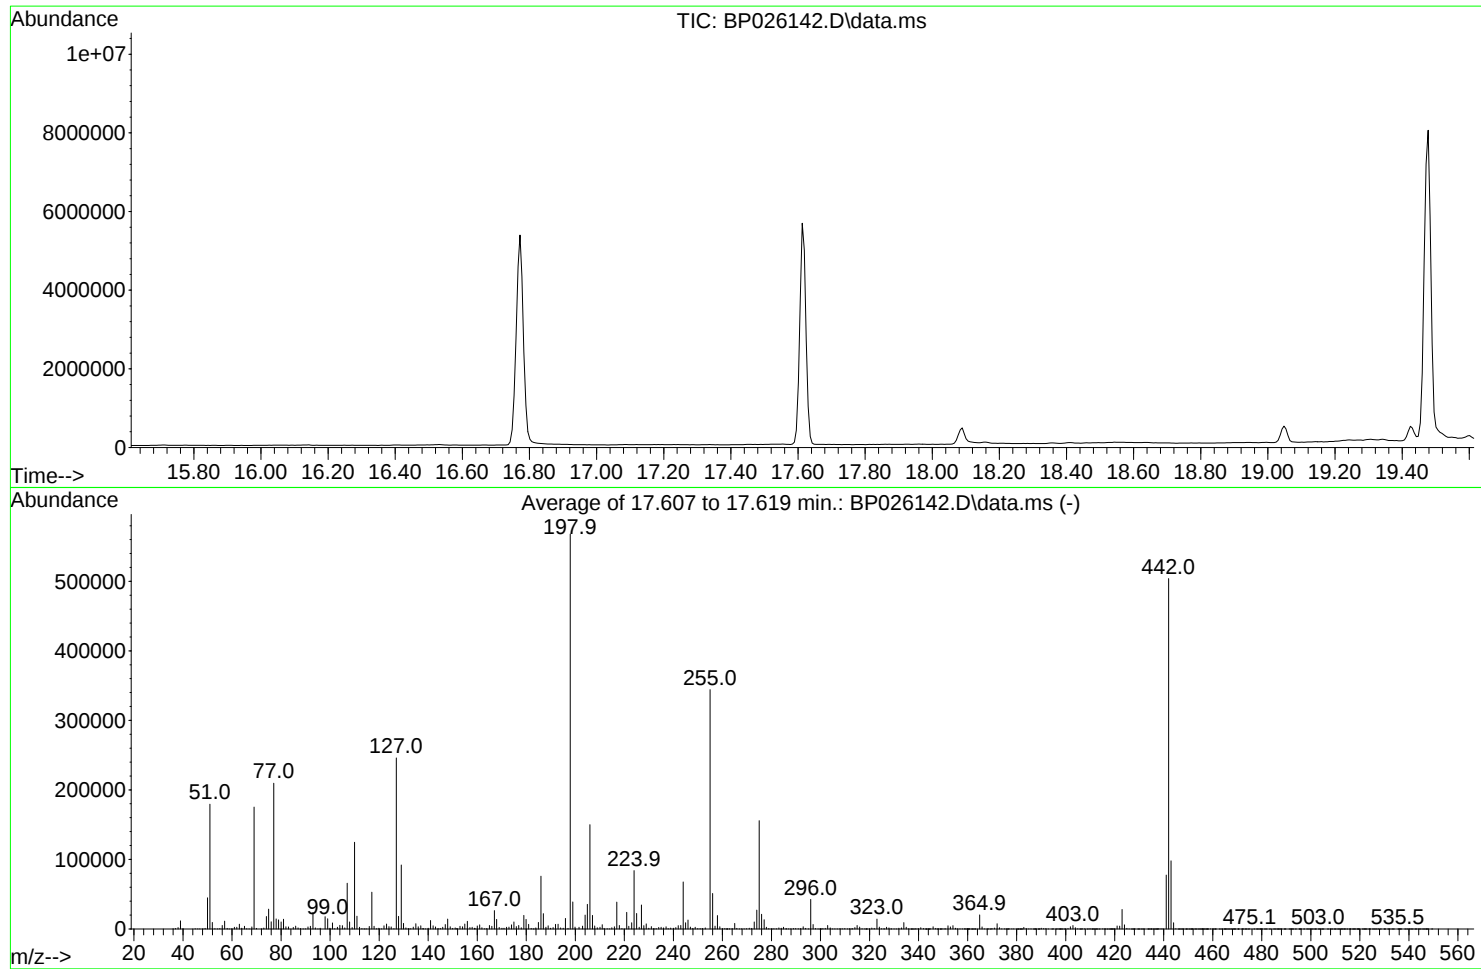




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2891	PASS
69	69	100	100	100.0	175261	PASS
70	69	0.00	2	0.4	730	PASS
197	198	0.00	2	0.1	748	PASS
198	198	100	100	100.0	567984	PASS
199	198	5	9	6.8	38899	PASS
365	198	1	100	3.6	20169	PASS
441	443	0.01	150	79.0	77420	PASS
442	442	100	100	100.0	503872	PASS
443	442	15	24	19.5	98037	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111825\
Data File : BP026142.D
Acq On : 18 Nov 2025 13:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 19 00:44:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 00:37:08 2025
Response via : Initial Calibration

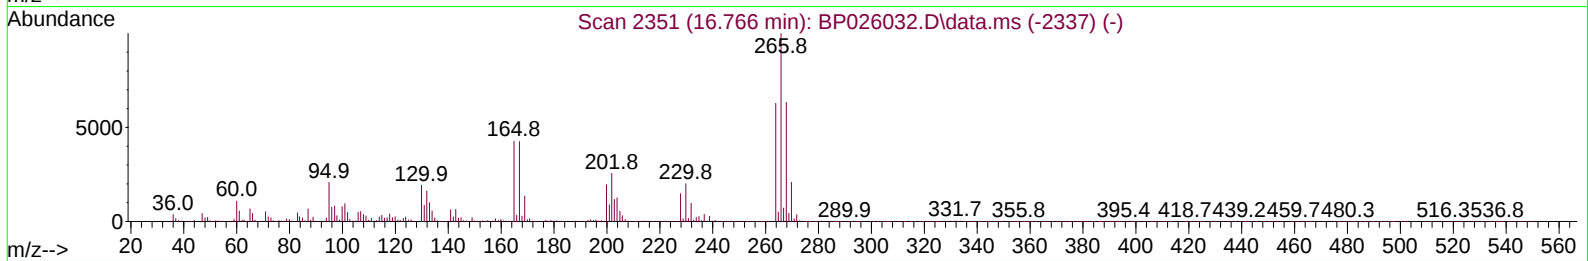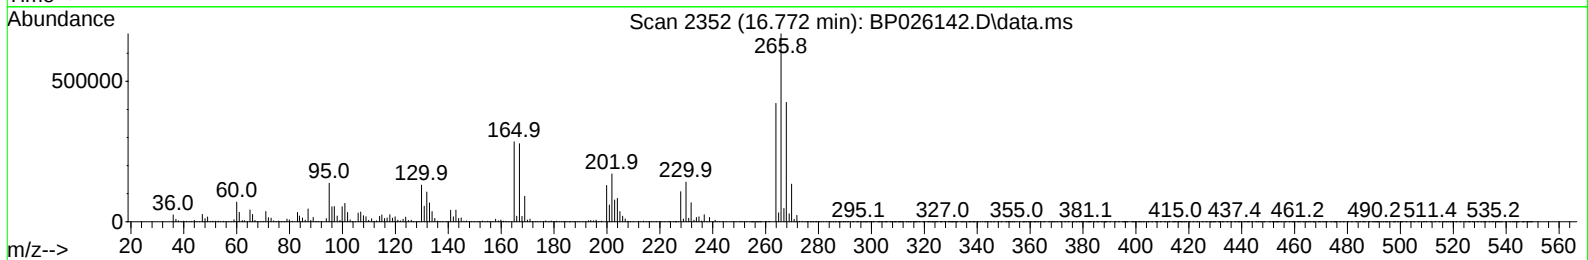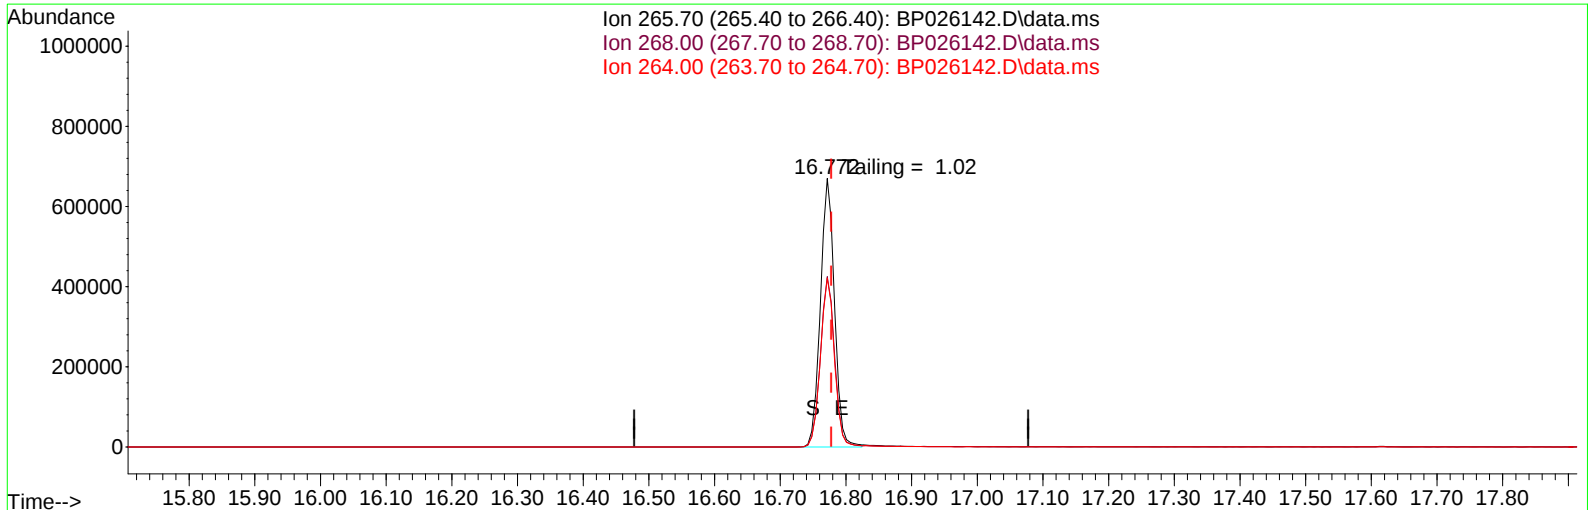

TIC: BP026142.D\data.ms

(70) Pentachlorophenol (C)

16.772min (-0.006) 1416102.53 ng




response 1013882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.49
264.00	62.70	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111825\
Data File : BP026142.D
Acq On : 18 Nov 2025 13:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 19 00:44:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 00:37:08 2025
Response via : Initial Calibration

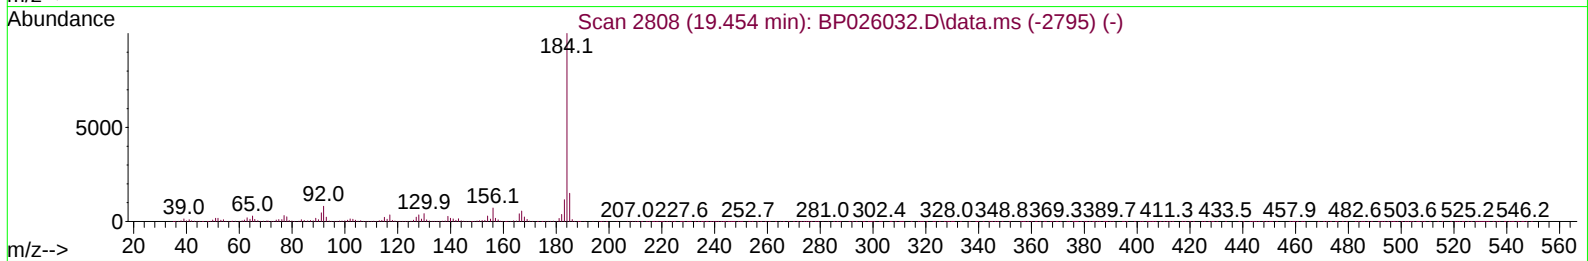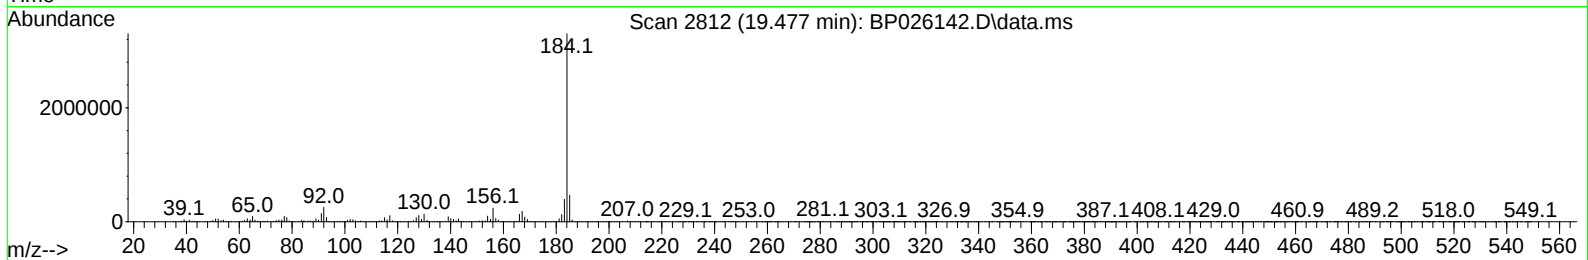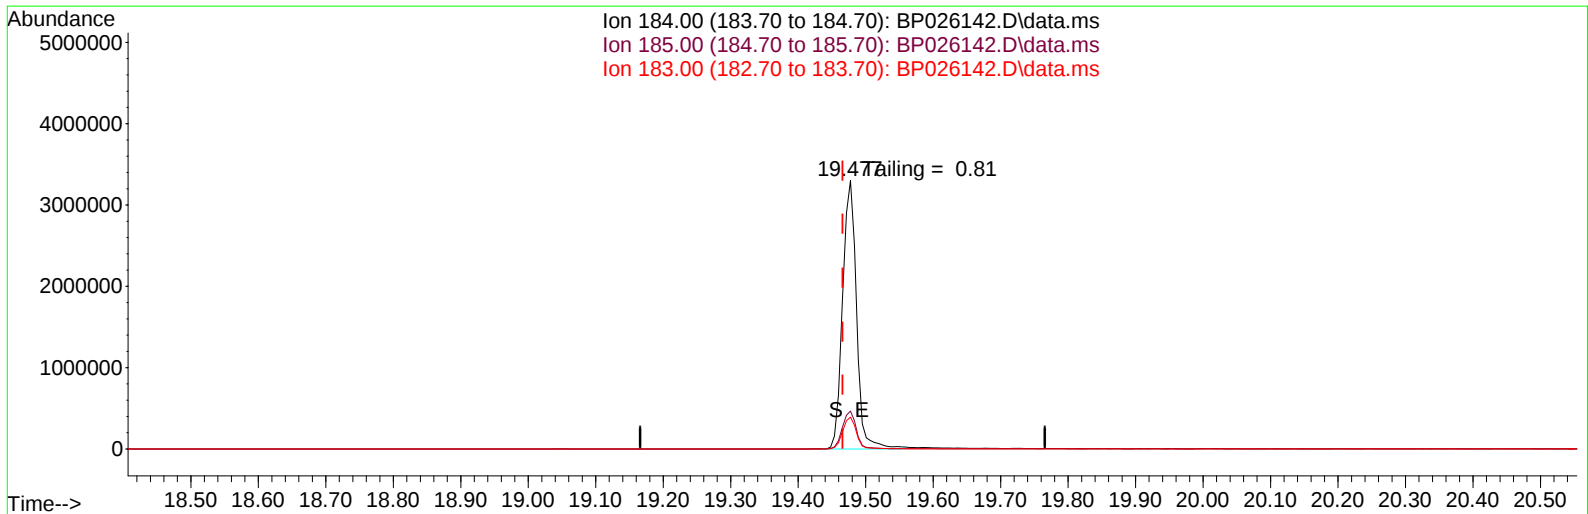

TIC: BP026142.D\data.ms

(77) Benzidine

19.477min (+ 0.012) 743702.57 ng

response 4726021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.13
183.00	11.30	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/18/2025	BNA_P	<u>BP026142.D</u>
Compound Name	Response	Retention Time
DDT	2472778	20.777
DDD	49260	20.377
DDE	4029	19.789
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53289	2526067	2.11

Instrument :
BNA_P
ClientSampleId :
DFTPP