


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112725\
Data File : BP026189.D
Acq On : 26 Nov 2025 13:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

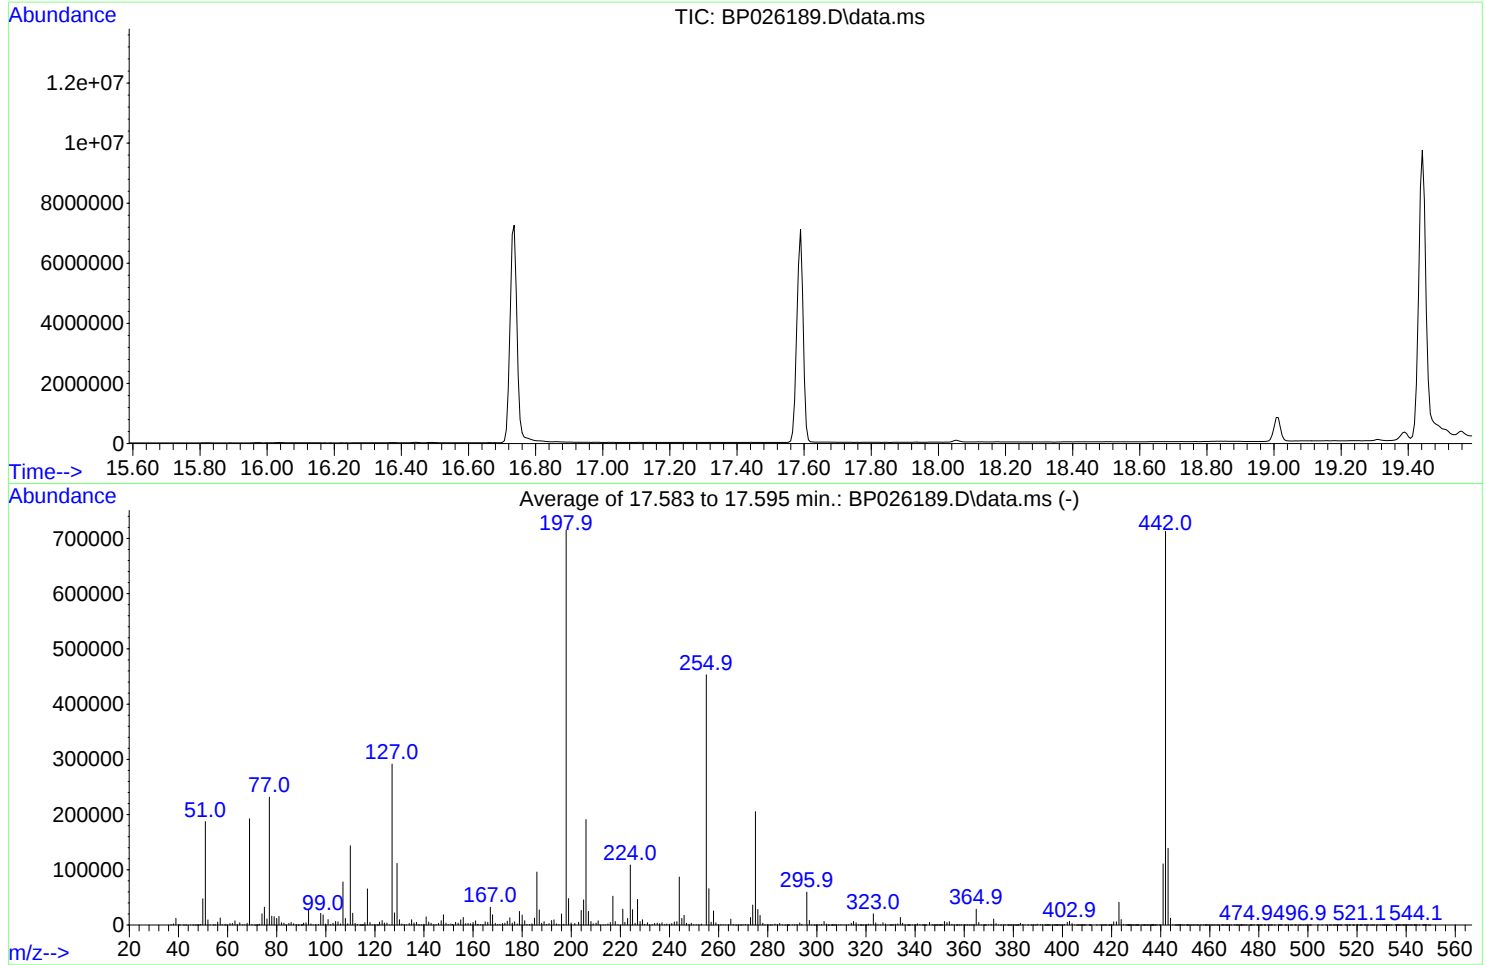

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	3227	PASS
69	69	100	100	100.0	192350	PASS
70	69	0.00	2	0.5	1041	PASS
197	198	0.00	2	0.2	1508	PASS
198	198	100	100	100.0	715009	PASS
199	198	5	9	6.7	47935	PASS
365	198	1	100	4.0	28789	PASS
441	443	0.01	150	79.7	110650	PASS
442	442	100	100	100.0	712930	PASS
443	442	15	24	19.5	138829	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/27/2025	BNA_P	<u>BP026189.D</u>
Compound Name	Response	Retention Time
DDT	3414858	20.742
DDD	40682	20.277
DDE	3383	19.754
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44065	3458923	1.27

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112725\
Data File : BP026189.D
Acq On : 26 Nov 2025 13:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 26 15:09:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

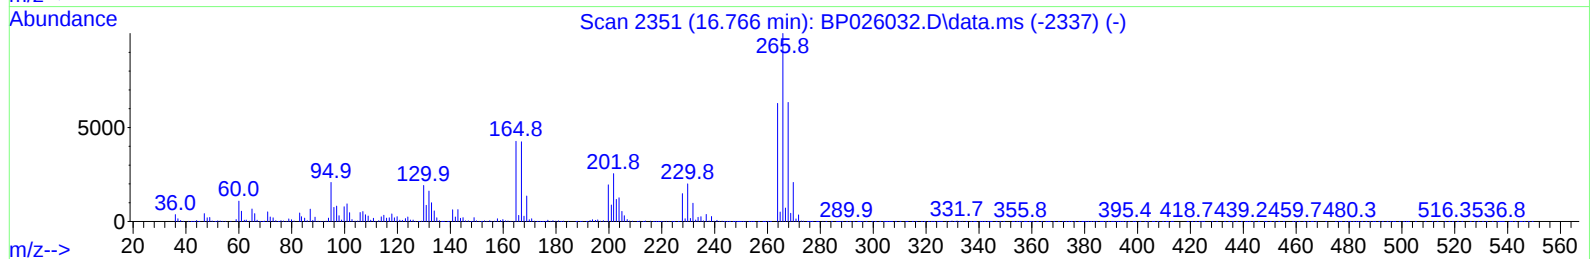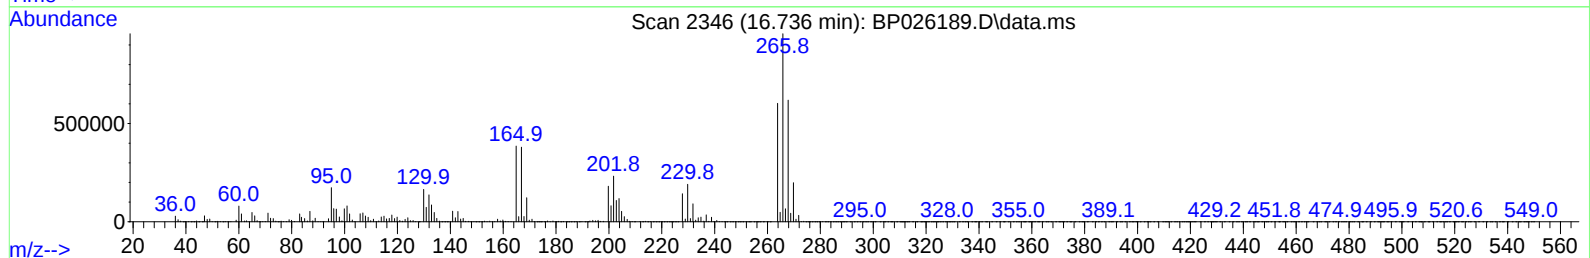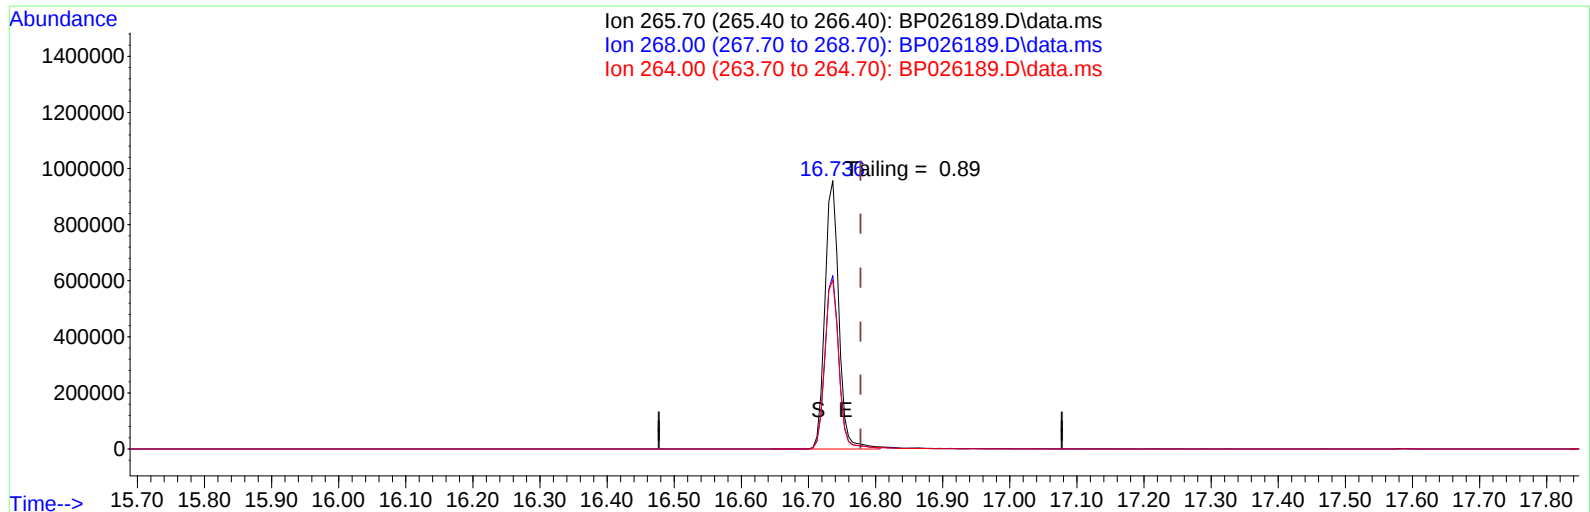

TIC: BP026189.D\data.ms

(70) Pentachlorophenol (C)

16.736min (-0.041) 64652.85 ng




response 1389037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.65
264.00	62.70	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112725\
Data File : BP026189.D
Acq On : 26 Nov 2025 13:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 26 15:09:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

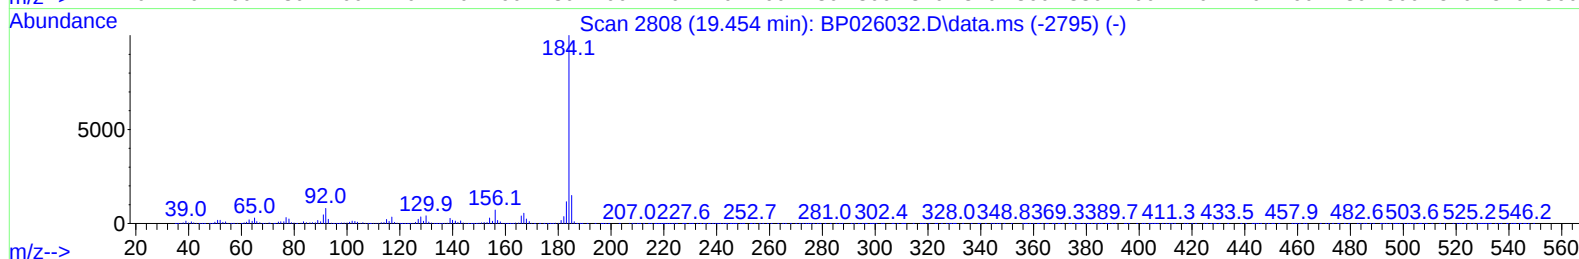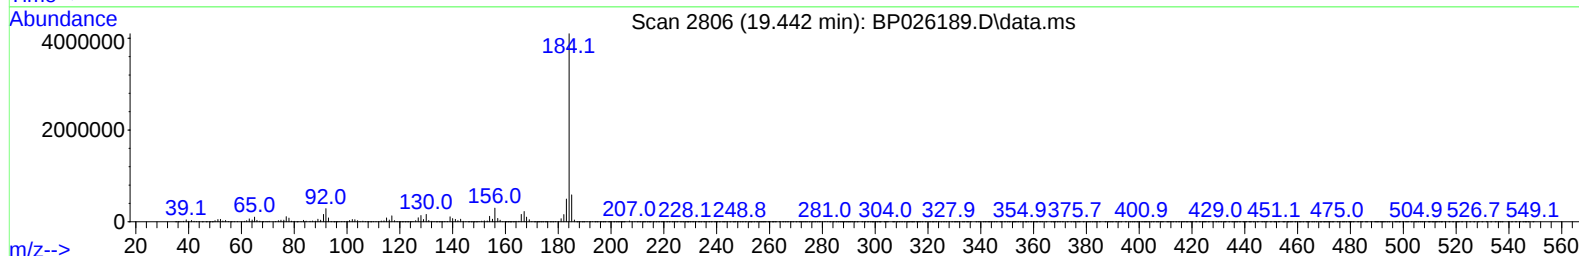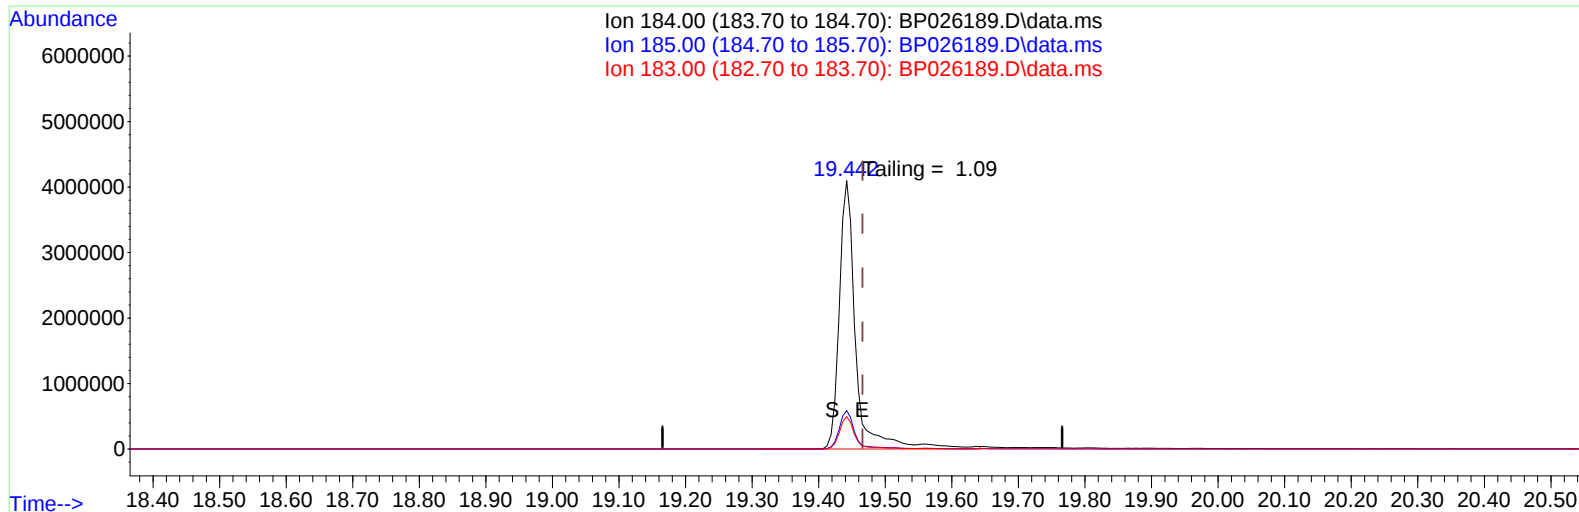

TIC: BP026189.D\data.ms

(77) Benzidine

19.442min (-0.024) 26907.41 ng

response 6791277

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.33
183.00	11.30	12.05
0.00	0.00	0.00