

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
 Data File : BP026056.D
 Acq On : 03 Nov 2025 13:21
 Operator : RC/JU
 Sample : PB170346BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB170346BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP026056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.272	389	397	414	rBV	5413073	7923486	41.75%	10.070%
2	6.819	652	660	676	rBV	5186721	7838000	41.30%	9.961%
3	7.654	795	802	810	rBV	1017977	1707632	9.00%	2.170%
4	8.795	987	996	1011	rBV	3178746	4845683	25.53%	6.158%
5	10.431	1265	1274	1284	rBV	1320019	2305679	12.15%	2.930%
6	12.913	1688	1696	1707	rBV	7620379	11483154	60.50%	14.594%
7	14.307	1925	1933	1941	rBV	2054961	2968731	15.64%	3.773%
8	15.825	2184	2191	2210	rBV	5624761	7912305	41.69%	10.055%
9	17.113	2404	2410	2422	rBV2	2468950	3652627	19.25%	4.642%
10	19.871	2872	2879	2891	rBV	12745653	18979070	100.00%	24.120%
11	21.577	3162	3169	3182	rBV2	2586472	4399319	23.18%	5.591%
12	24.895	3724	3733	3749	rVB	1549113	4671005	24.61%	5.936%




Sum of corrected areas: 78686691

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026056.D
Acq On : 03 Nov 2025 13:21
Operator : RC/JU
Sample : PB170346BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170346BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

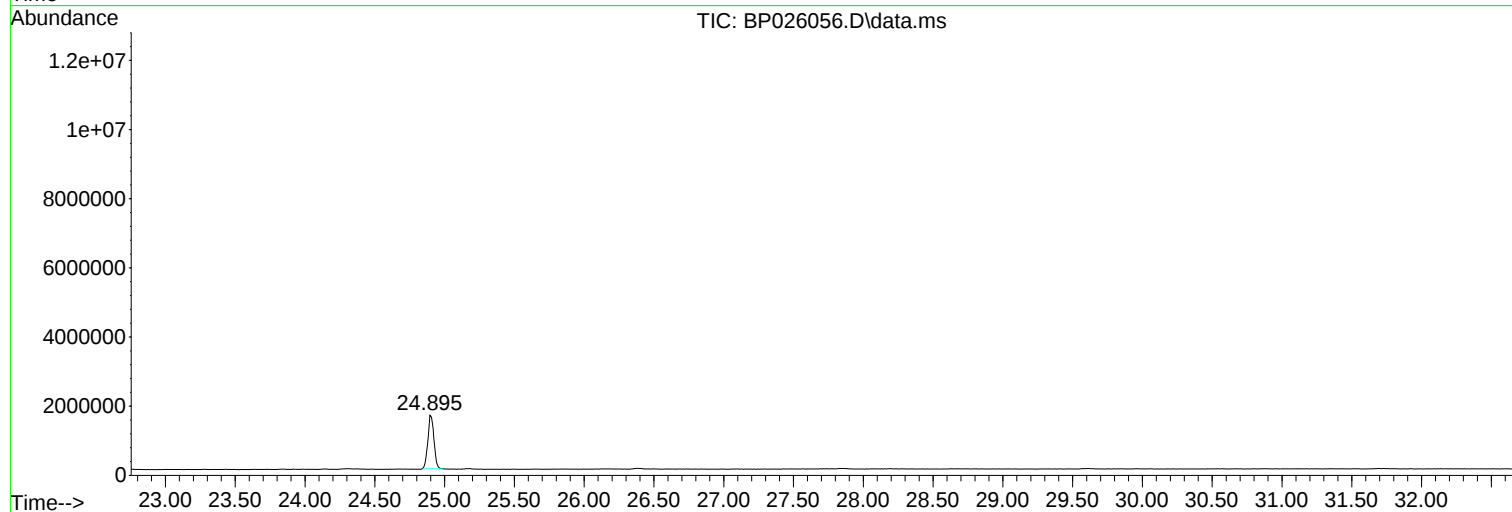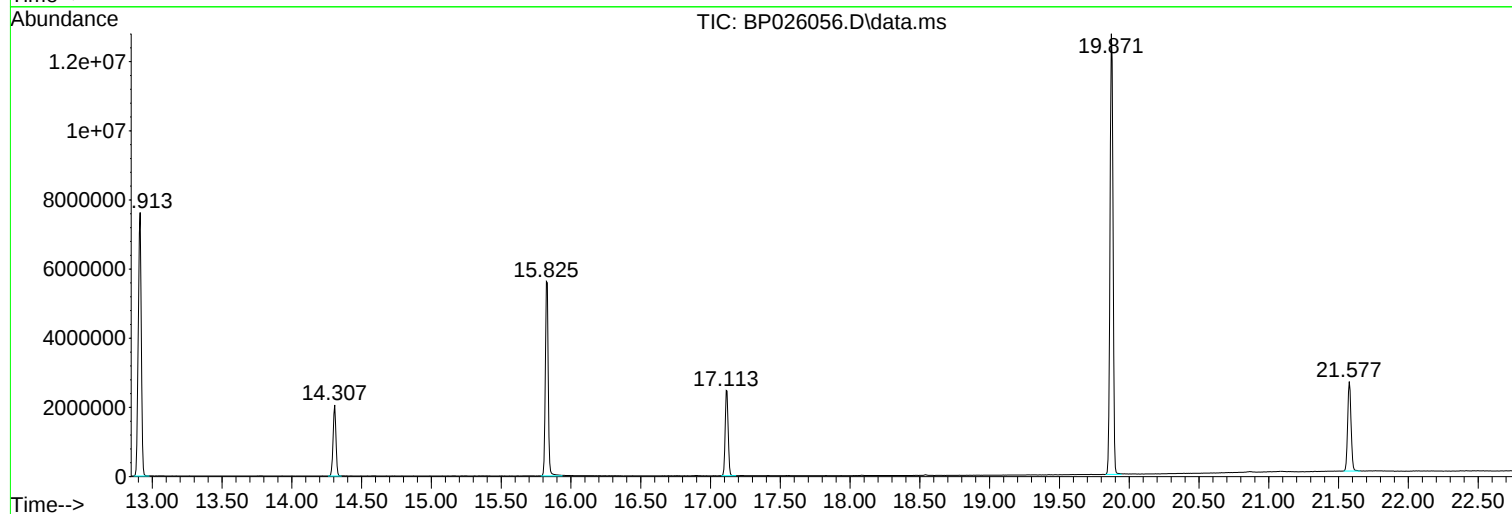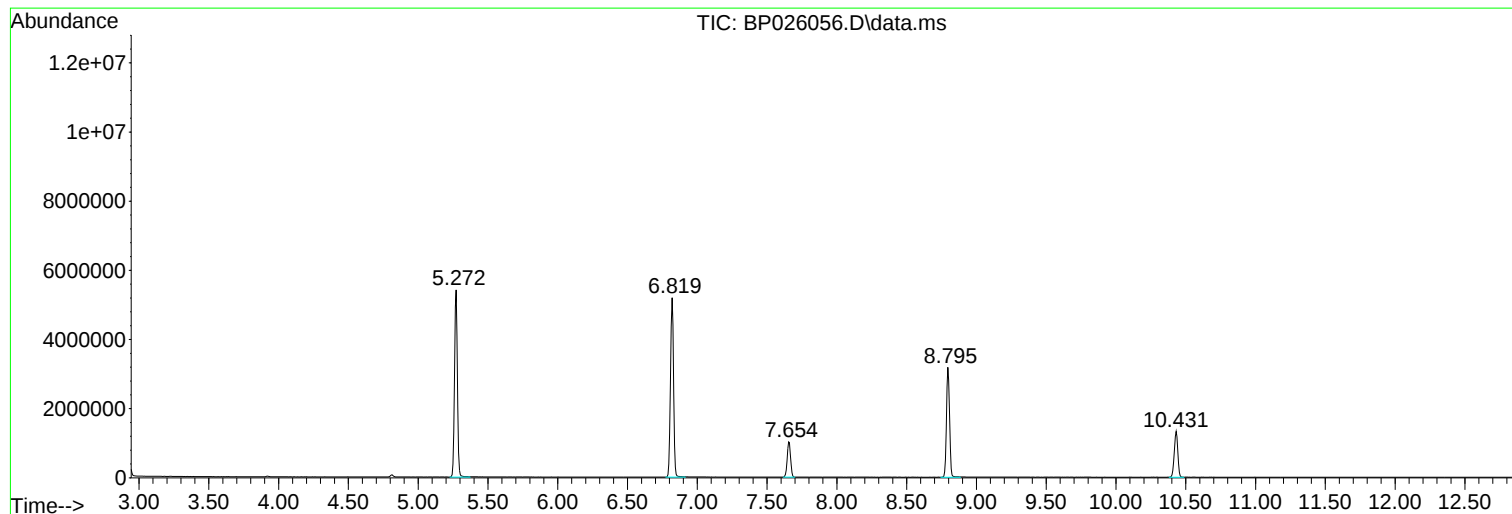

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026056.D
Acq On : 03 Nov 2025 13:21
Operator : RC/JU
Sample : PB170346BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170346BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026056.D
Acq On : 03 Nov 2025 13:21
Operator : RC/JU
Sample : PB170346BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170346BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------