

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103125\
 Data File : P0114809.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 13:58
 Operator : YP/AJ
 Sample : Q3495-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-1025-2

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/03/2025
 Supervised By :Yogesh Patel 11/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 14:23:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.653	152.9E6	102.1E6	28.156	25.508
2) SA Decachlor...	9.943	8.649	79154518	74336680	21.739	22.302m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103125\
Data File : PO114809.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 13:58
Operator : YP/AJ
Sample : Q3495-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-1025-2


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/03/2025
Supervised By :Yogesh Patel 11/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 14:23:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

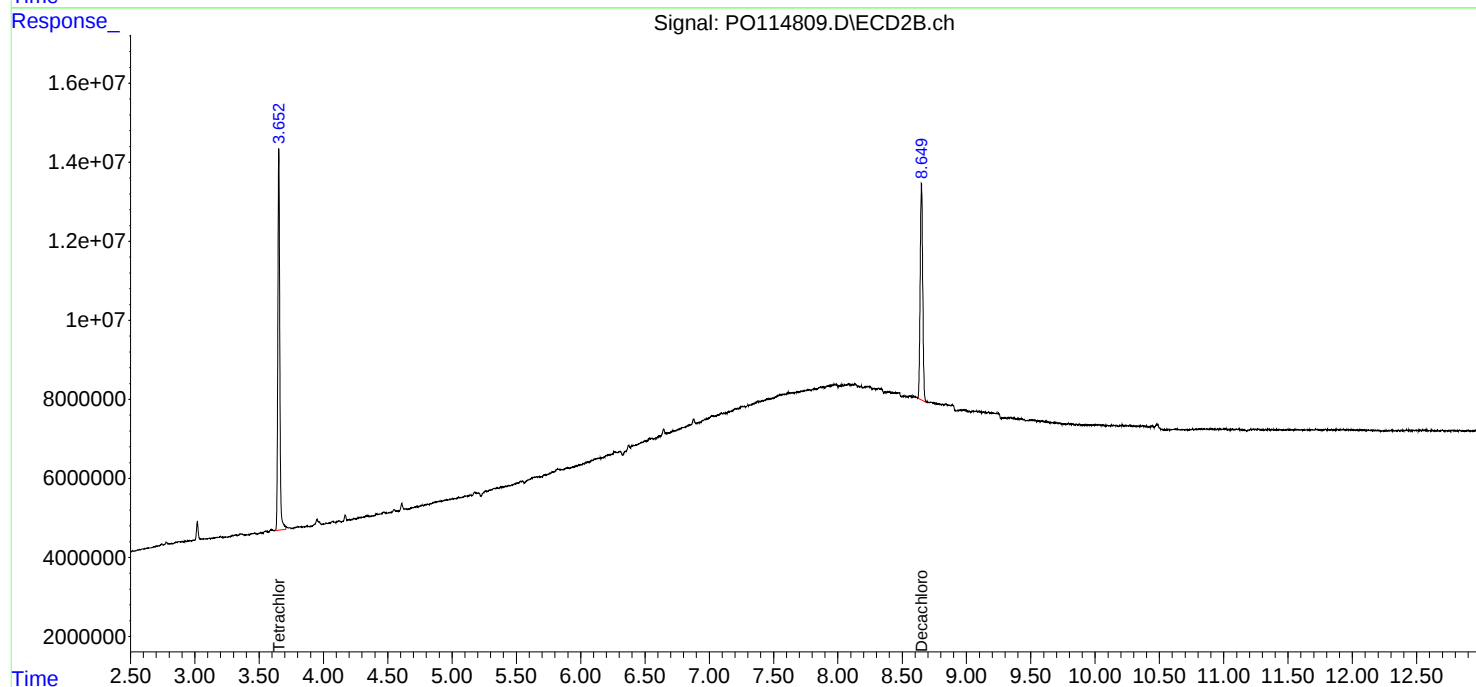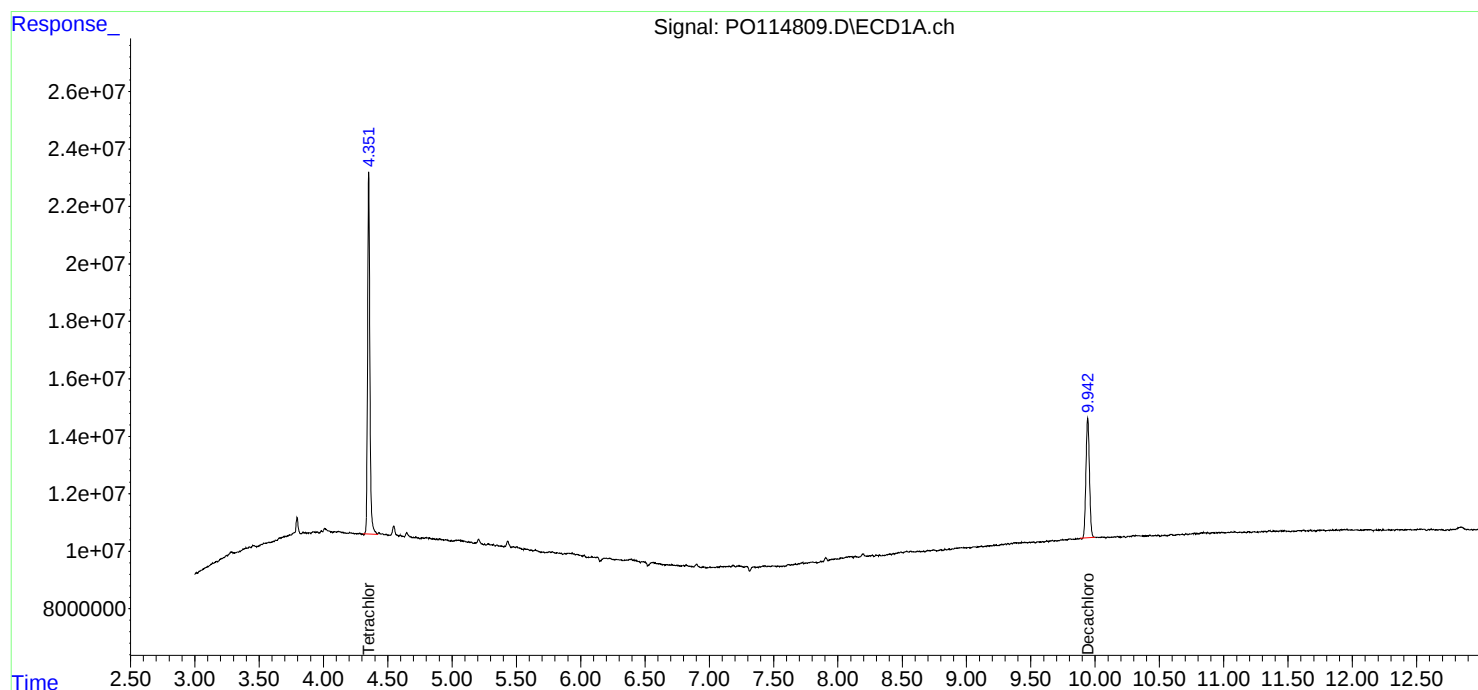

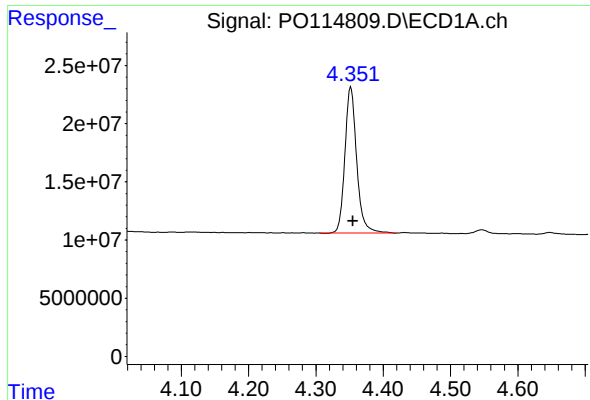


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.003 min
Response: 152856790
Conc: 28.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-1025-2


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/03/2025
Supervised By :Yogesh Patel 11/03/2025

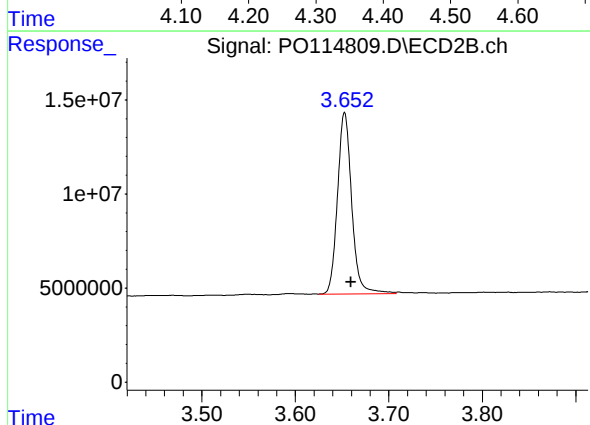


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.007 min
Response: 102091263
Conc: 25.51 ng/ml

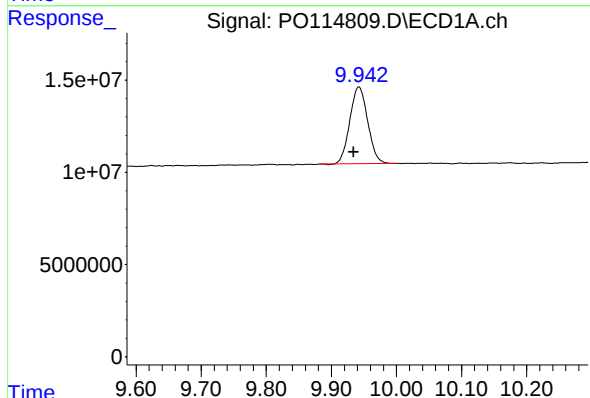

#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: 0.008 min
Response: 79154518
Conc: 21.74 ng/ml

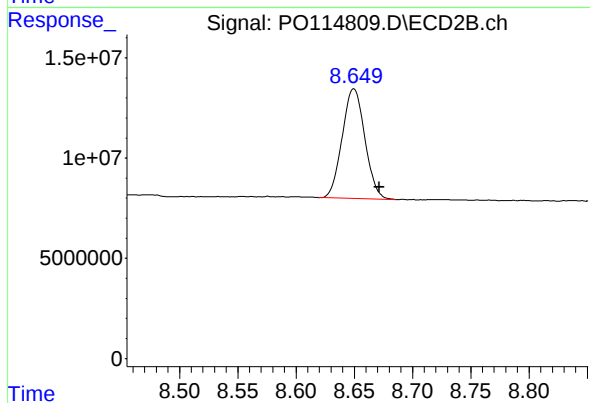

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.022 min
Response: 74336680
Conc: 22.30 ng/ml m