


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
Data File : BG064653.D
Acq On : 31 Oct 2025 12:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 16:40:26 2025

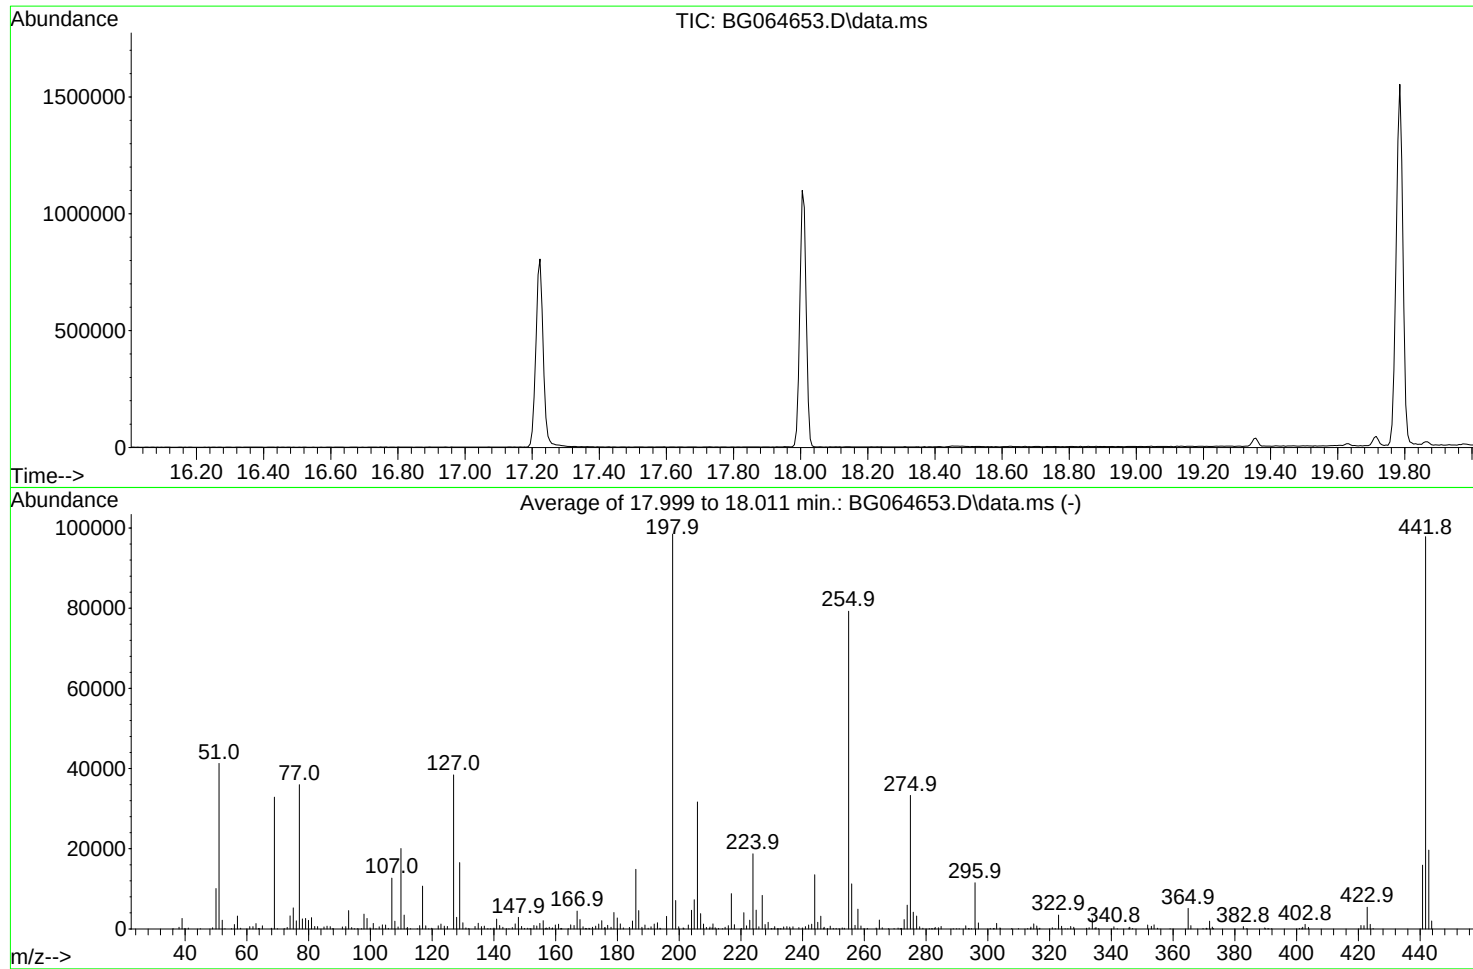




AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.6	203	PASS
69	69	100	100	100.0	32859	PASS
70	69	0.00	2	0.2	60	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98488	PASS
199	198	5	9	7.2	7105	PASS
365	198	1	100	5.2	5145	PASS
441	443	0.01	150	81.0	15924	PASS
442	442	100	100	100.0	97829	PASS
443	442	15	24	20.1	19658	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
Data File : BG064653.D
Acq On : 31 Oct 2025 12:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 31 13:23:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

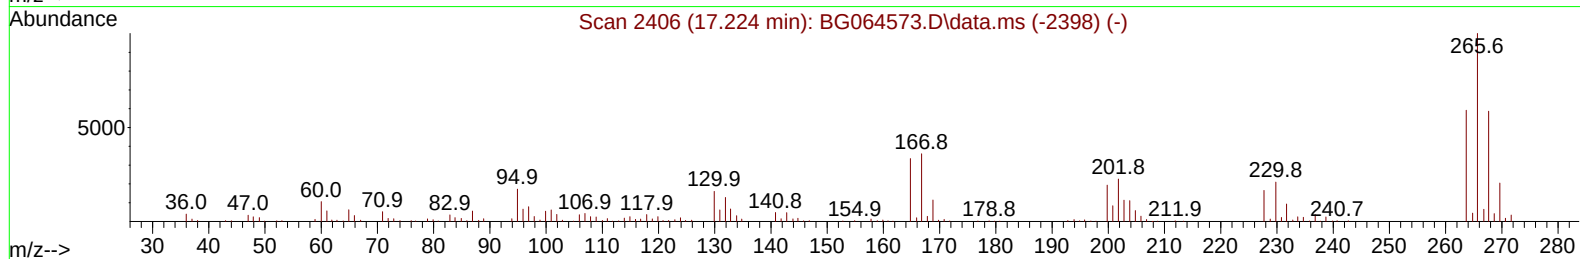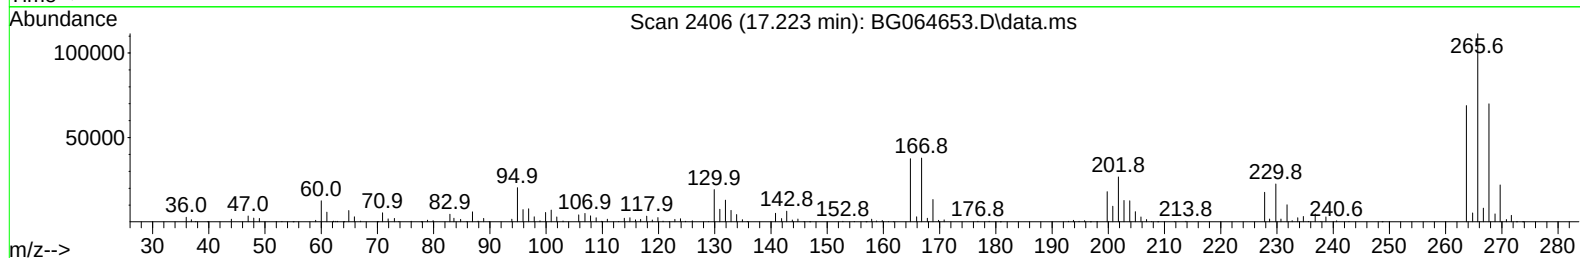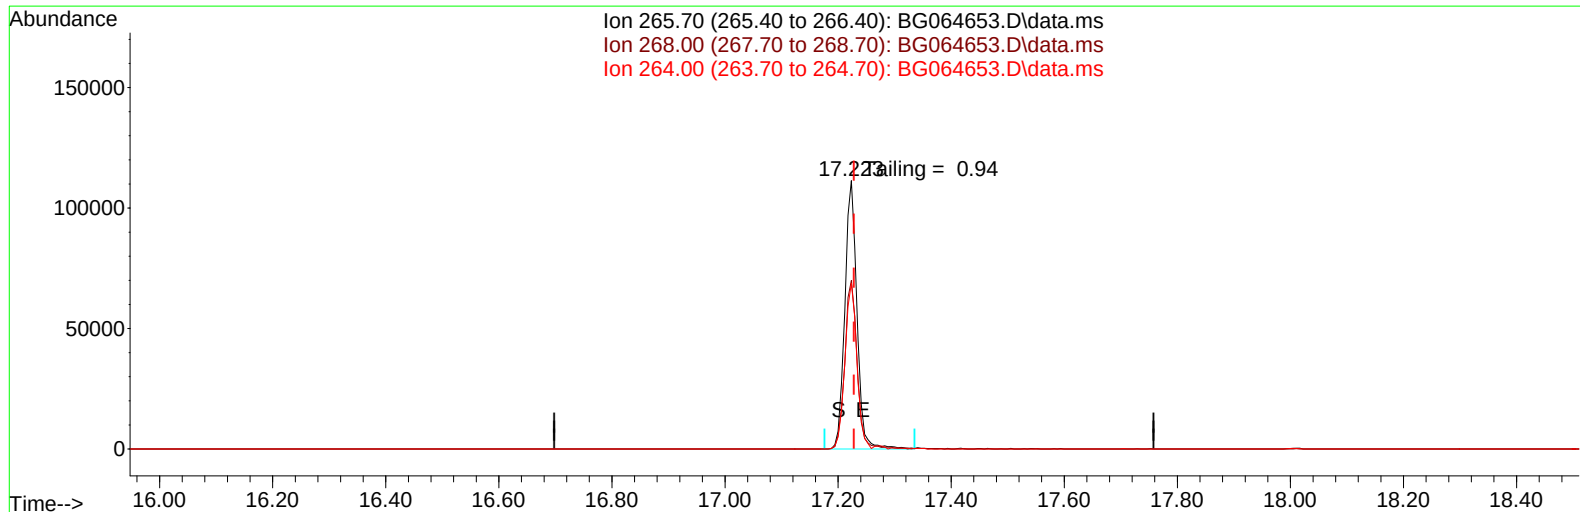

TIC: BG064653.D\data.ms

(70) Pentachlorophenol (C)

17.223min (-0.004) 30324.08 ng m




response 166681

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.76
264.00	59.10	61.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
Data File : BG064653.D
Acq On : 31 Oct 2025 12:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 31 13:23:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

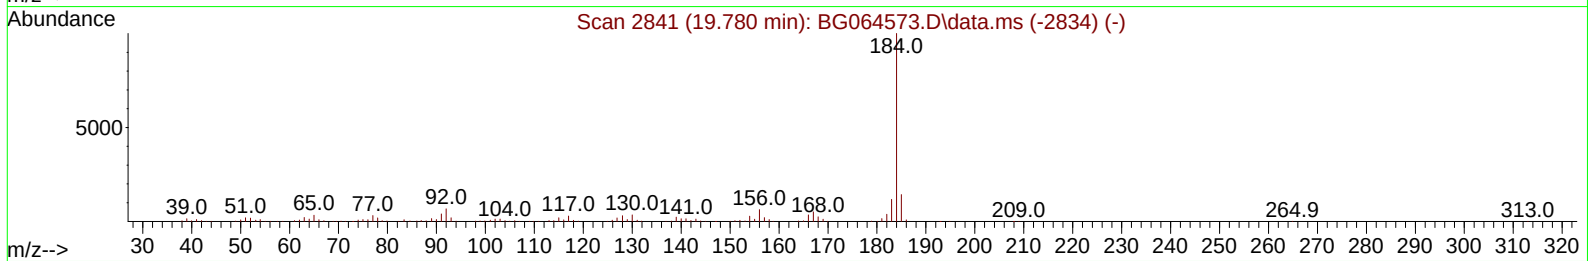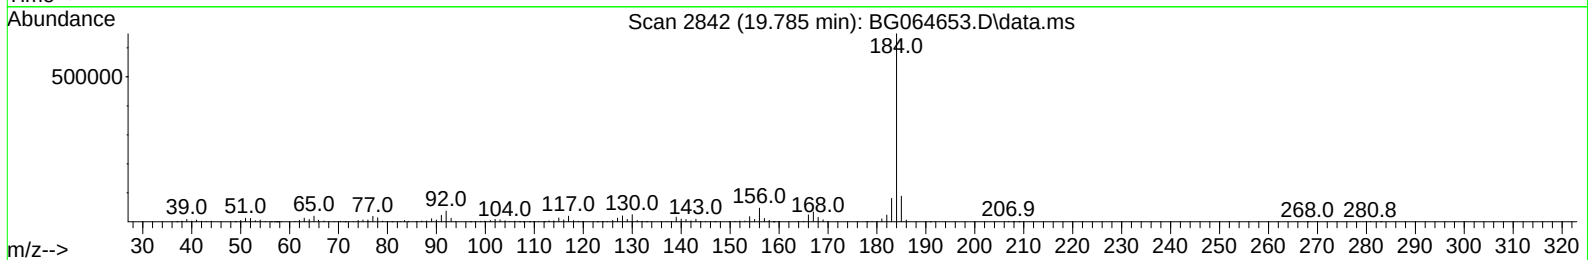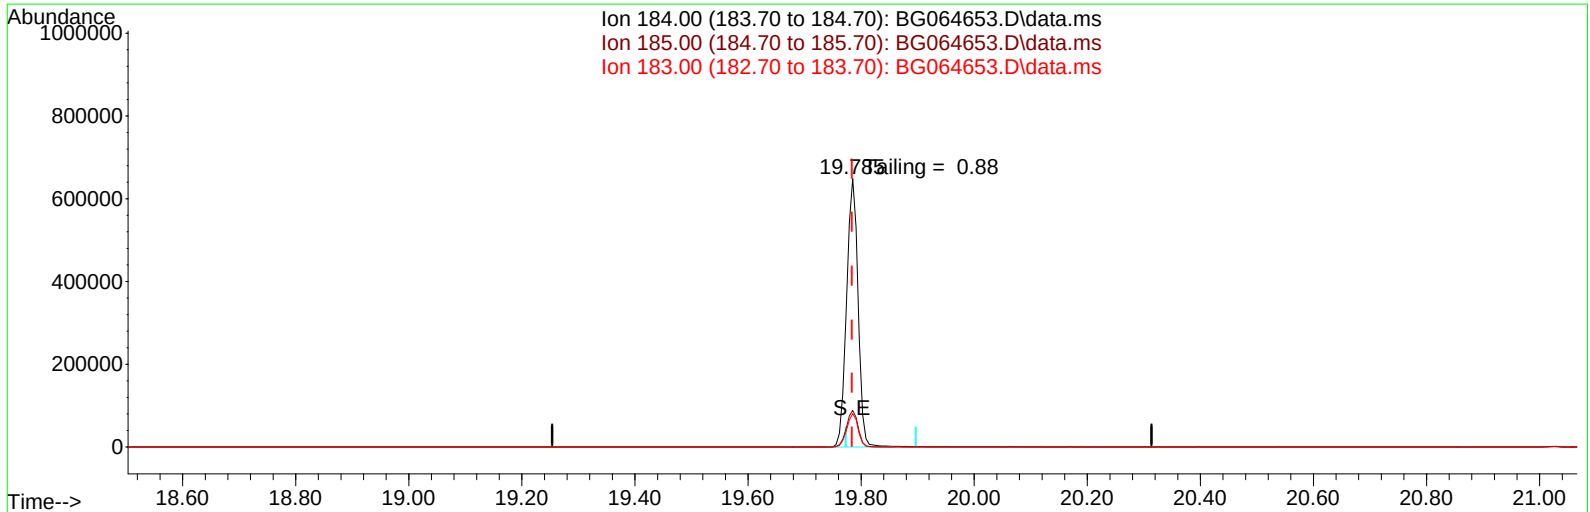

TIC: BG064653.D\data.ms

(77) Benzidine

19.785min (+ 0.002) 516456.63 ng

response 740529

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.67
183.00	11.80	12.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/31/2025	BNA_G	<u>BG064653.D</u>
Compound Name	Response	Retention Time
DDT	481237	21.025
DDD	7452	20.572
DDE	956	20.079
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8408	489645	1.72

Instrument :
BNA_G
ClientSampleId :
DFTPP