
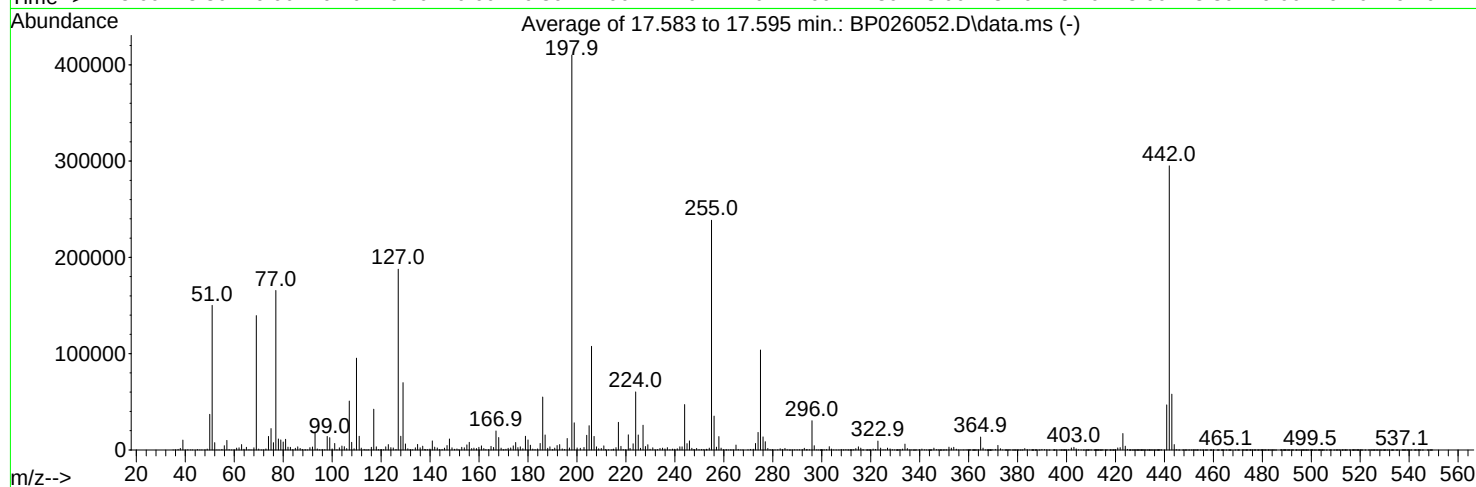


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026052.D
Acq On : 03 Nov 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 30 11:51:34 2025

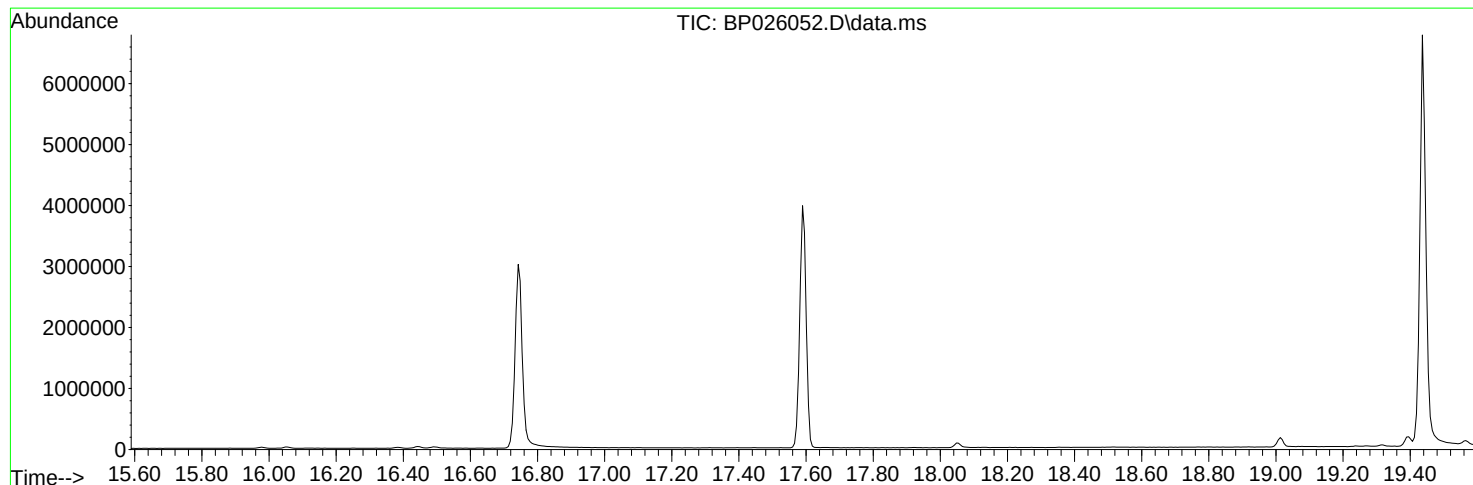




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2201	PASS
69	69	100	100	100.0	139597	PASS
70	69	0.00	2	0.6	886	PASS
197	198	0.00	2	0.5	2141	PASS
198	198	100	100	100.0	410085	PASS
199	198	5	9	6.9	28183	PASS
365	198	1	100	3.3	13331	PASS
441	443	0.01	150	80.8	46777	PASS
442	442	100	100	100.0	295123	PASS
443	442	15	24	19.6	57925	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026052.D
Acq On : 03 Nov 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 03 11:20:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

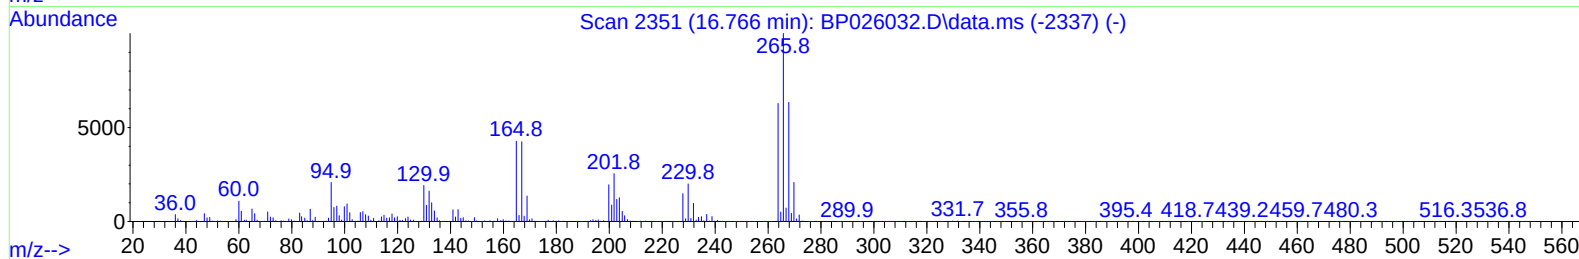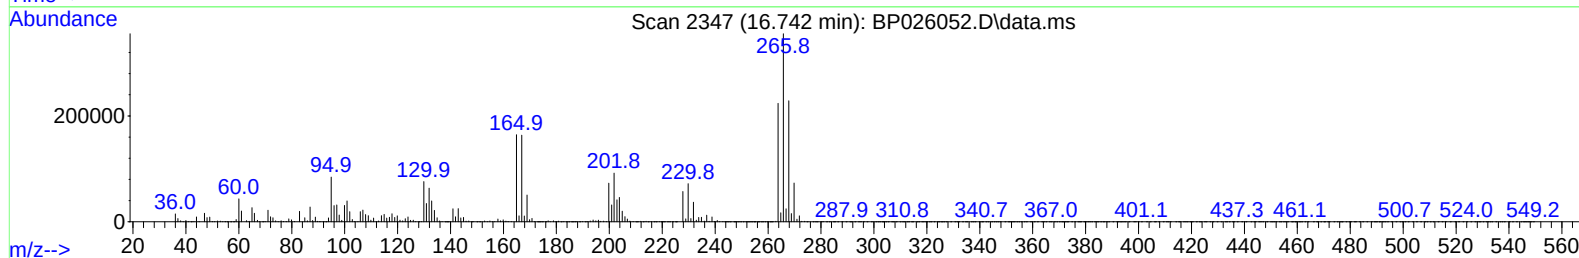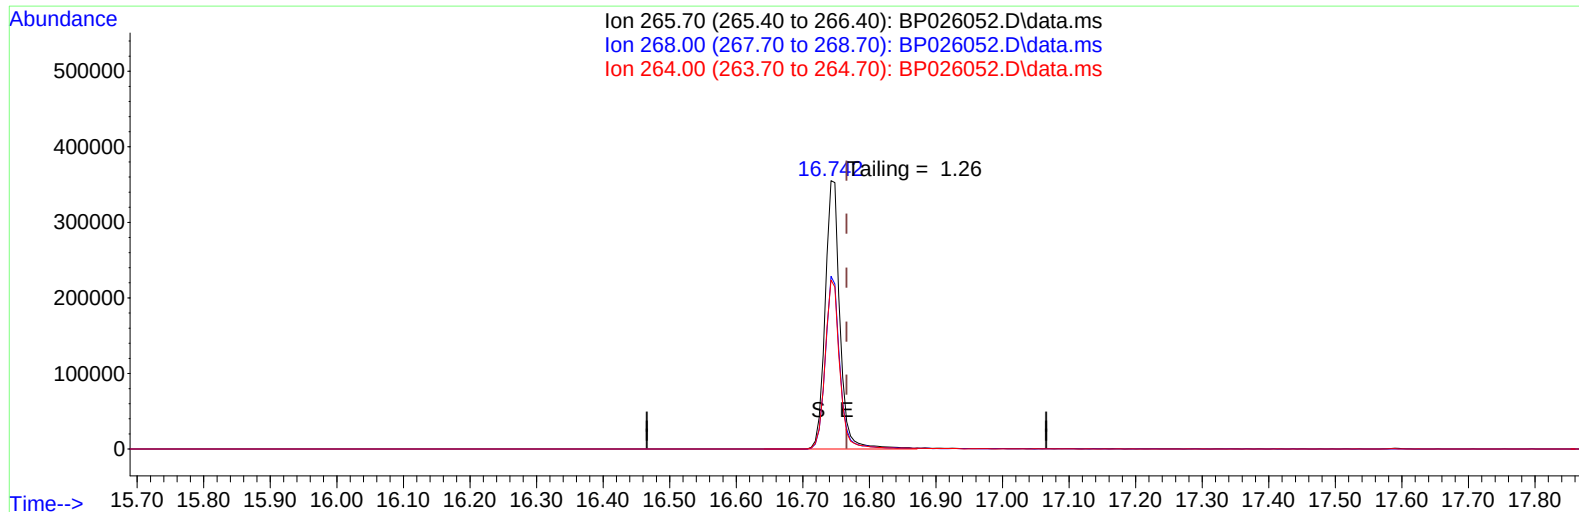

TIC: BP026052.D\data.ms

(70) Pentachlorophenol (C)

16.742min (-0.023) 2966656.68 ng




response 549178

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.31
264.00	62.80	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026052.D
Acq On : 03 Nov 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 03 11:20:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

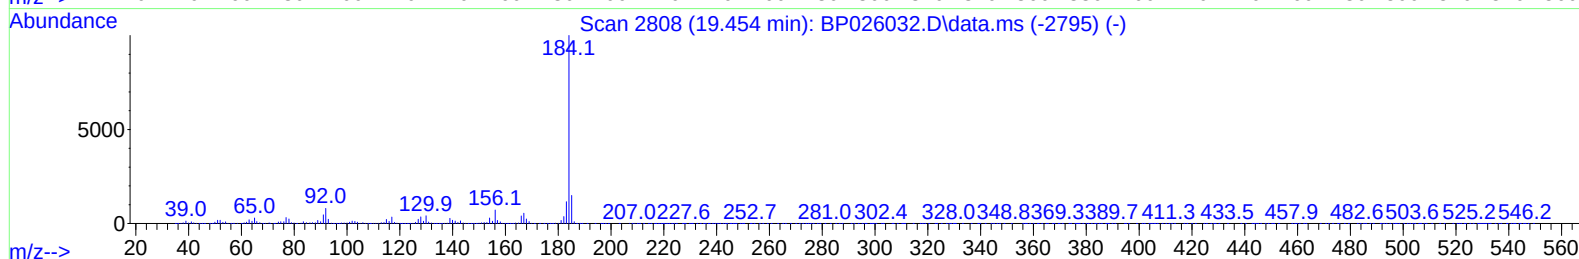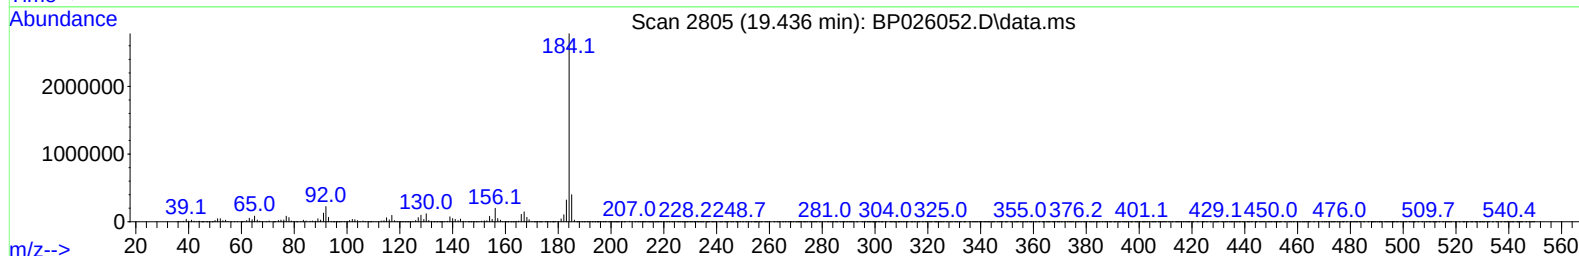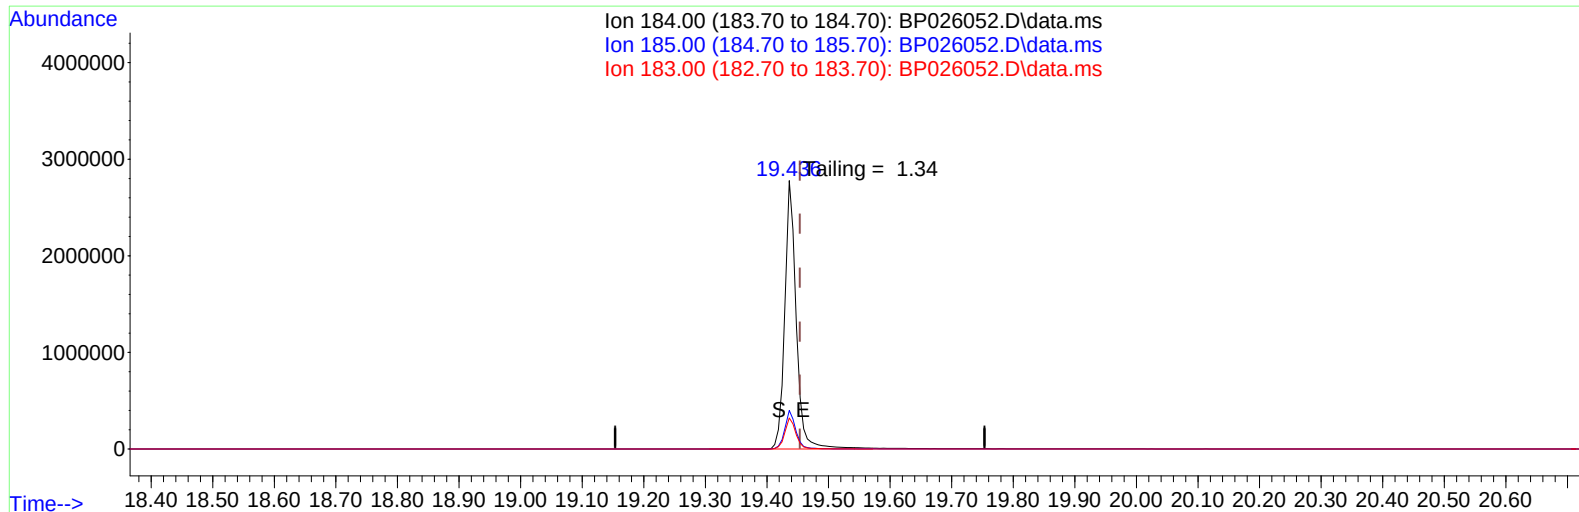

TIC: BP026052.D\data.ms

(77) Benzidine

19.436min (-0.017) 1459112.87 ng

response 3666573

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.38
183.00	11.50	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2025	BNA_P	<u>BP026052.D</u>
Compound Name	Response	Retention Time
DDT	1332752	20.748
DDD	9563	20.283
DDE	937	19.754
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10500	1343252	0.78

Instrument :
BNA_P
ClientSampleId :
DFTPP