


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110325\
Data File : VX048444.D
Acq On : 03 Nov 2025 08:20
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102925W.M
Title : SW846 8260
Last Update : Thu Oct 30 02:37:17 2025

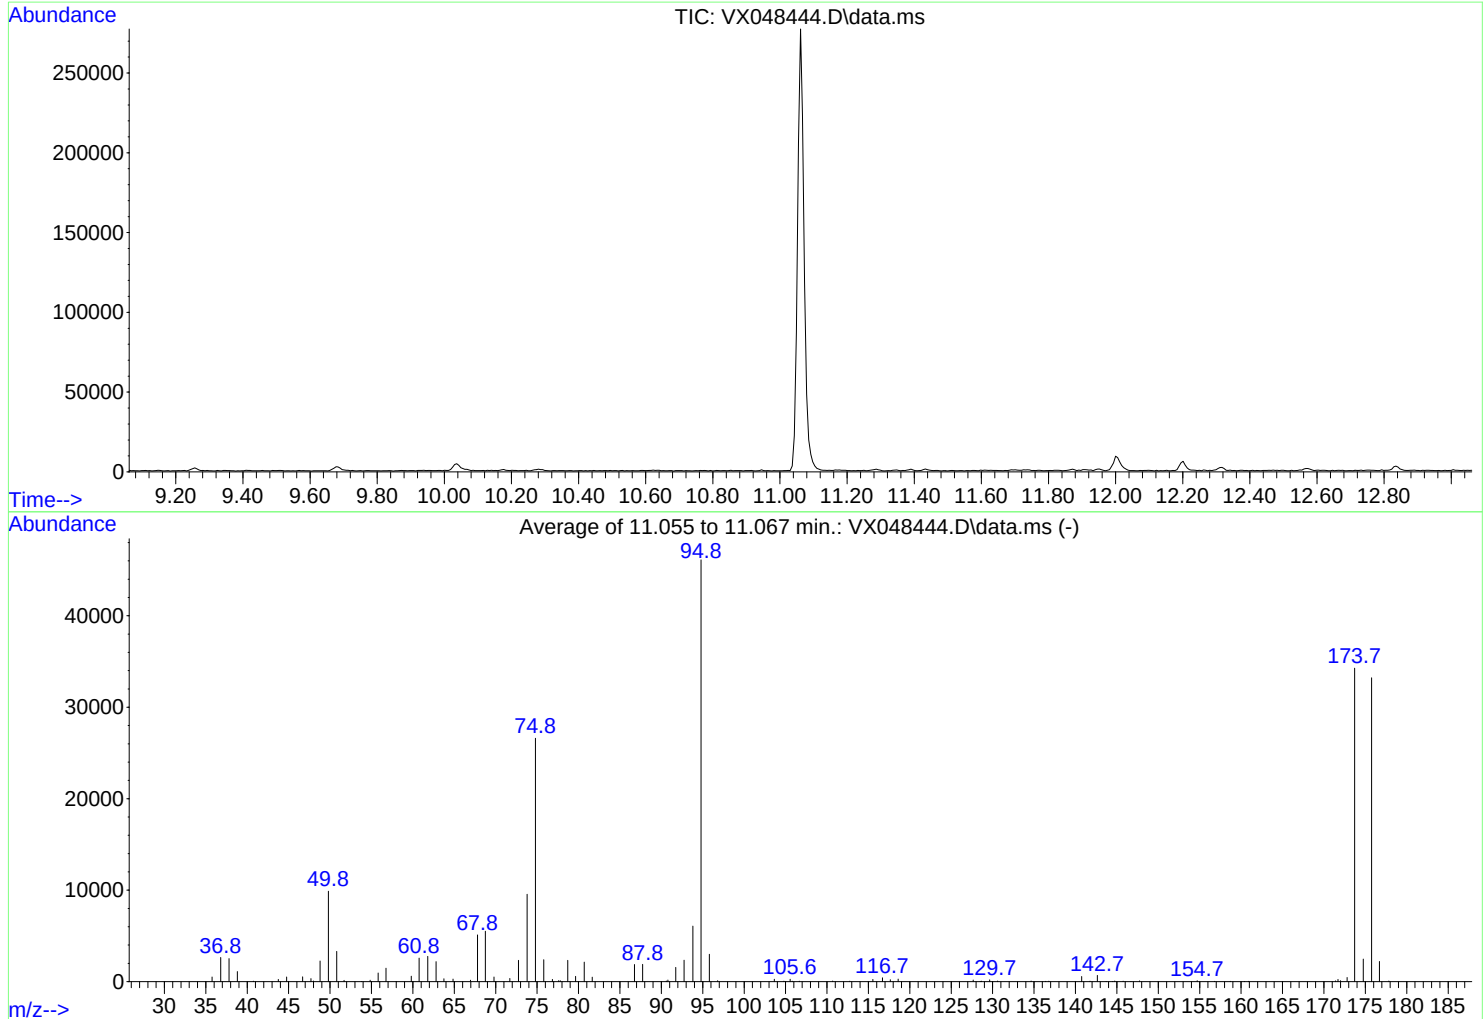

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	9885	PASS
75	95	30	60	57.7	26600	PASS
95	95	100	100	100.0	46112	PASS
96	95	5	9	6.5	2992	PASS
173	174	0.00	2	1.3	456	PASS
174	95	50	100	74.3	34275	PASS
175	174	5	9	7.2	2472	PASS
176	174	95	101	96.9	33221	PASS
177	176	5	9	6.6	2196	PASS