


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102825\
Data File : BN038110.D
Acq On : 28 Oct 2025 12:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 29 13:09:46 2025

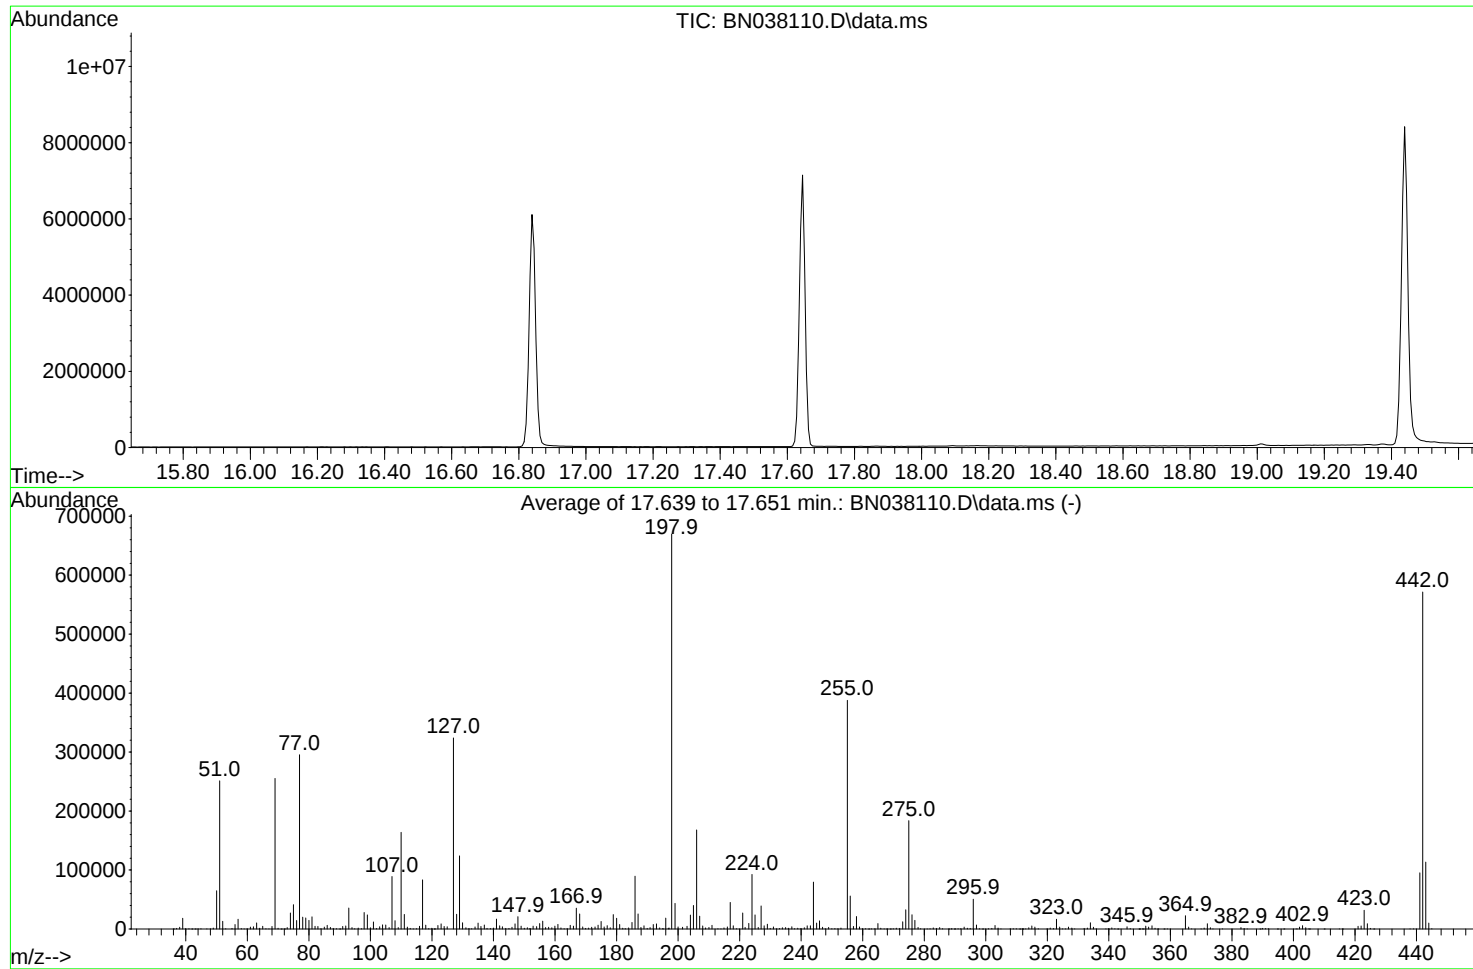




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	4477	PASS
69	69	100	100	100.0	255398	PASS
70	69	0.00	2	0.5	1371	PASS
197	198	0.00	2	0.2	1550	PASS
198	198	100	100	100.0	669440	PASS
199	198	5	9	6.5	43461	PASS
365	198	1	100	3.4	22528	PASS
441	443	0.01	150	83.9	95293	PASS
442	442	100	100	100.0	571285	PASS
443	442	15	24	19.9	113539	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102825\
Data File : BN038110.D
Acq On : 28 Oct 2025 12:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 28 18:06:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 28 12:54:48 2025
Response via : Initial Calibration

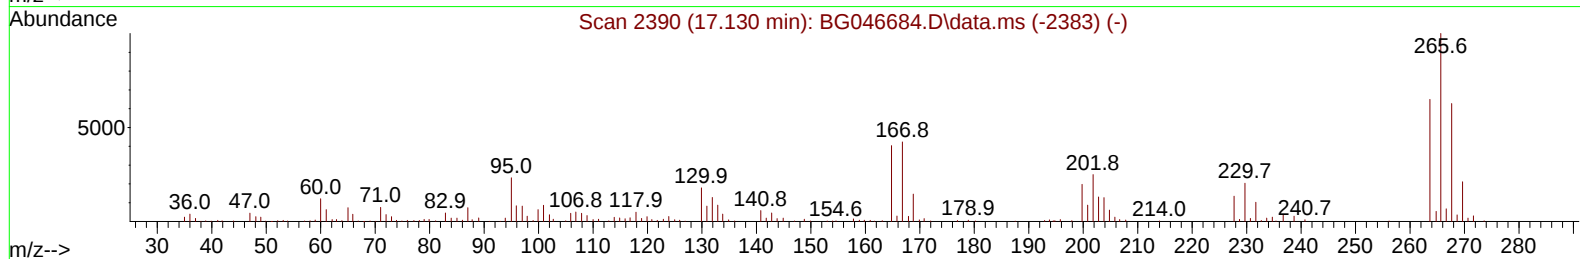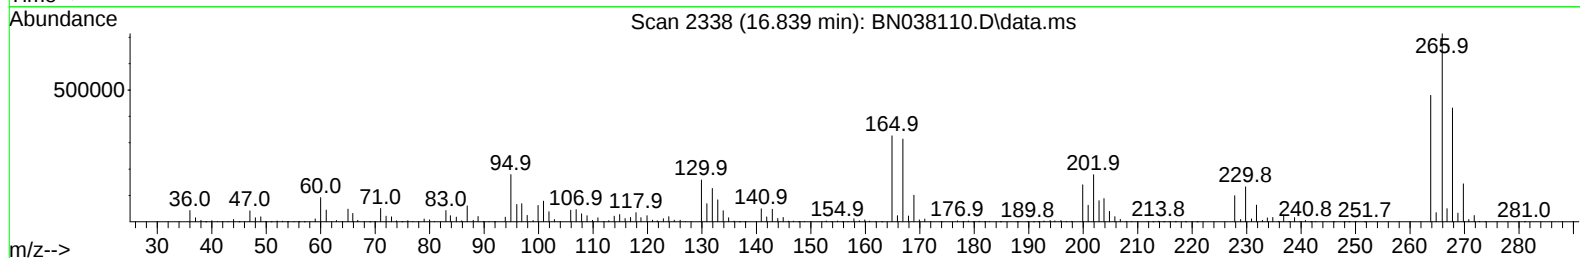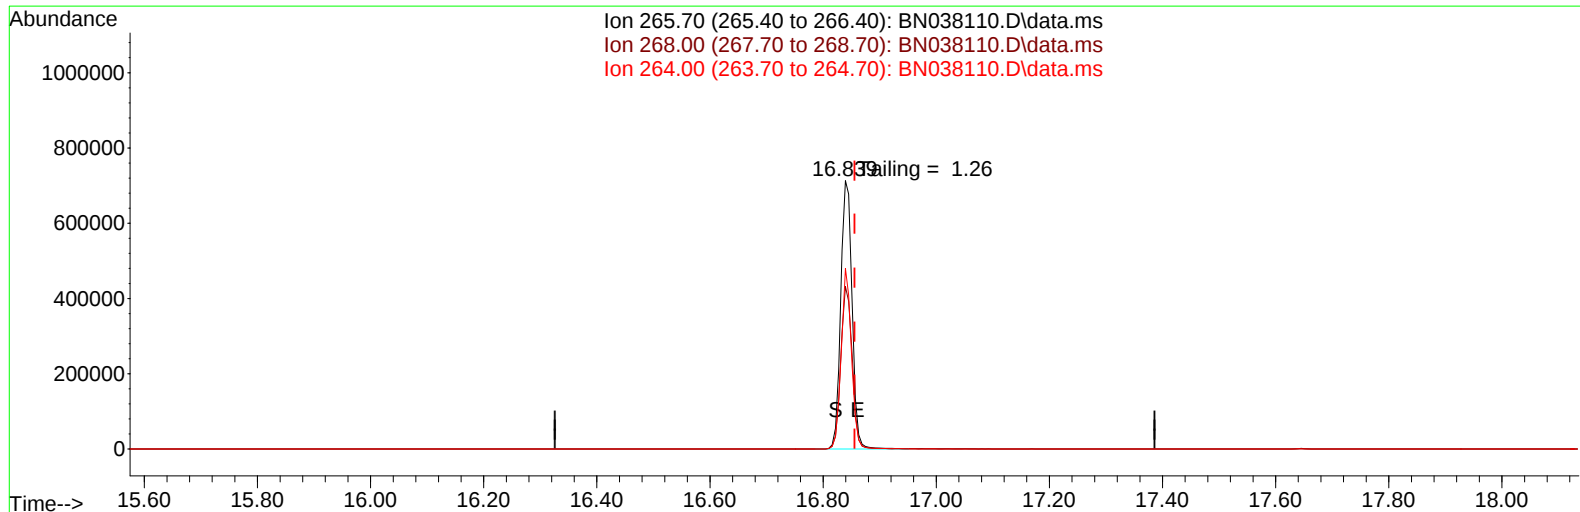

TIC: BN038110.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.017) 31764.46 ng




response 993628

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.51
264.00	61.60	67.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102825\
Data File : BN038110.D
Acq On : 28 Oct 2025 12:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 28 18:06:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 28 12:54:48 2025
Response via : Initial Calibration

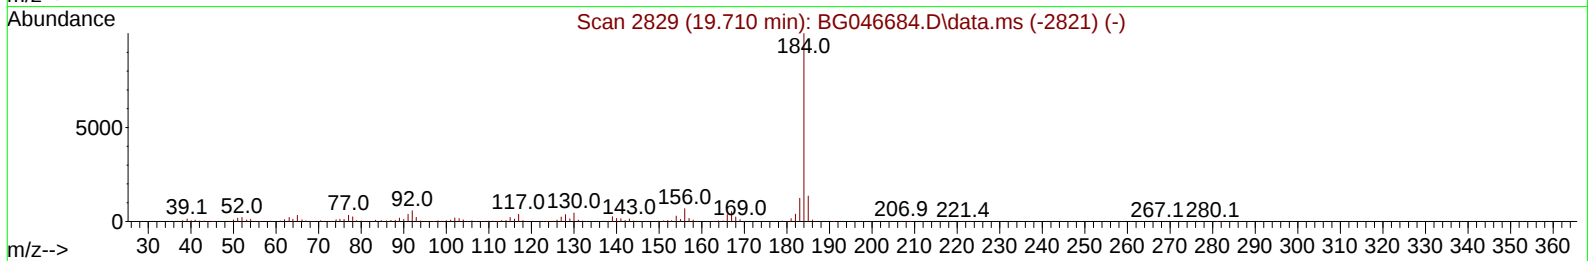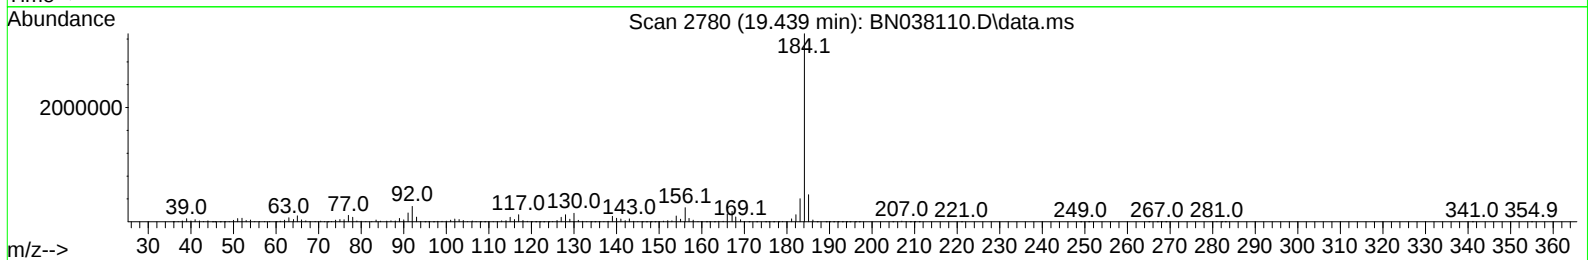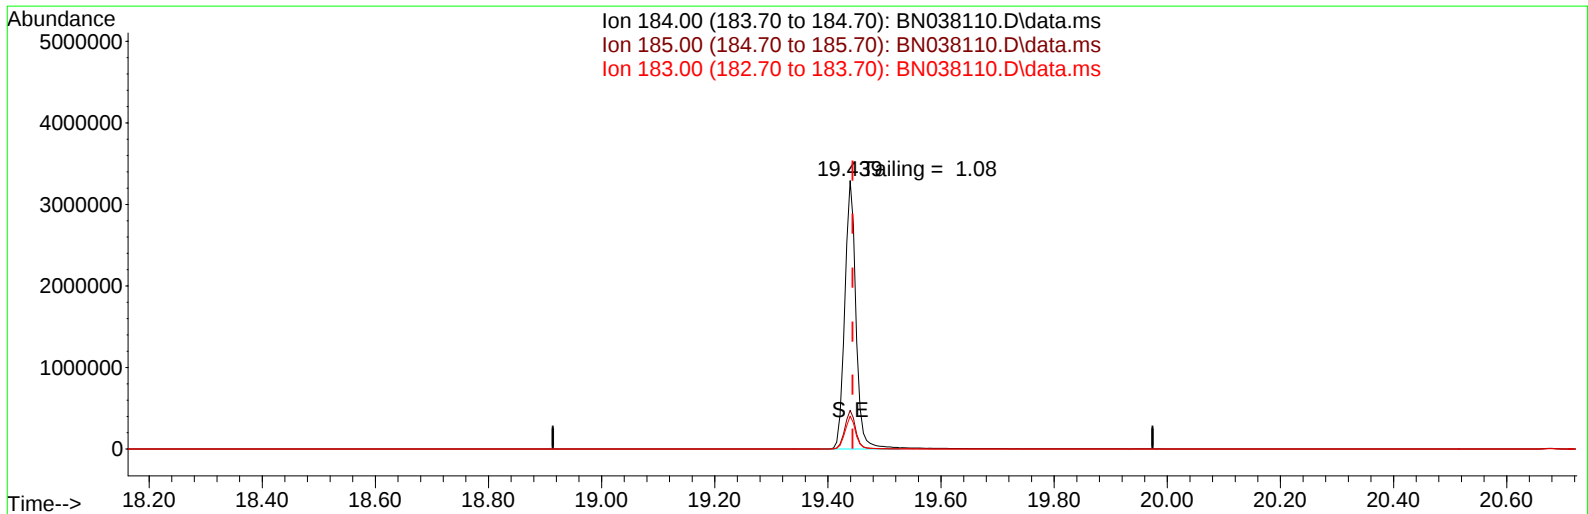

TIC: BN038110.D\data.ms

(77) Benzidine

19.439min (-0.005) 0.00 ng

response 4602519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	12.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/28/2025	BNA_N	<u>BN038110.D</u>
Compound Name	Response	Retention Time
DDT	2477320	20.674
DDD	29265	20.233
DDE	1740	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31005	2508325	1.24

Instrument :
BNA_N
ClientSampleId :
DFTPP