
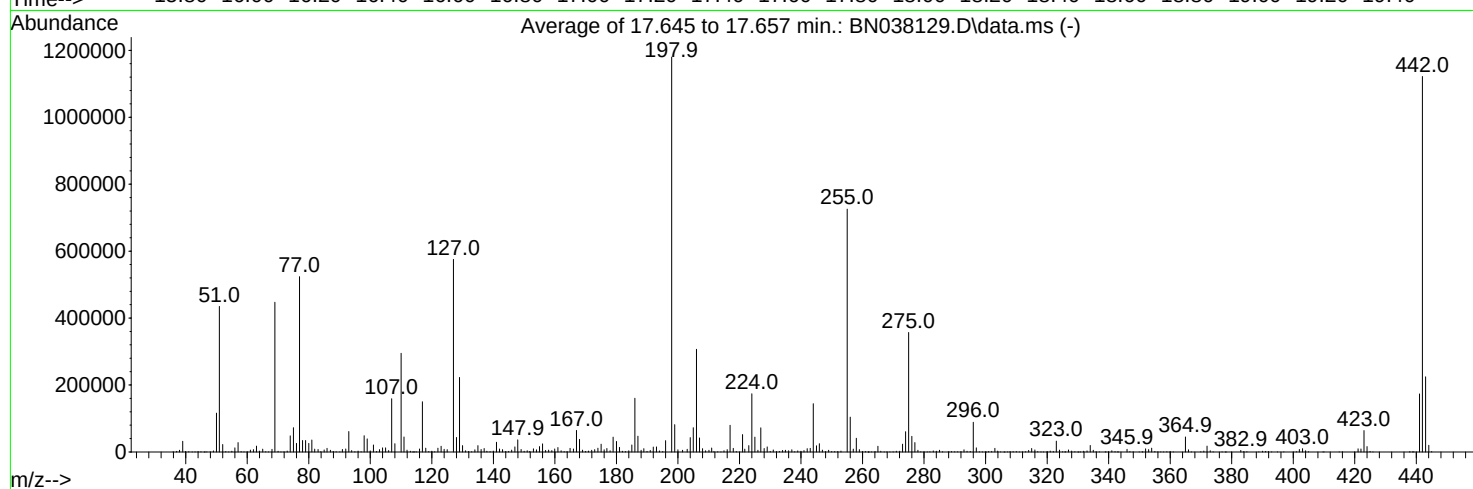


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110425\
Data File : BN038129.D
Acq On : 04 Nov 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 29 13:09:46 2025

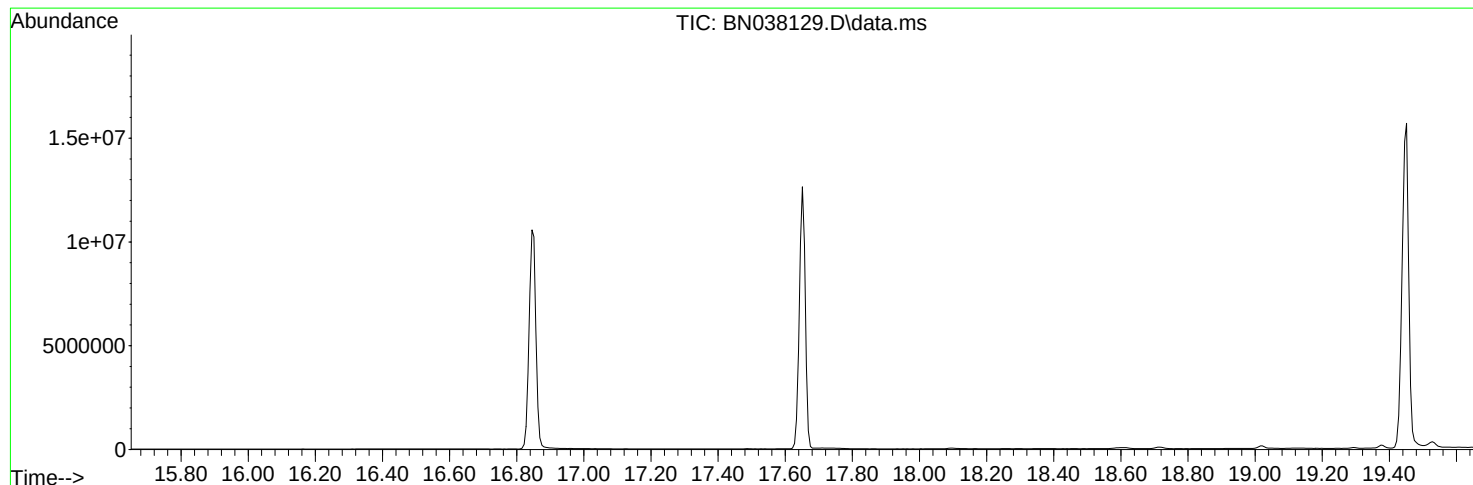




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2467

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	7977	PASS
69	69	100	100	100.0	447289	PASS
70	69	0.00	2	0.5	2389	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1179904	PASS
199	198	5	9	6.9	81427	PASS
365	198	1	100	3.8	44821	PASS
441	443	0.01	150	77.2	173248	PASS
442	442	100	100	100.0	1122112	PASS
443	442	15	24	20.0	224533	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110425\
Data File : BN038129.D
Acq On : 04 Nov 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 14:05:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 04 14:05:21 2025
Response via : Initial Calibration

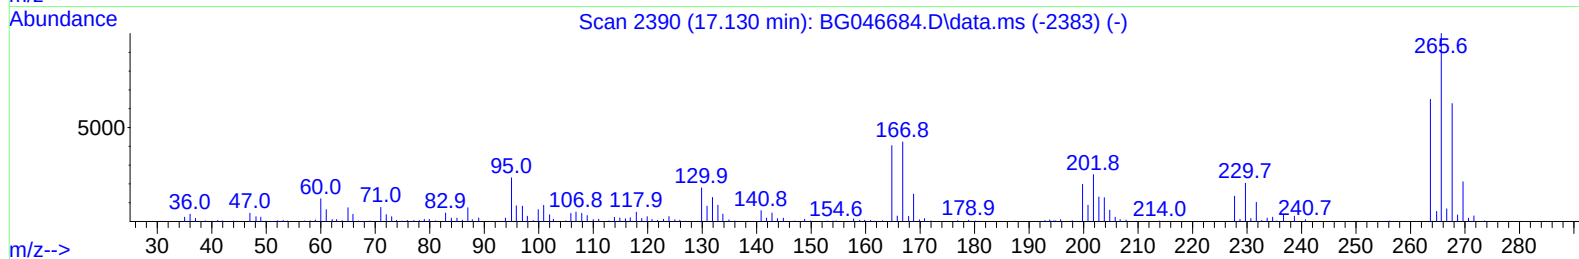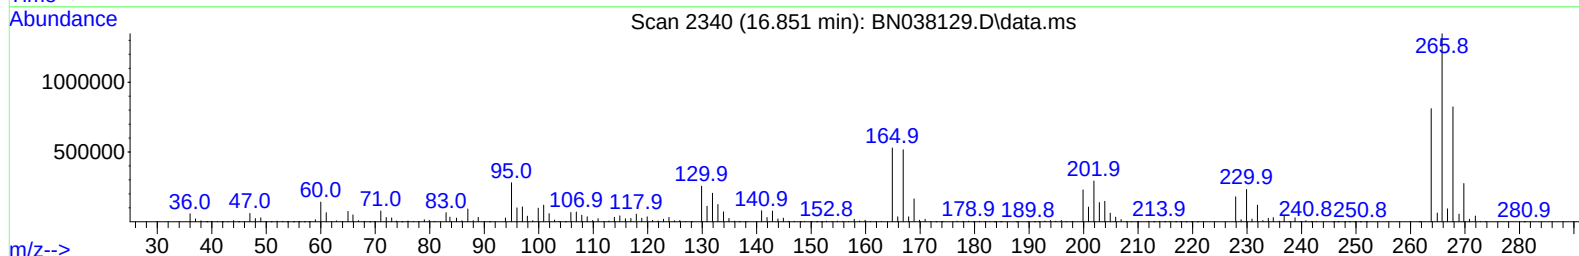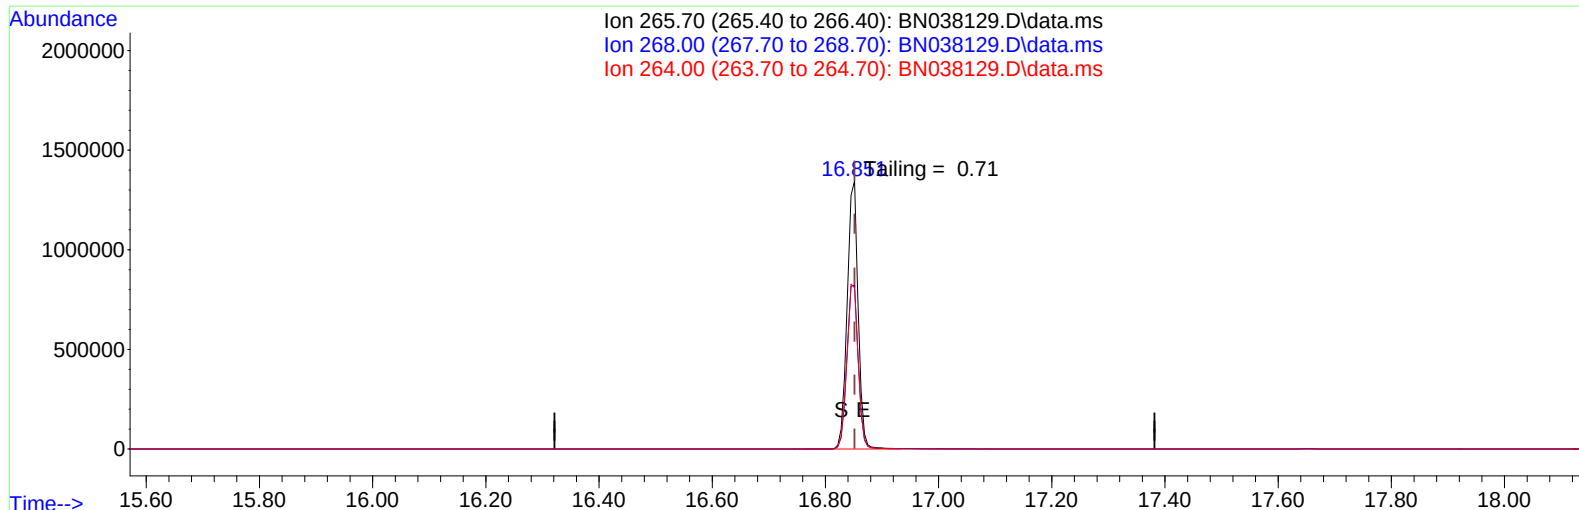

TIC: BN038129.D\data.ms

(70) Pentachlorophenol (C)

16.851min (0.000) 277.93 ng




response 1813451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.08
264.00	61.60	60.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110425\
Data File : BN038129.D
Acq On : 04 Nov 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 14:05:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 04 14:05:21 2025
Response via : Initial Calibration

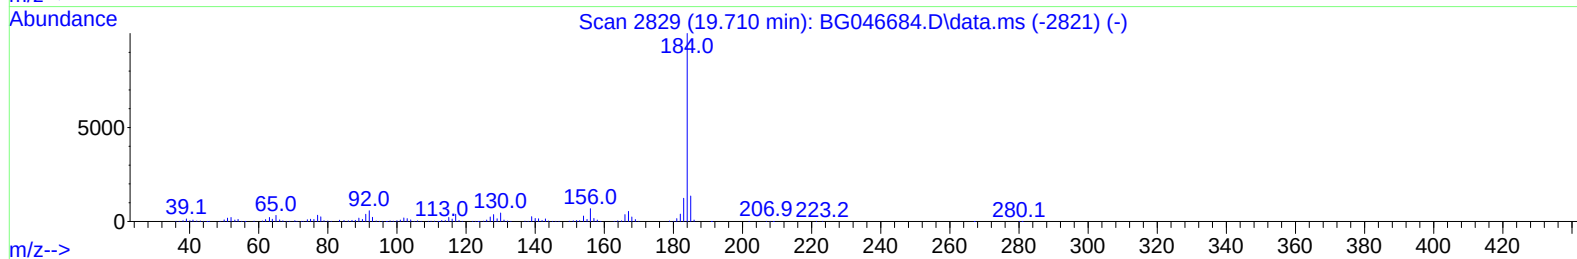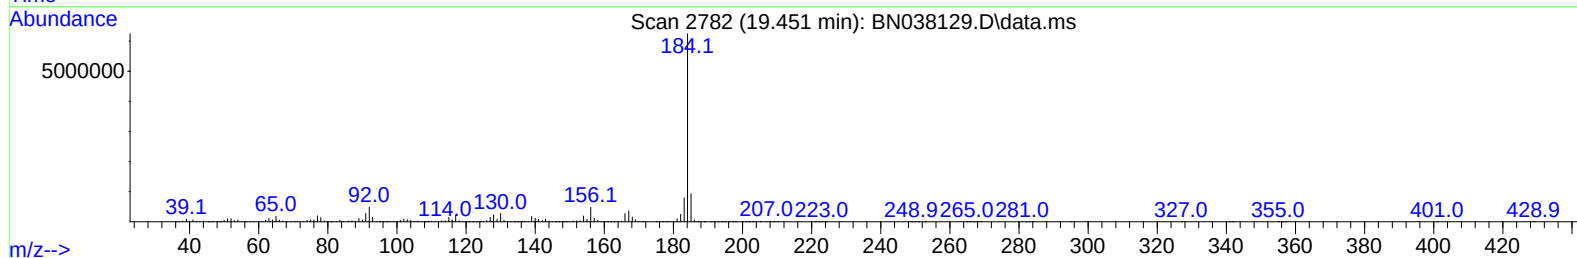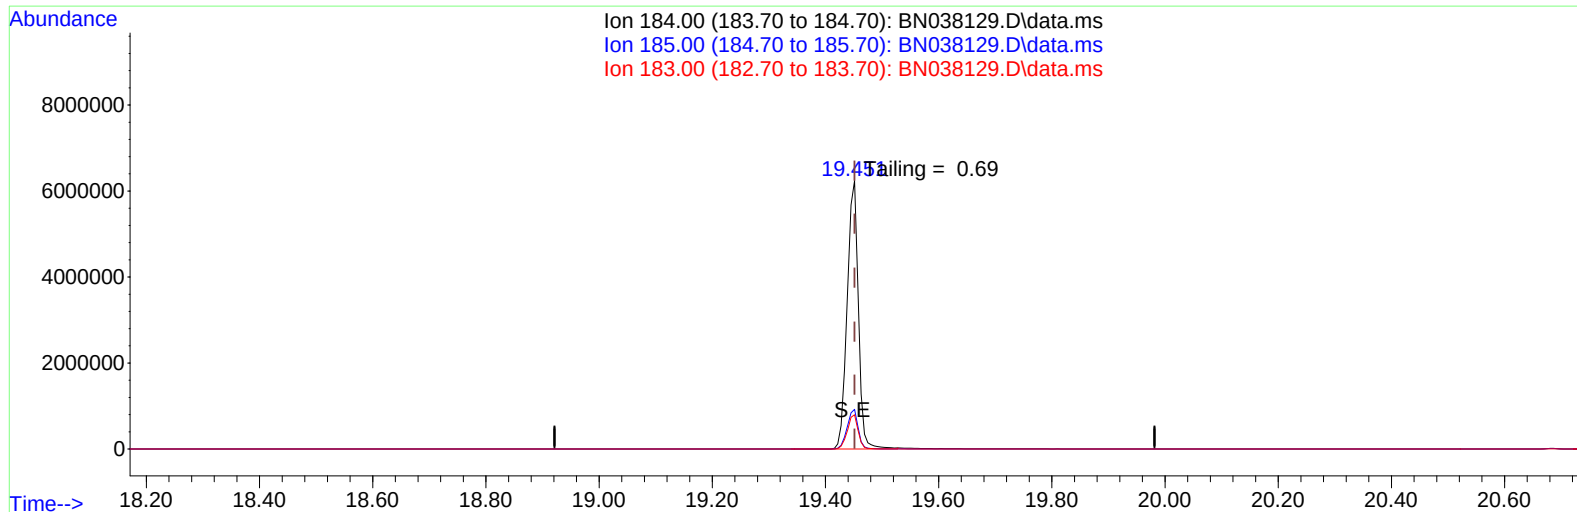

TIC: BN038129.D\data.ms

(77) Benzidine

19.451min (0.000) 0.00 ng

response 8673581

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.80
183.00	13.20	12.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2025	BNA_N	<u>BN038129.D</u>
Compound Name	Response	Retention Time
DDT	4564306	20.686
DDD	39263	20.233
DDE	2743	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42006	4606312	0.91

Instrument :
BNA_N
ClientSampleId :
DFTPP