
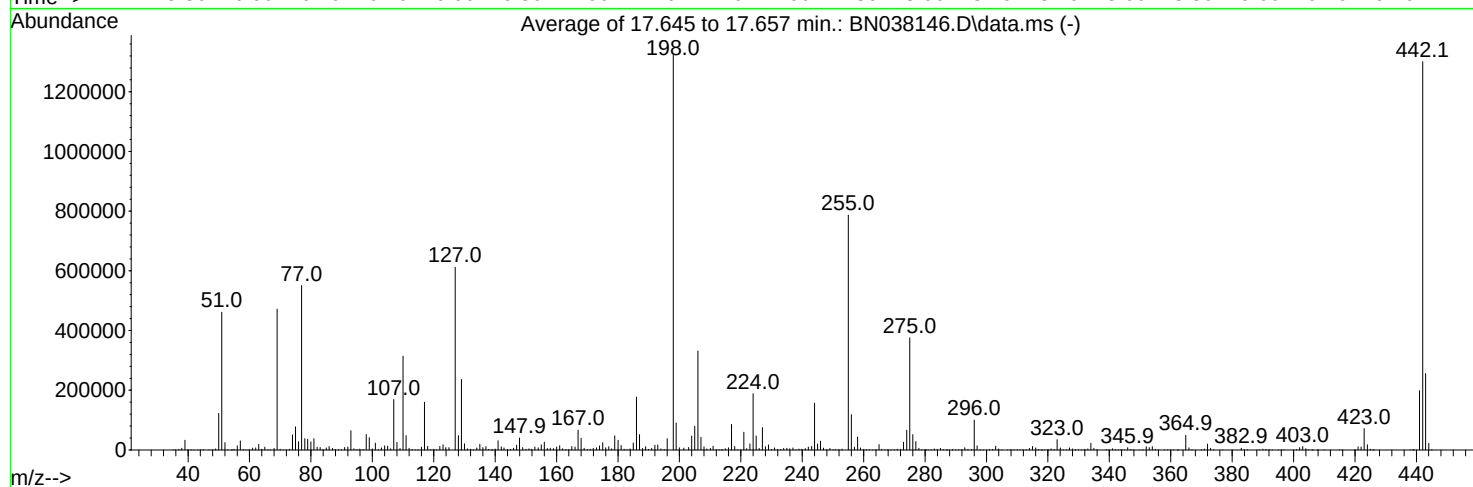


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110725\
Data File : BN038146.D
Acq On : 07 Nov 2025 09:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 29 13:09:46 2025

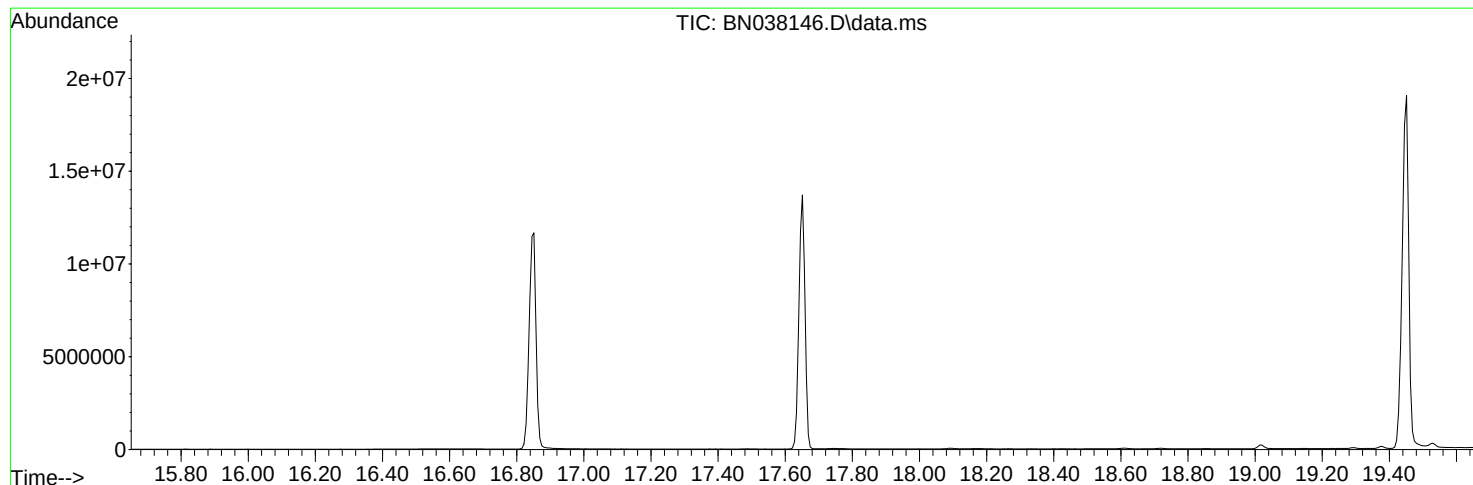




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2467

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.1	5202	PASS
69	69	100	100	100.0	472117	PASS
70	69	0.00	2	0.5	2484	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1322837	PASS
199	198	5	9	6.8	90568	PASS
365	198	1	100	3.7	49155	PASS
441	443	0.01	150	77.5	198677	PASS
442	442	100	100	100.0	1300779	PASS
443	442	15	24	19.7	256235	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110725\
Data File : BN038146.D
Acq On : 07 Nov 2025 09:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 07 09:43:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 07 09:43:12 2025
Response via : Initial Calibration

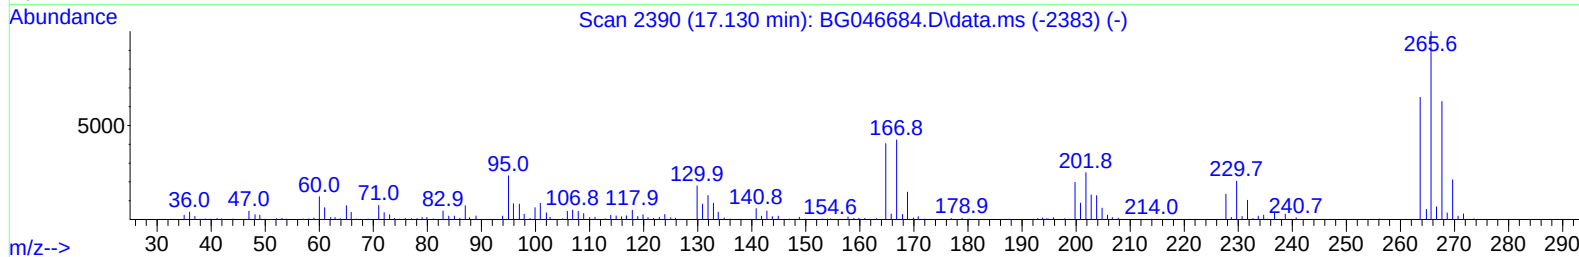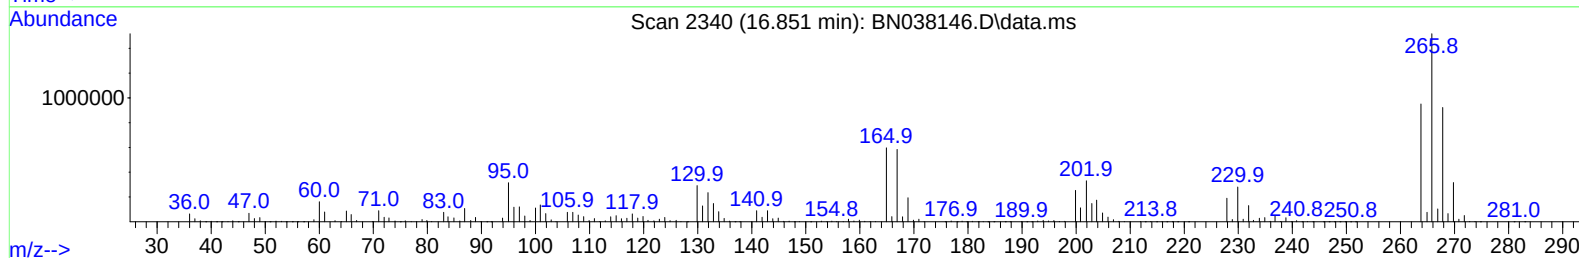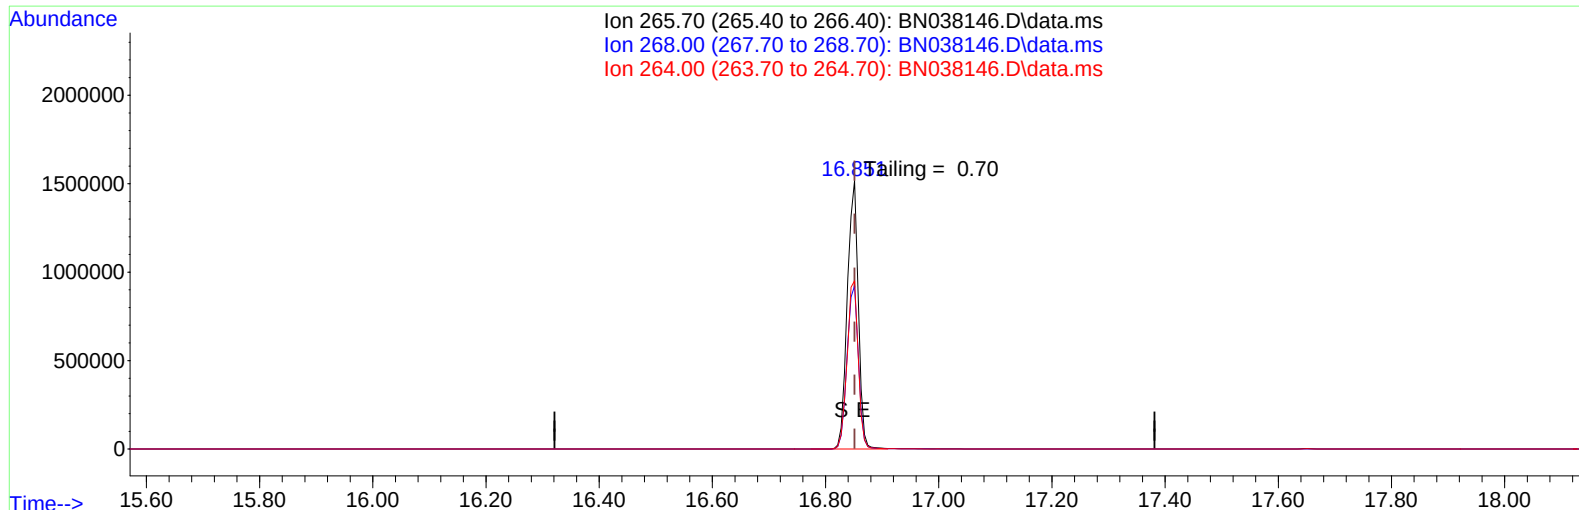

TIC: BN038146.D\data.ms

(70) Pentachlorophenol (C)

16.851min (0.000) 278.07 ng




response 2058575

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.80
264.00	61.60	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110725\
Data File : BN038146.D
Acq On : 07 Nov 2025 09:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 07 09:43:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 07 09:43:12 2025
Response via : Initial Calibration

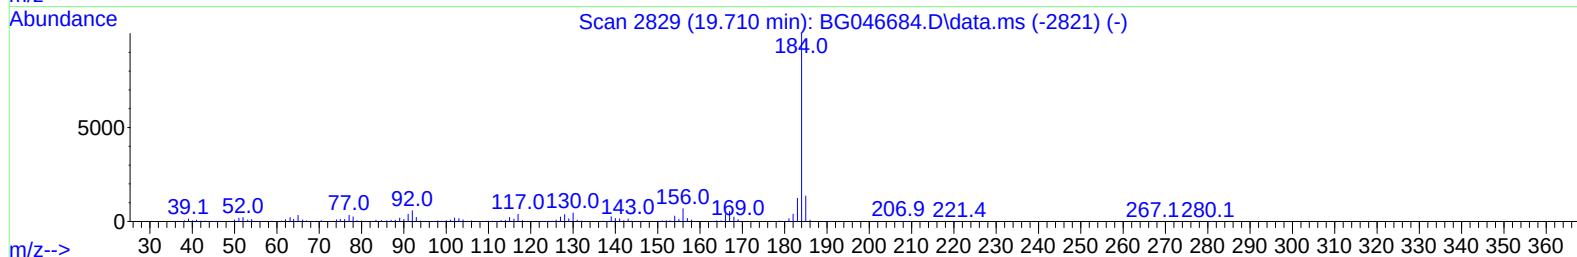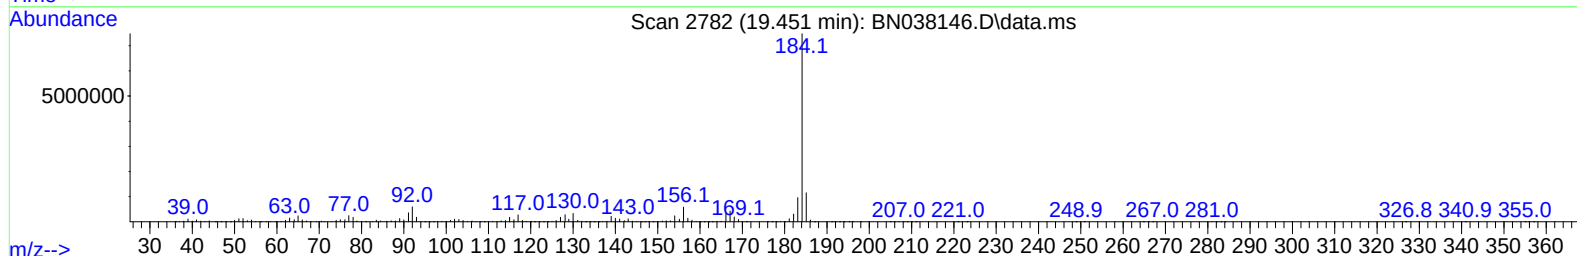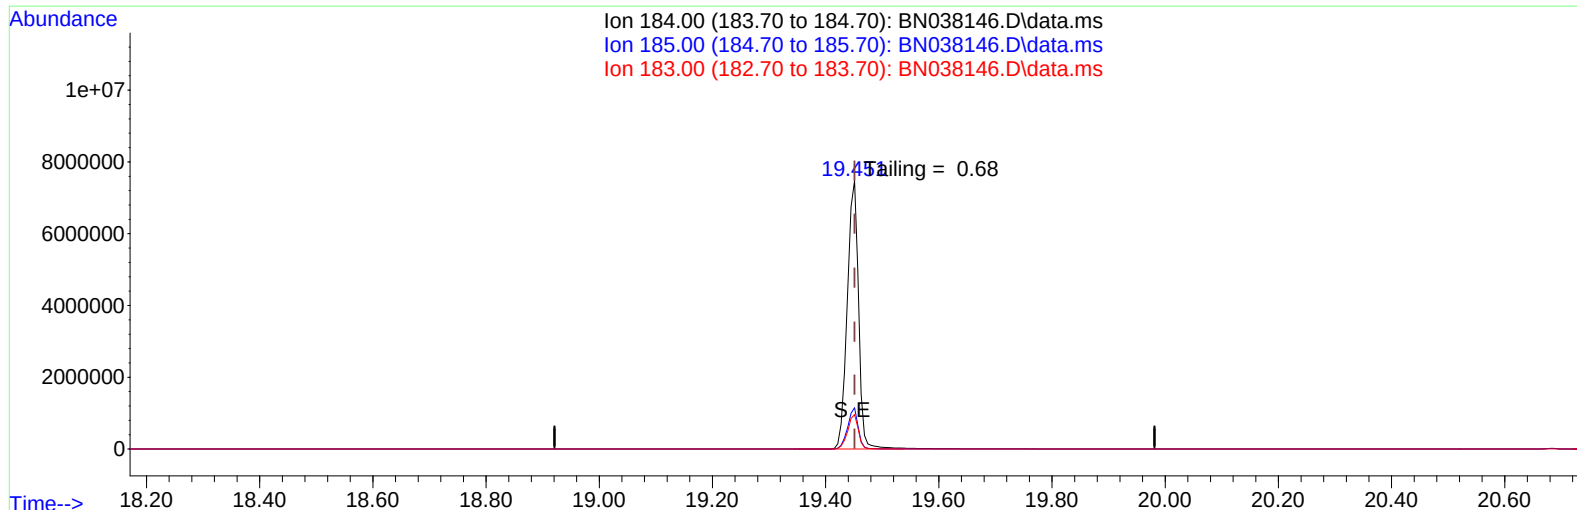

TIC: BN038146.D\data.ms

(77) Benzidine

19.451min (0.000) 0.00 ng

response 10437790

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.39
183.00	13.20	12.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2025	BNA_N	<u>BN038146.D</u>
Compound Name	Response	Retention Time
DDT	5230342	20.686
DDD	41900	20.239
DDE	3070	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44970	5275312	0.85

Instrument :
BNA_N
ClientSampleId :
DFTPP