
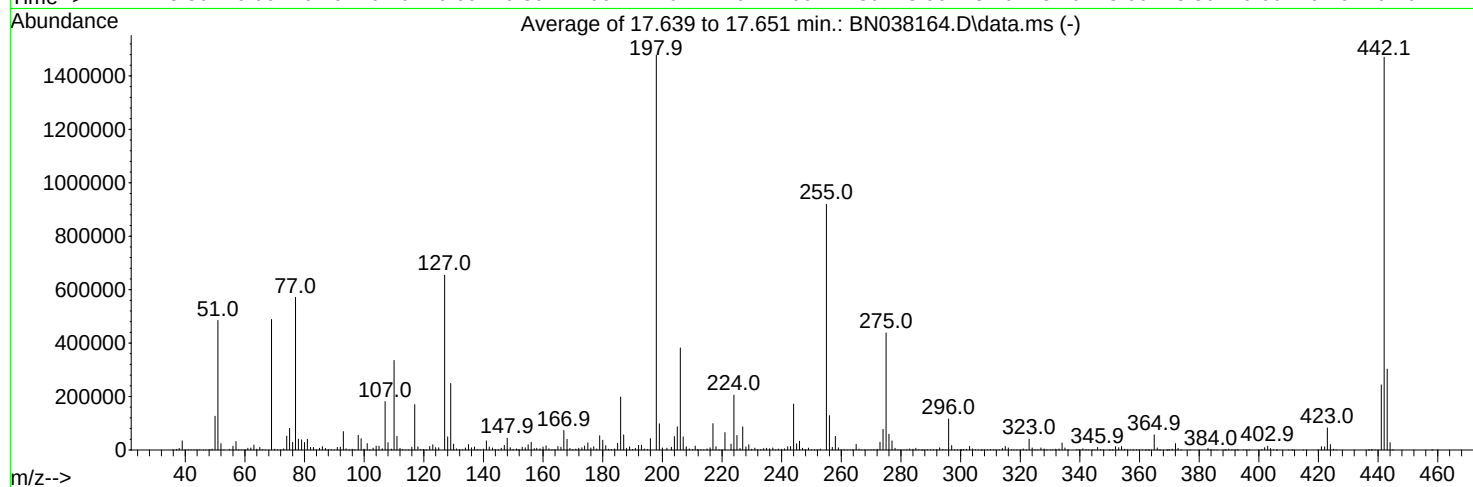


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110725\
Data File : BN038164.D
Acq On : 07 Nov 2025 21:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 29 13:09:46 2025

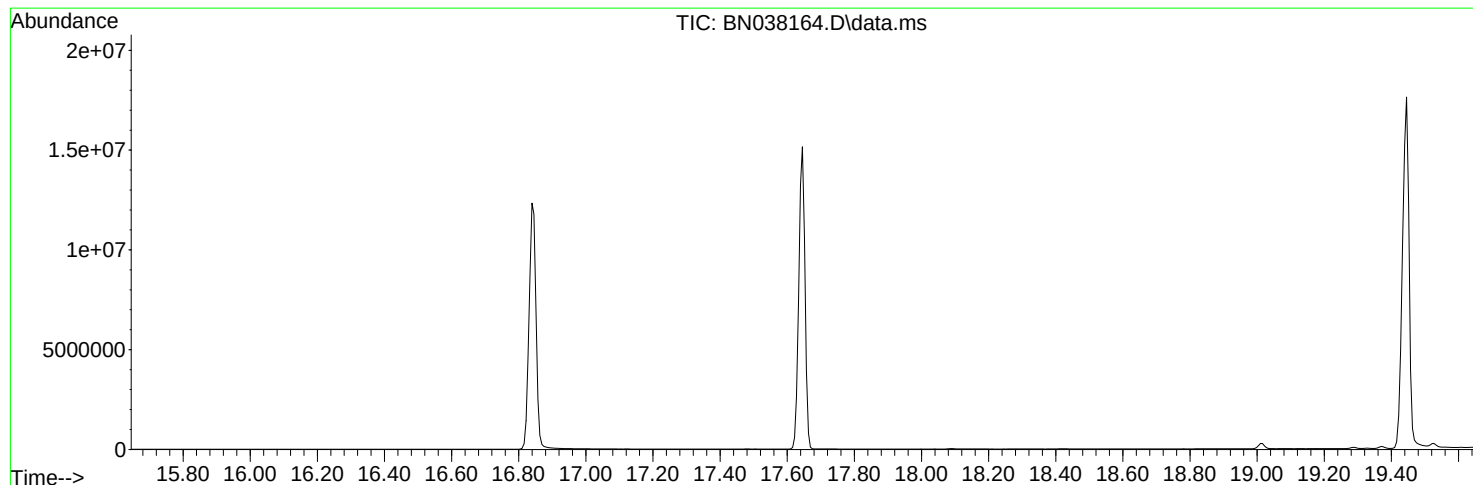




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	488379	PASS
70	69	0.00	2	0.5	2561	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1477973	PASS
199	198	5	9	6.6	97949	PASS
365	198	1	100	3.8	56592	PASS
441	443	0.01	150	80.4	243627	PASS
442	442	100	100	100.0	1469952	PASS
443	442	15	24	20.6	303061	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110725\
Data File : BN038164.D
Acq On : 07 Nov 2025 21:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 08 04:08:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 08 04:08:47 2025
Response via : Initial Calibration

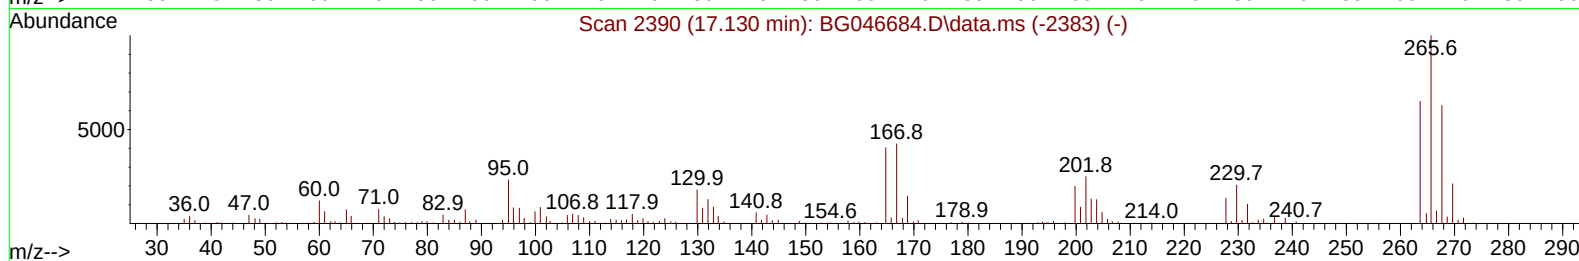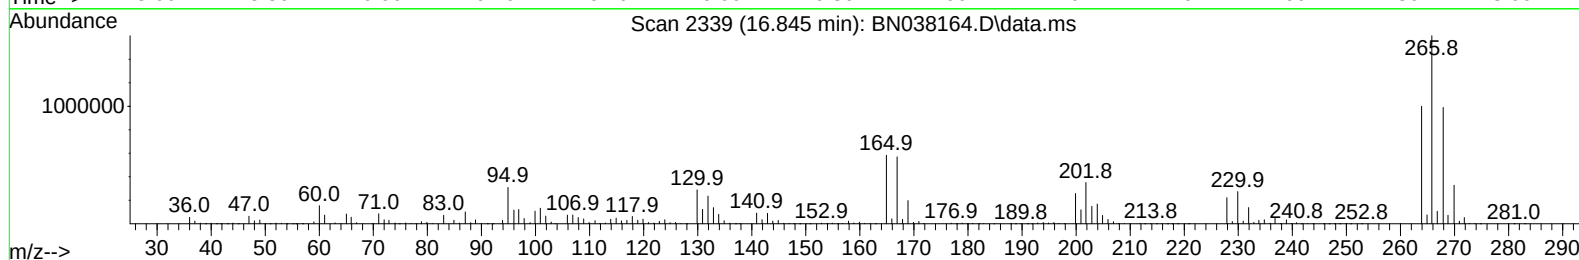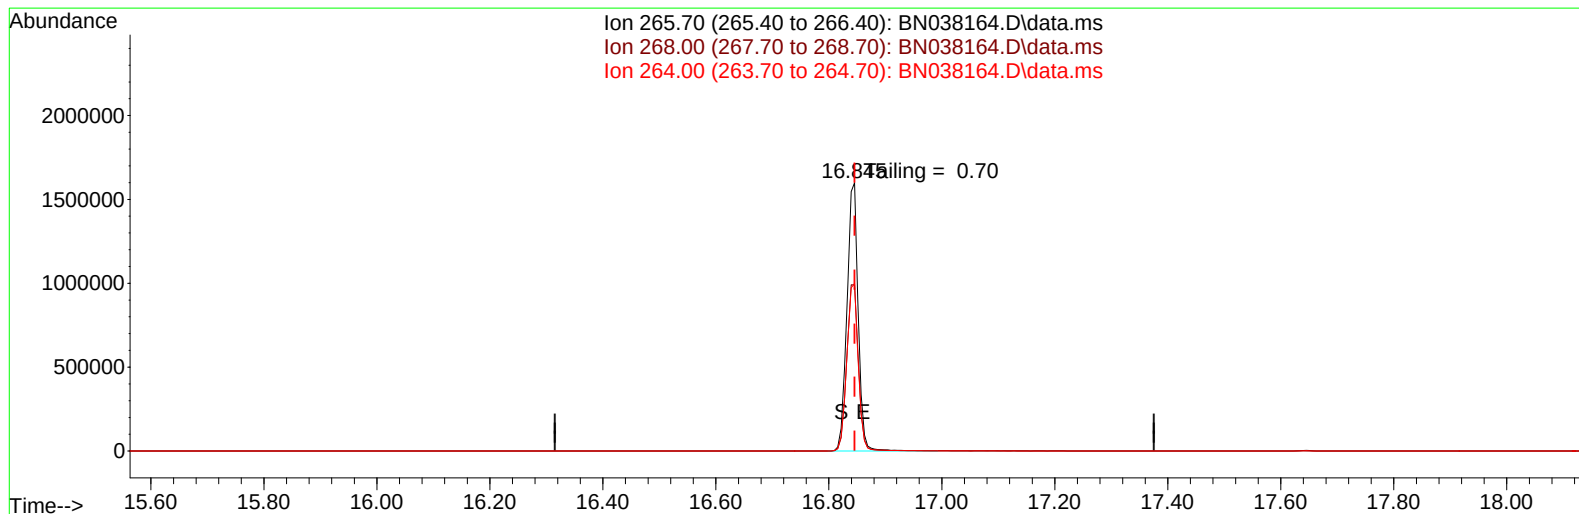

TIC: BN038164.D\data.ms

(70) Pentachlorophenol (C)

16.845min (0.000) 236023.12 ng




response 2207882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.90
264.00	61.60	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110725\
Data File : BN038164.D
Acq On : 07 Nov 2025 21:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 08 04:08:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 08 04:08:47 2025
Response via : Initial Calibration

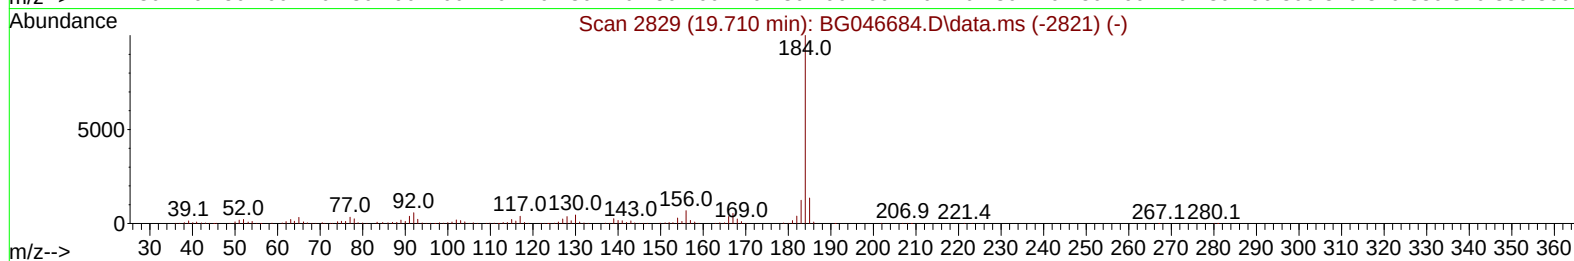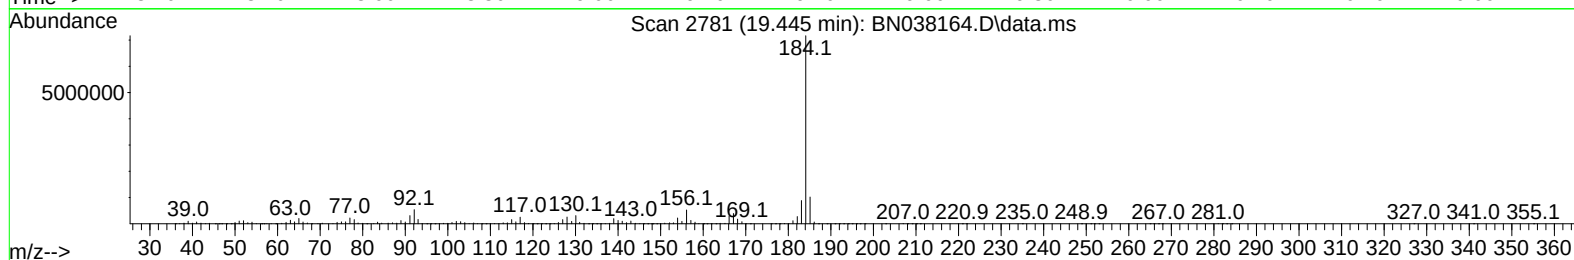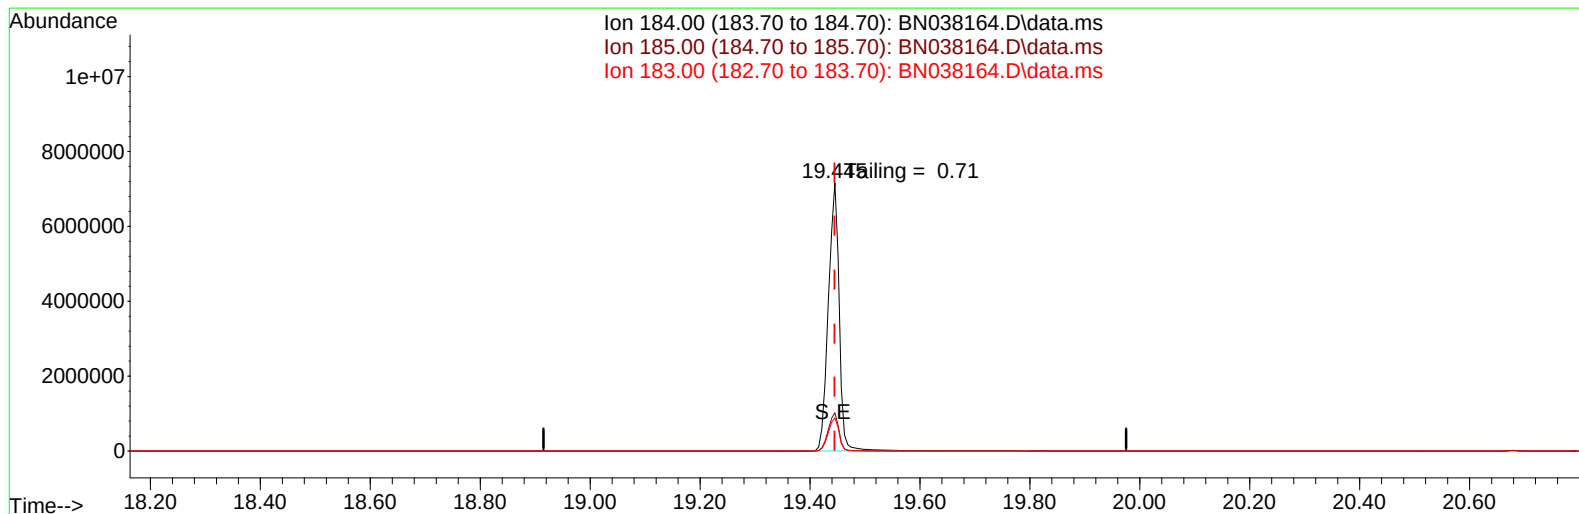

TIC: BN038164.D\data.ms

(77) Benzidine

19.445min (0.000) 4251.91 ng m

response 9910482

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.24
183.00	13.20	12.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2025	BNA_N	<u>BN038164.D</u>
Compound Name	Response	Retention Time
DDT	4972953	20.68
DDD	128730	20.233
DDE	11311	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
140041	5112994	2.74

Instrument :
BNA_N
ClientSampleId :
DFTPP