


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111025\
Data File : BN038173.D
Acq On : 10 Nov 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 29 13:09:46 2025

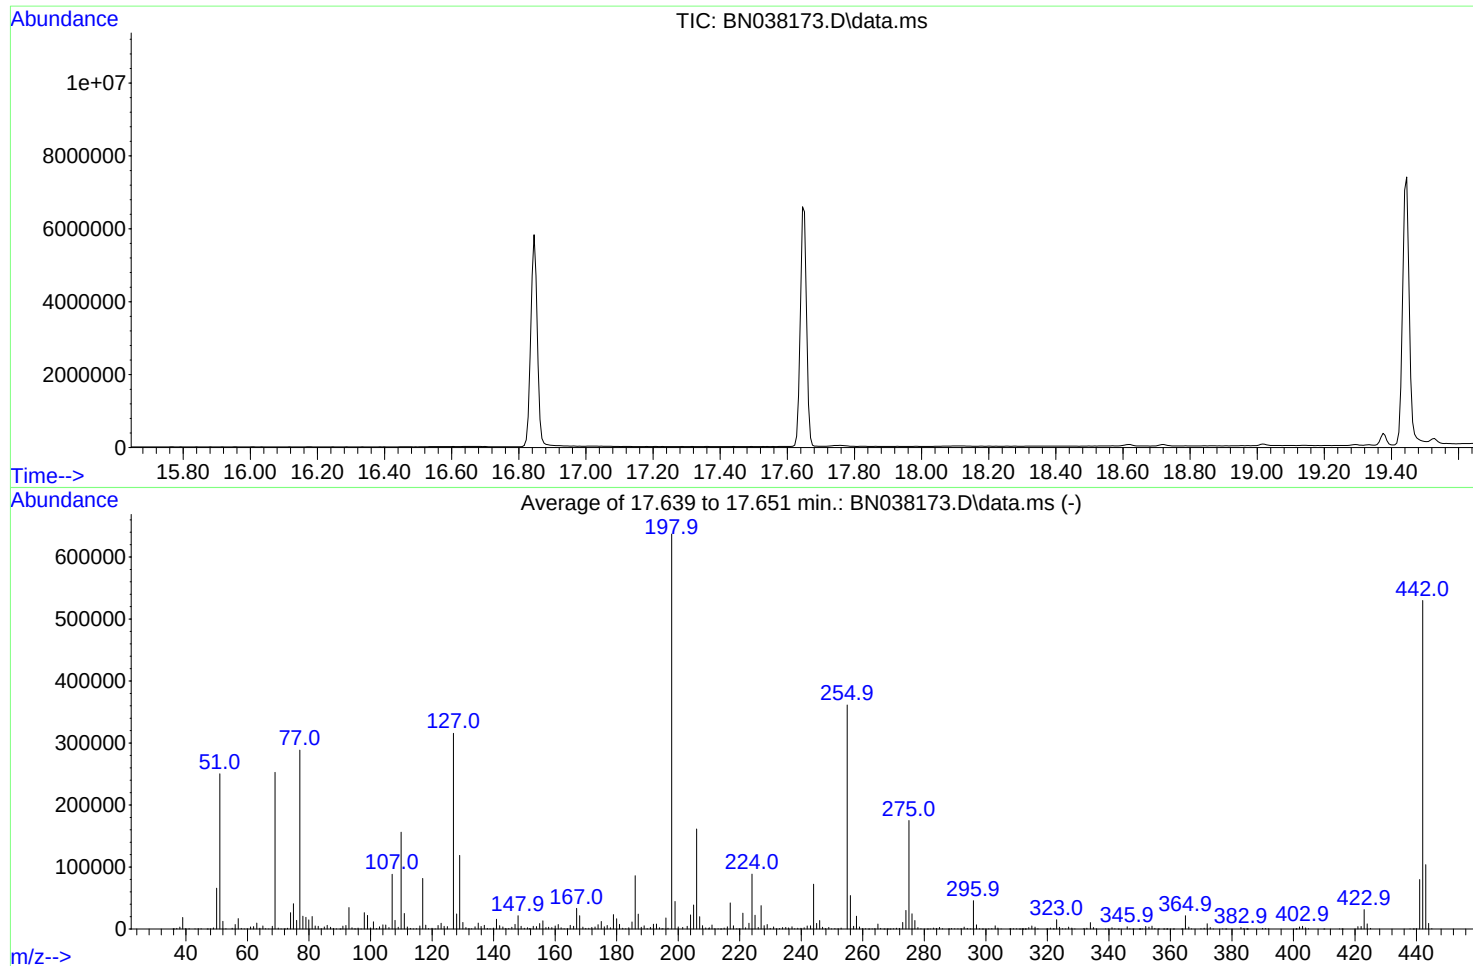

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	4319	PASS
69	69	100	100	100.0	252715	PASS
70	69	0.00	2	0.6	1513	PASS
197	198	0.00	2	0.2	1239	PASS
198	198	100	100	100.0	636949	PASS
199	198	5	9	7.0	44288	PASS
365	198	1	100	3.4	21461	PASS
441	443	0.01	150	76.8	79795	PASS
442	442	100	100	100.0	529877	PASS
443	442	15	24	19.6	103875	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/10/2025	BNA_N	<u>BN038173.D</u>
Compound Name	Response	Retention Time
DDT	2452624	20.68
DDD	63755	20.239
DDE	8751	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
72506	2525130	2.87

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111025\
Data File : BN038173.D
Acq On : 10 Nov 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 10 10:10:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 10 10:10:34 2025
Response via : Initial Calibration

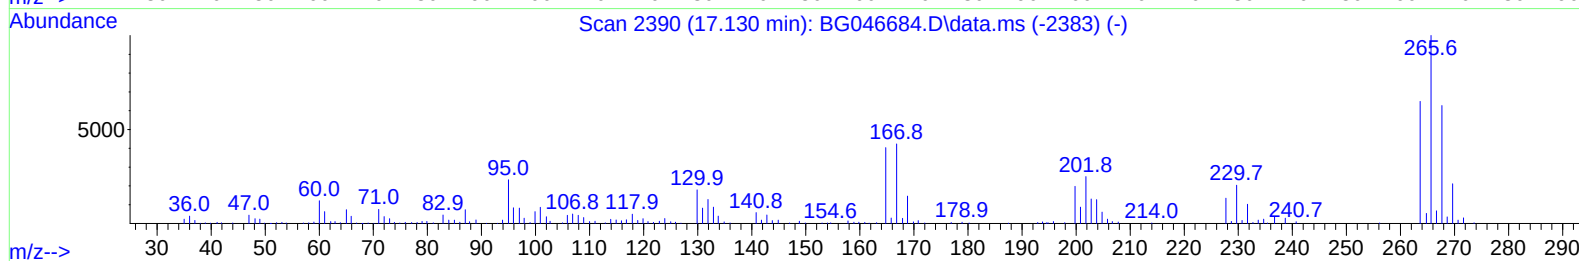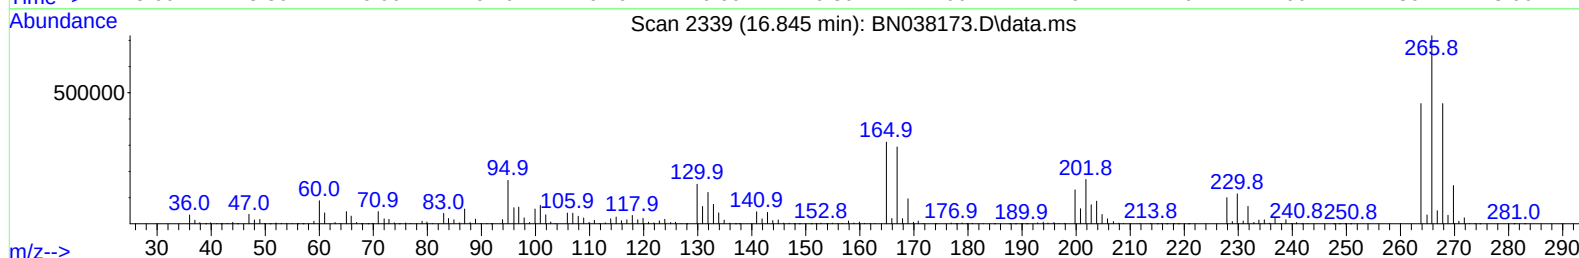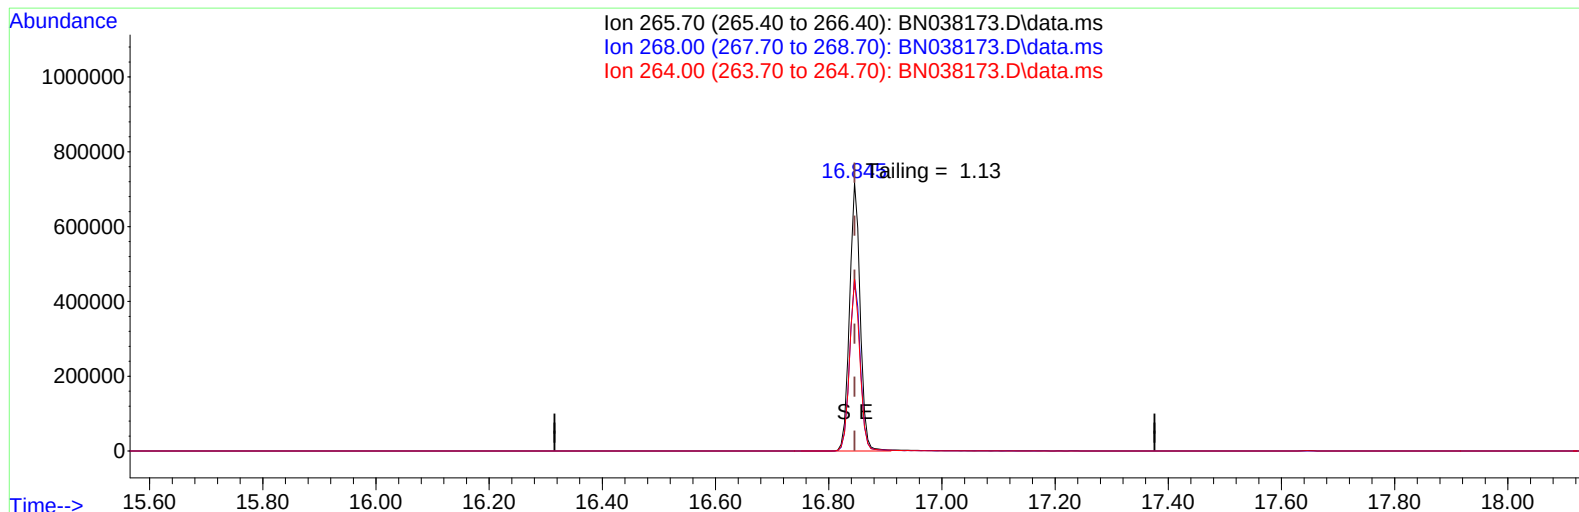

TIC: BN038173.D\data.ms

(70) Pentachlorophenol (C)

16.845min (0.000) 277.71 ng




response 940981

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.90
264.00	61.60	63.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111025\
Data File : BN038173.D
Acq On : 10 Nov 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 10 10:10:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 10 10:10:34 2025
Response via : Initial Calibration

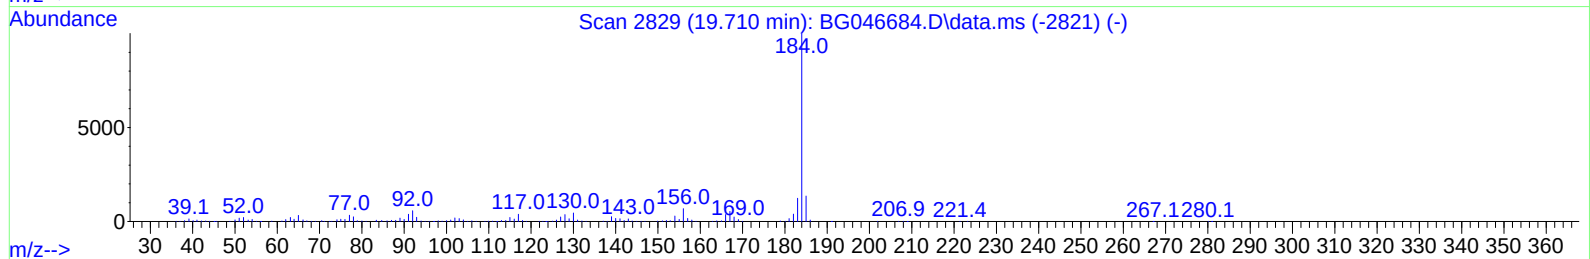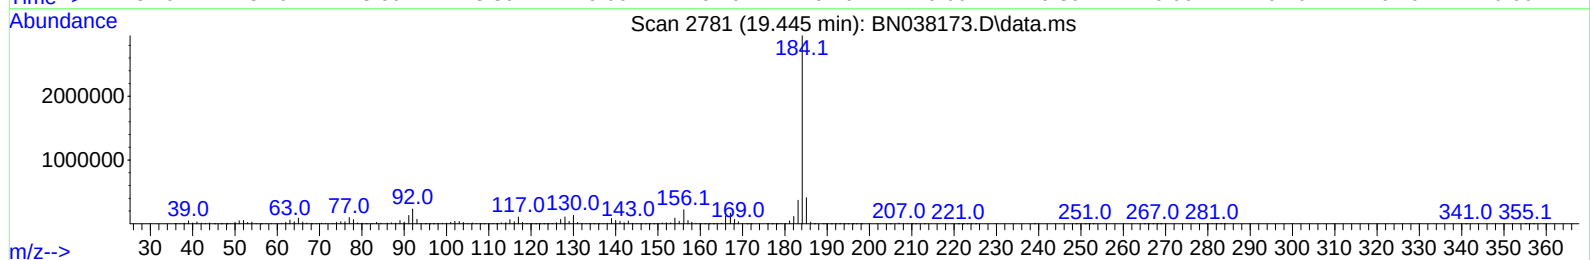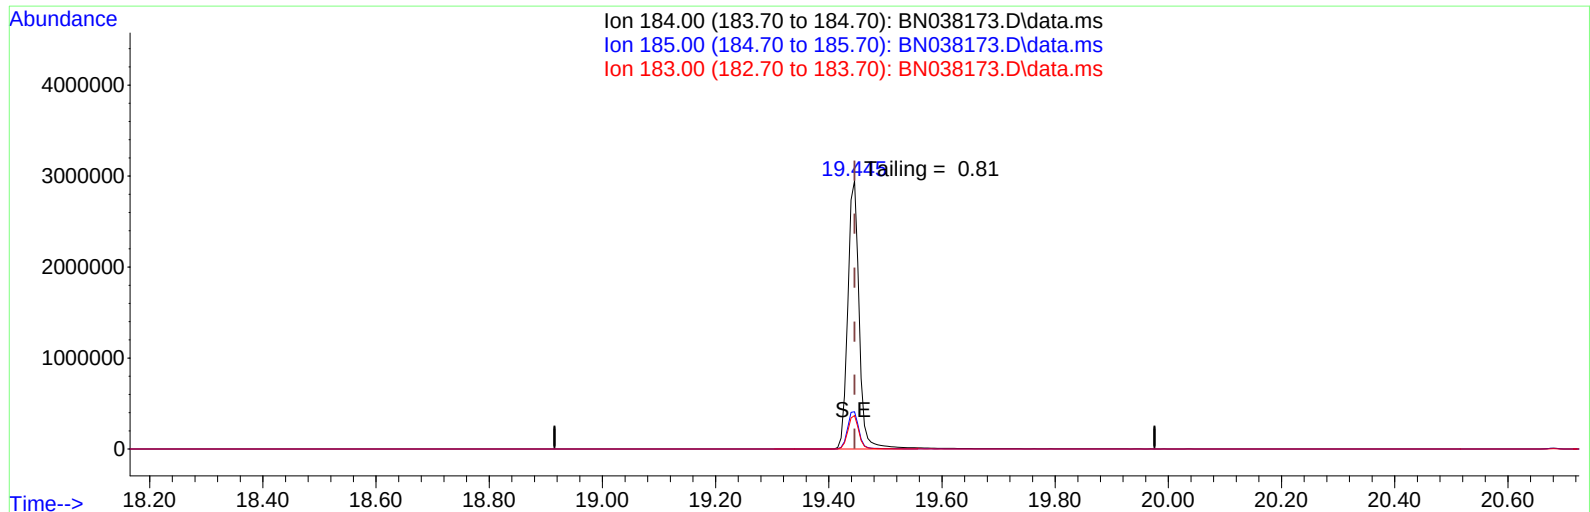

TIC: BN038173.D\data.ms

(77) Benzidine

19.445min (0.000) 280.15 ng

response 4168590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	12.49
0.00	0.00	0.00