


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110625\
Data File : BG064698.D
Acq On : 6 Nov 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 03 18:16:26 2025

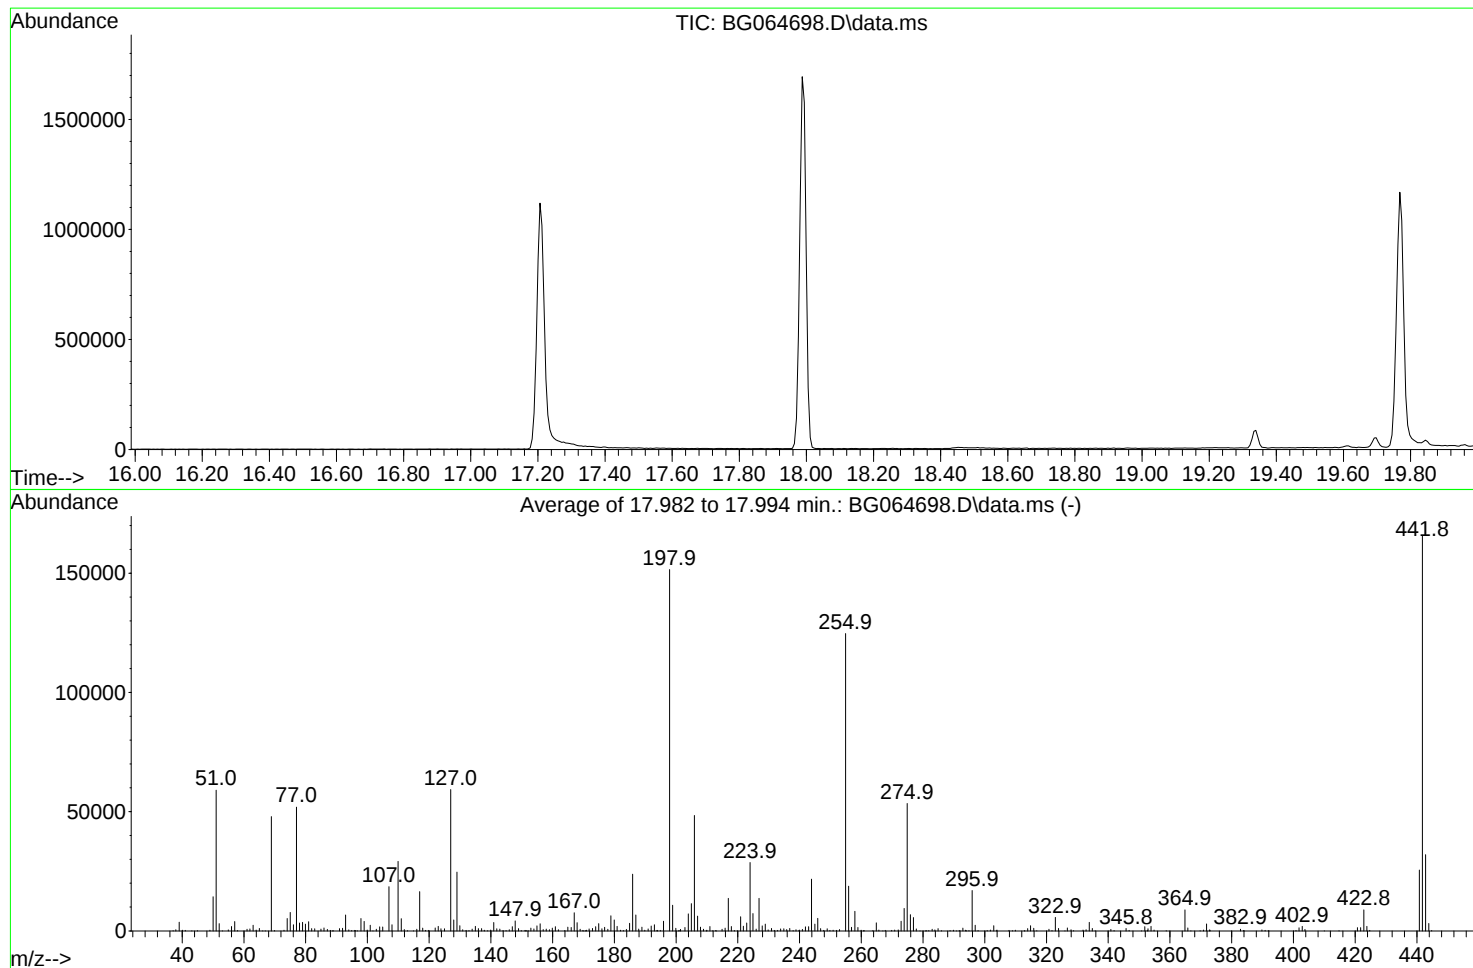




AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	47968	PASS
70	69	0.00	2	0.3	164	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	151528	PASS
199	198	5	9	7.1	10749	PASS
365	198	1	100	5.8	8816	PASS
441	443	0.01	150	79.9	25541	PASS
442	442	100	100	100.0	165560	PASS
443	442	15	24	19.3	31960	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110625\
Data File : BG064698.D
Acq On : 6 Nov 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 06 12:08:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

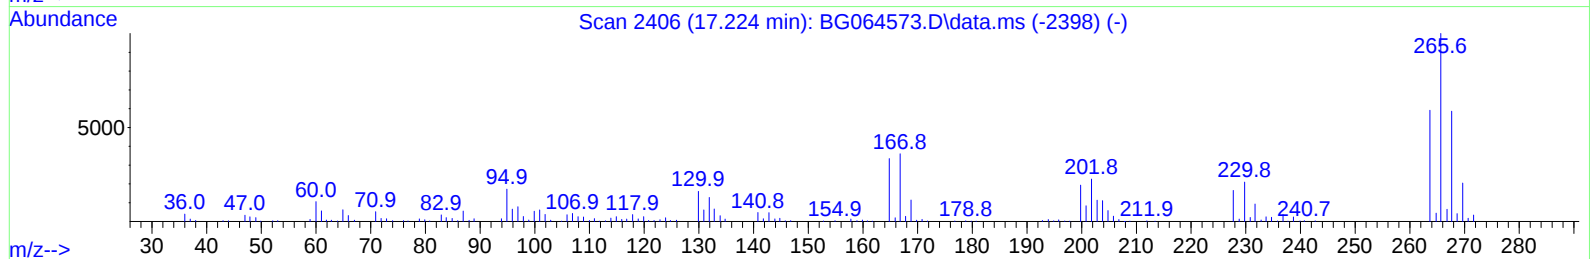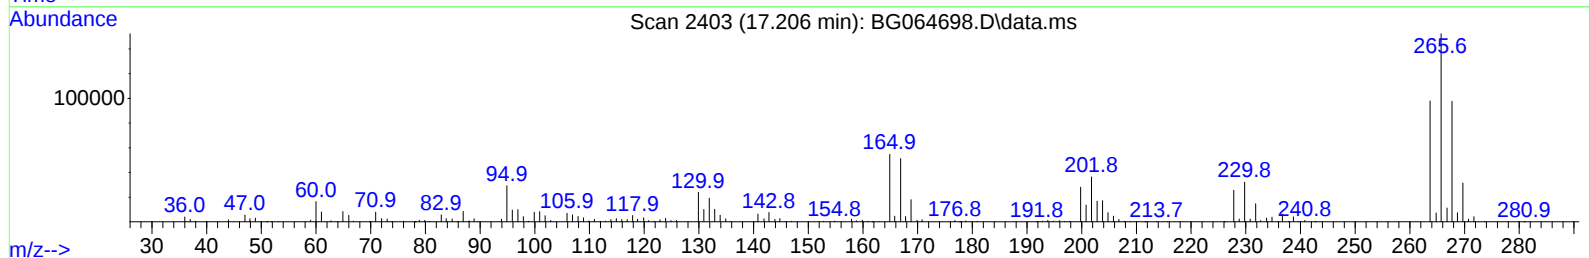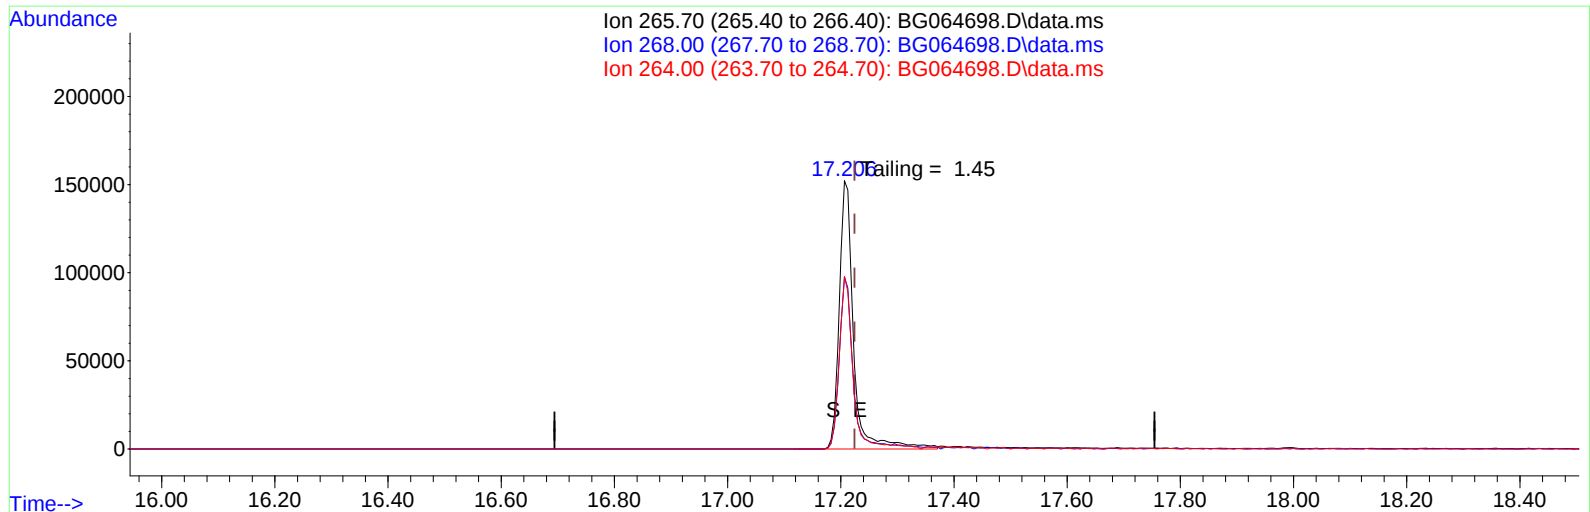

TIC: BG064698.D\data.ms

(70) Pentachlorophenol (C)

17.206min (-0.018) 138576.30 ng




response 268700

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	69.06
264.00	59.10	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110625\
Data File : BG064698.D
Acq On : 6 Nov 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 06 12:08:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

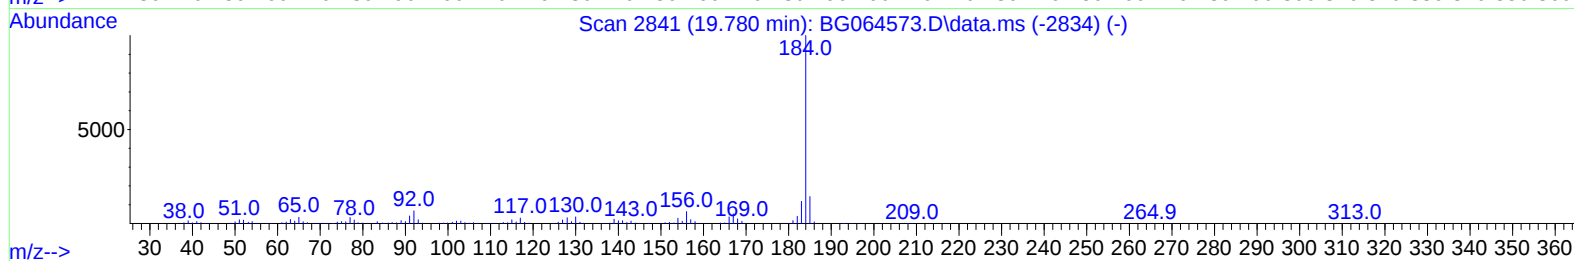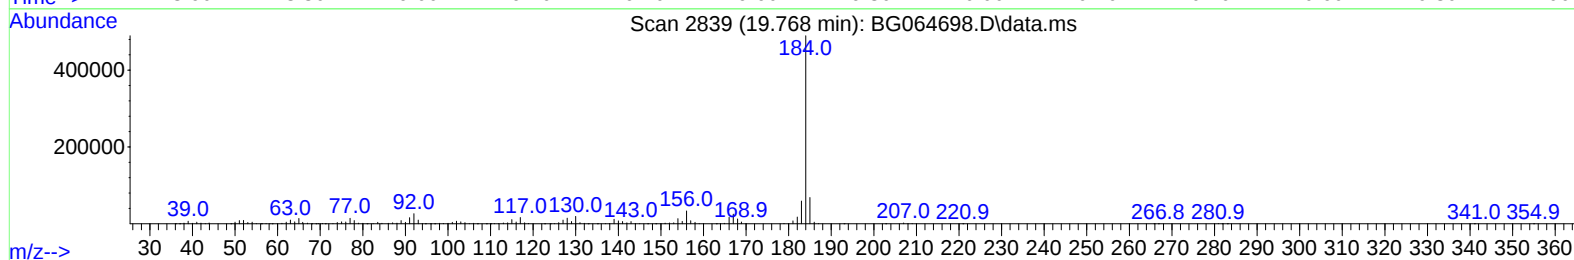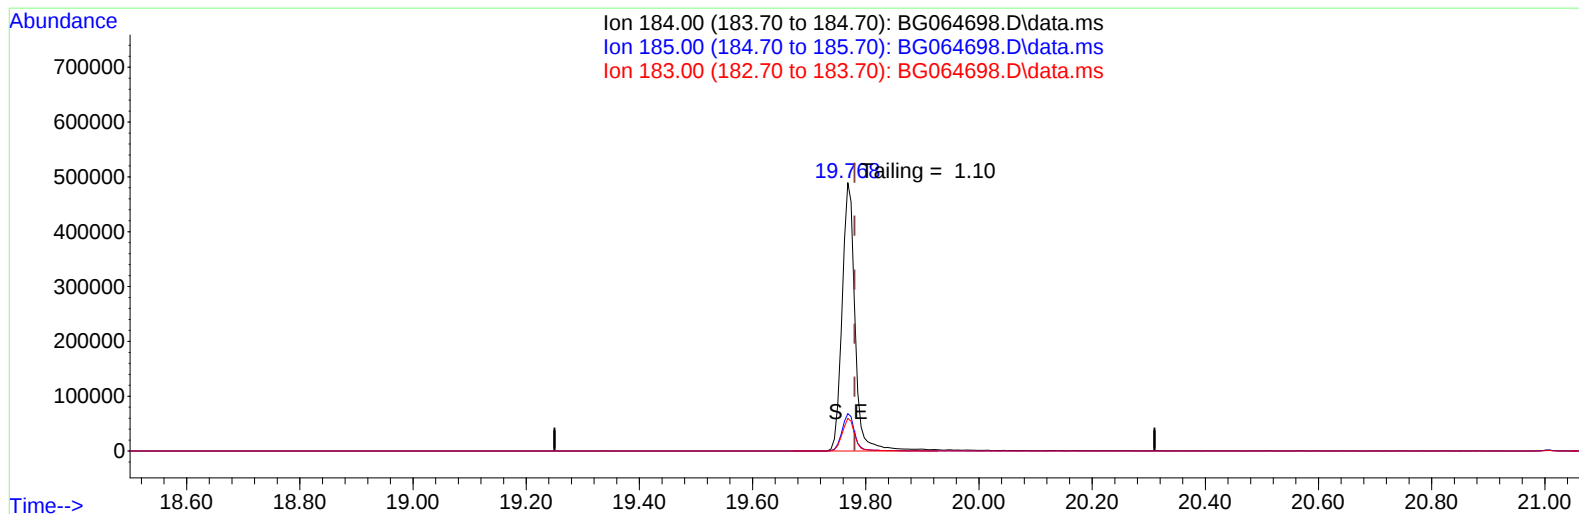

TIC: BG064698.D\data.ms

(77) Benzidine

19.768min (-0.012) 39040.29 ng

response 778451

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.96
183.00	11.80	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/6/2025	BNA_G	<u>BG064698.D</u>
Compound Name	Response	Retention Time
DDT	527950	21.008
DDD	16253	20.555
DDE	64	19.709
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16317	544267	3.00

Instrument :
BNA_G
ClientSampleId :
DFTPP