


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP110625\  
Data File : BP026075.D  
Acq On : 06 Nov 2025 12:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP102925.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Oct 30 11:51:34 2025

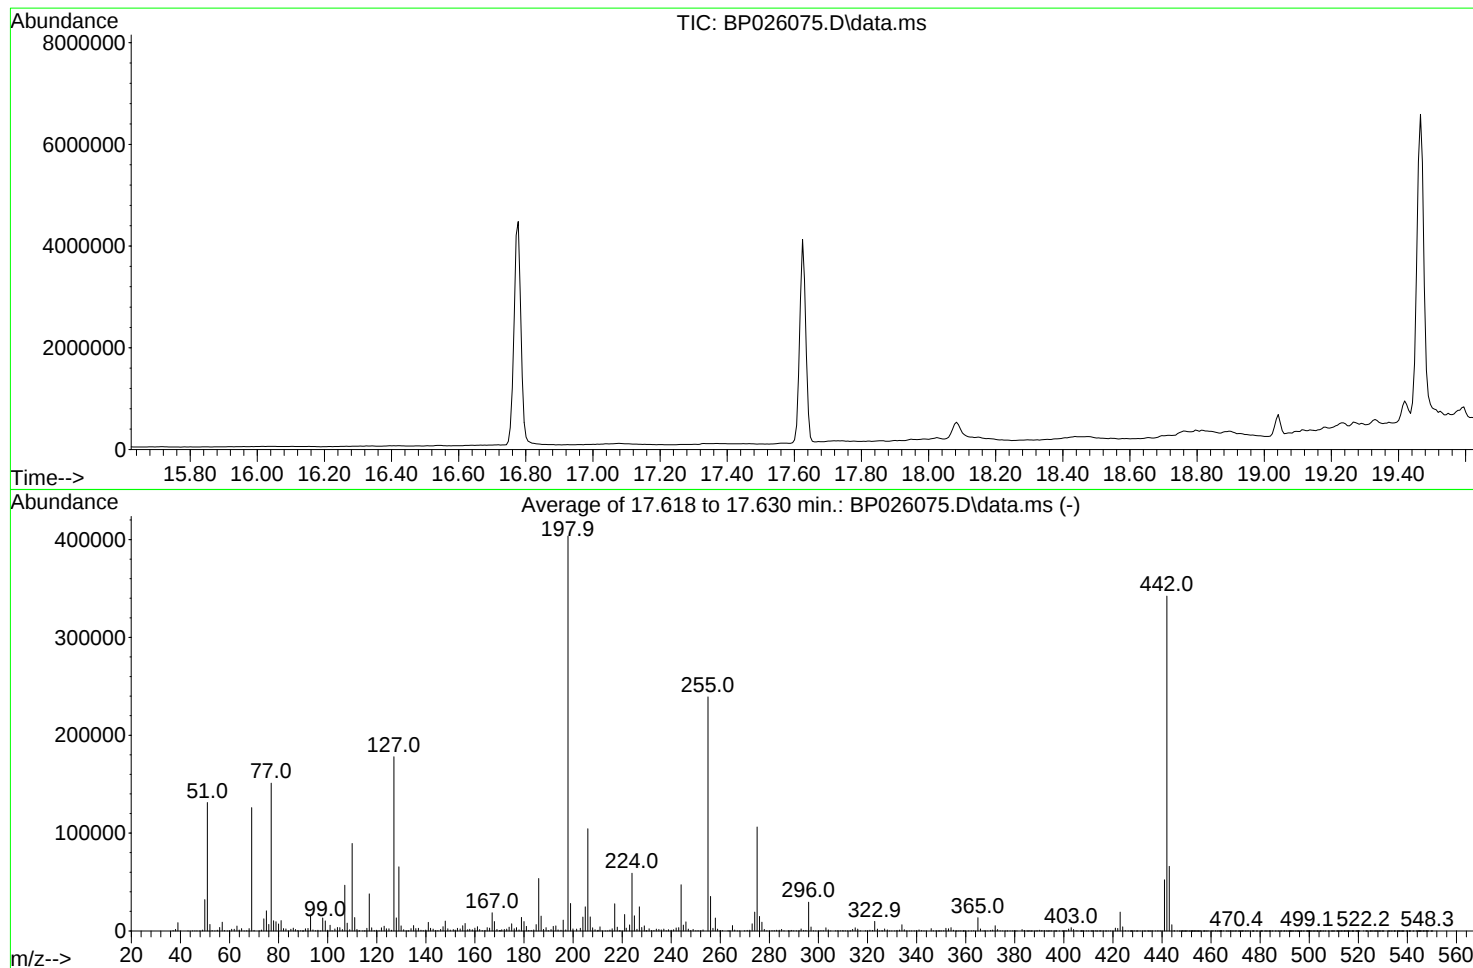




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 68             | 69              | 0.00            | 2               | 1.8          | 2308       | PASS                |
| 69             | 69              | 100             | 100             | 100.0        | 126049     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 614        | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 1149       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 403539     | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 28122      | PASS                |
| 365            | 198             | 1               | 100             | 3.4          | 13536      | PASS                |
| 441            | 443             | 0.01            | 150             | 79.1         | 52220      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 342246     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 66054      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP110625\  
Data File : BP026075.D  
Acq On : 06 Nov 2025 12:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Nov 06 14:04:39 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP102925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 30 11:51:34 2025  
Response via : Initial Calibration

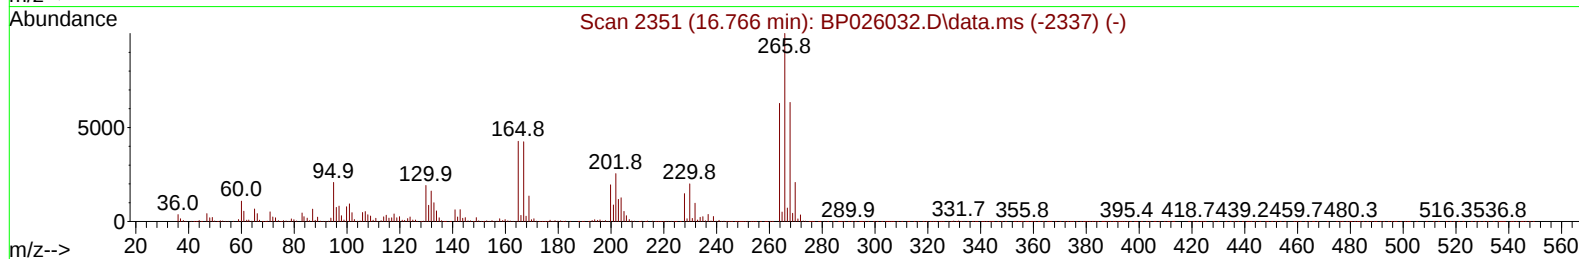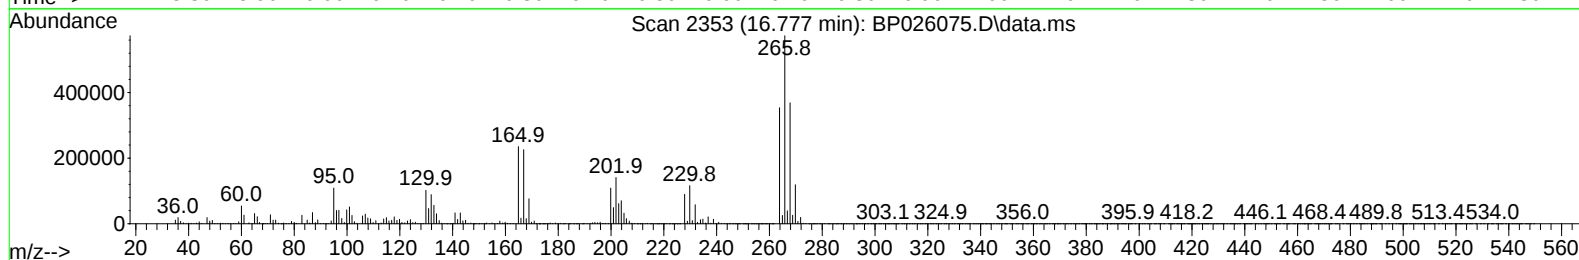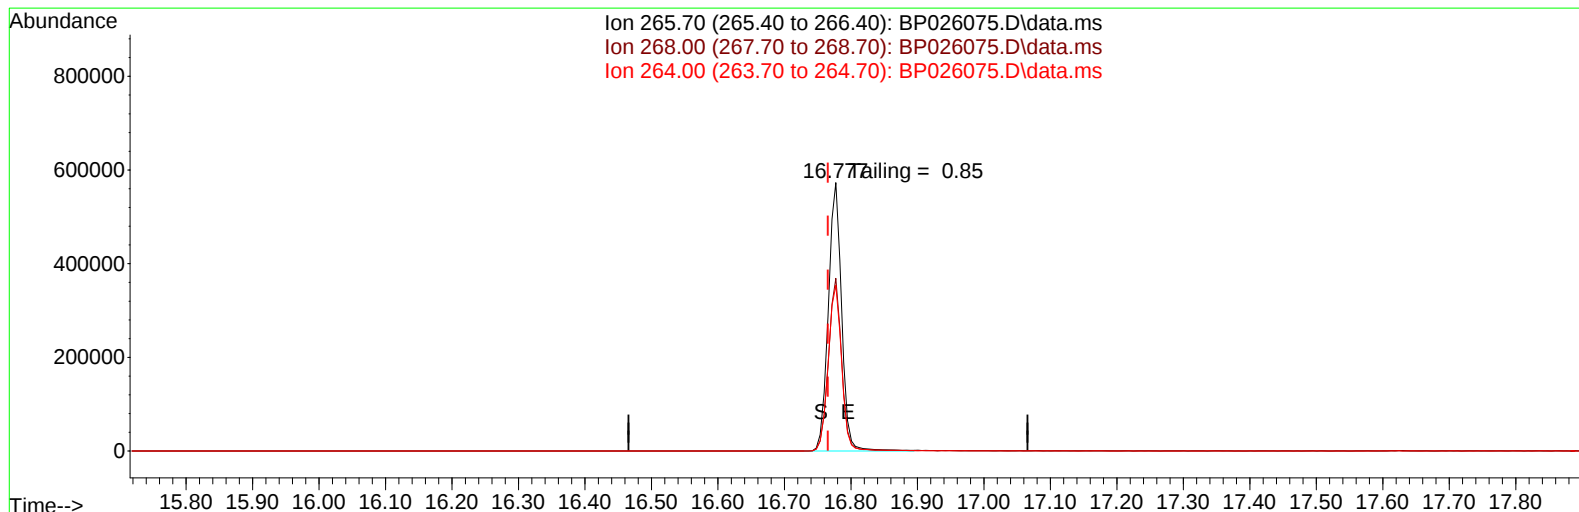

TIC: BP026075.D\data.ms

**(70) Pentachlorophenol (C)**

**16.777min (+ 0.012) 88742.13 ng**




**response 797426**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.30  | 64.36  |
| 264.00 | 62.80  | 61.69  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP110625\  
Data File : BP026075.D  
Acq On : 06 Nov 2025 12:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Nov 06 14:04:39 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP102925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 30 11:51:34 2025  
Response via : Initial Calibration

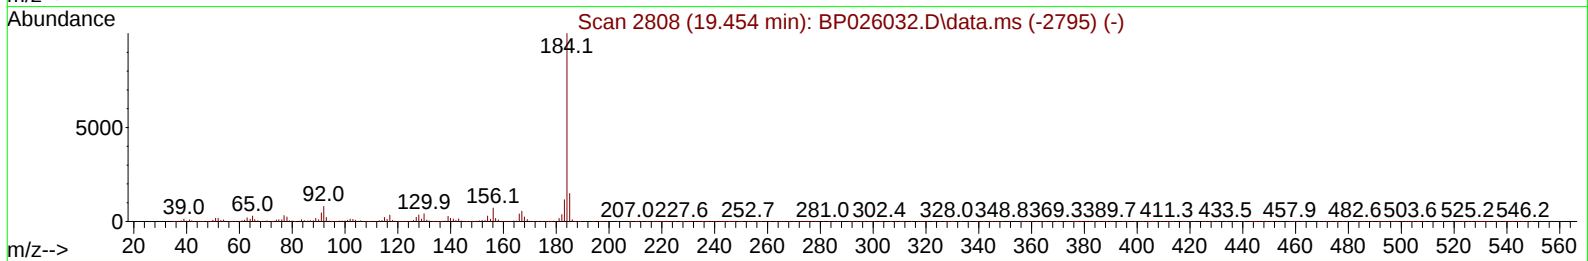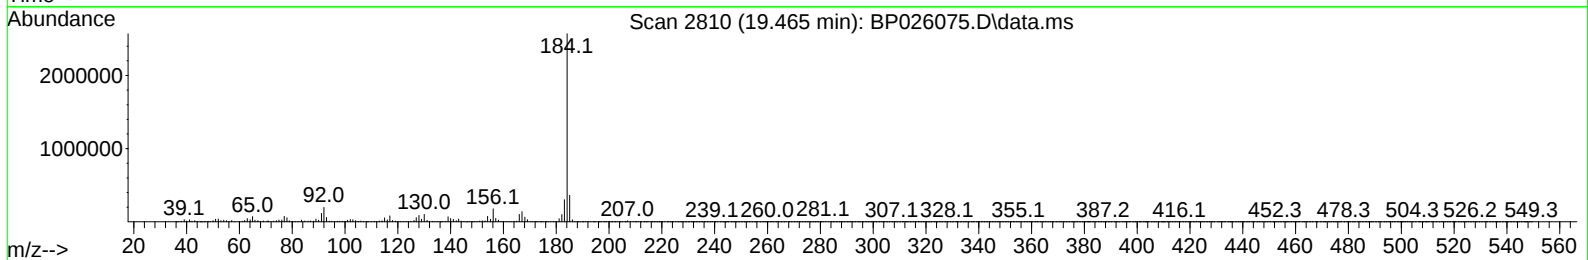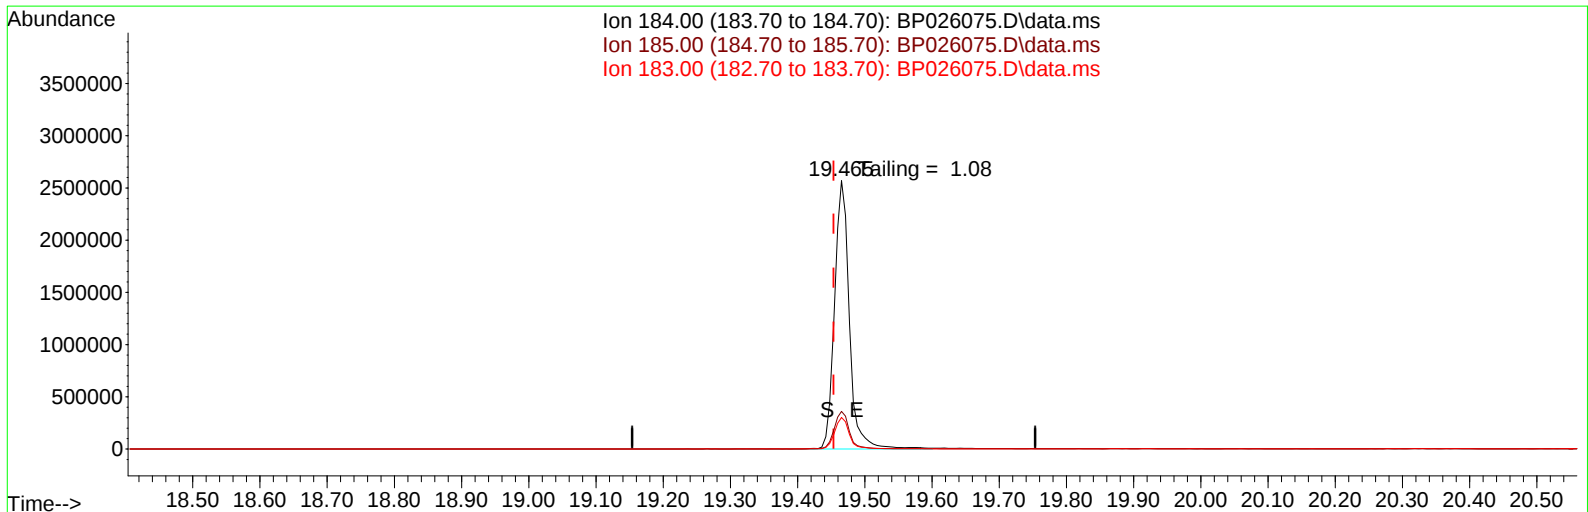

TIC: BP026075.D\data.ms

(77) Benzidine

19.465min (+ 0.012) 35734.65 ng

response 3913872

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 14.04  |
| 183.00 | 11.50  | 11.78  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/6/2025     | BNA_P            | <u>BP026075.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1775922          | 20.765             |
| DDD           | 39010            | 20.307             |
| DDE           | 3948             | 19.777             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 42958         | 1818880          | 2.36               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP