

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110625\
Data File : BP026081.D
Acq On : 06 Nov 2025 17:45
Operator : RC/JU
Sample : Q3534-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-1

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP026081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.855	317	326	331	rBV	12342431	19885082	100.00%	21.125%
2	5.296	395	401	408	rBV	3409556	4773446	24.01%	5.071%
3	6.849	659	665	674	rBV	1936686	2976072	14.97%	3.162%
4	7.678	798	806	813	rBV	961665	1557990	7.83%	1.655%
5	8.819	992	1000	1009	rBV	3235484	5085393	25.57%	5.402%
6	10.449	1270	1277	1294	rVB	1376759	2157045	10.85%	2.292%
7	12.931	1691	1699	1705	rBV	7634552	11010923	55.37%	11.697%
8	14.319	1929	1935	1947	rVB	1974724	2751816	13.84%	2.923%
9	15.831	2185	2192	2203	rBV	5204682	8634212	43.42%	9.173%
10	16.907	2369	2375	2382	rVB3	141536	213900	1.08%	0.227%
11	17.125	2405	2412	2420	rVB2	2329717	3252226	16.36%	3.455%
12	18.072	2568	2573	2581	rBV3	98173	227016	1.14%	0.241%
13	19.442	2798	2806	2817	rBV	2767161	3975709	19.99%	4.224%
14	19.860	2871	2877	2890	rVB	14215331	18654675	93.81%	19.818%
15	21.572	3161	3168	3178	rBV2	2346404	4209997	21.17%	4.472%
16	24.901	3725	3734	3745	rVB	1642197	4765476	23.97%	5.063%




Sum of corrected areas: 94130978

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110625\
Data File : BP026081.D
Acq On : 06 Nov 2025 17:45
Operator : RC/JU
Sample : Q3534-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

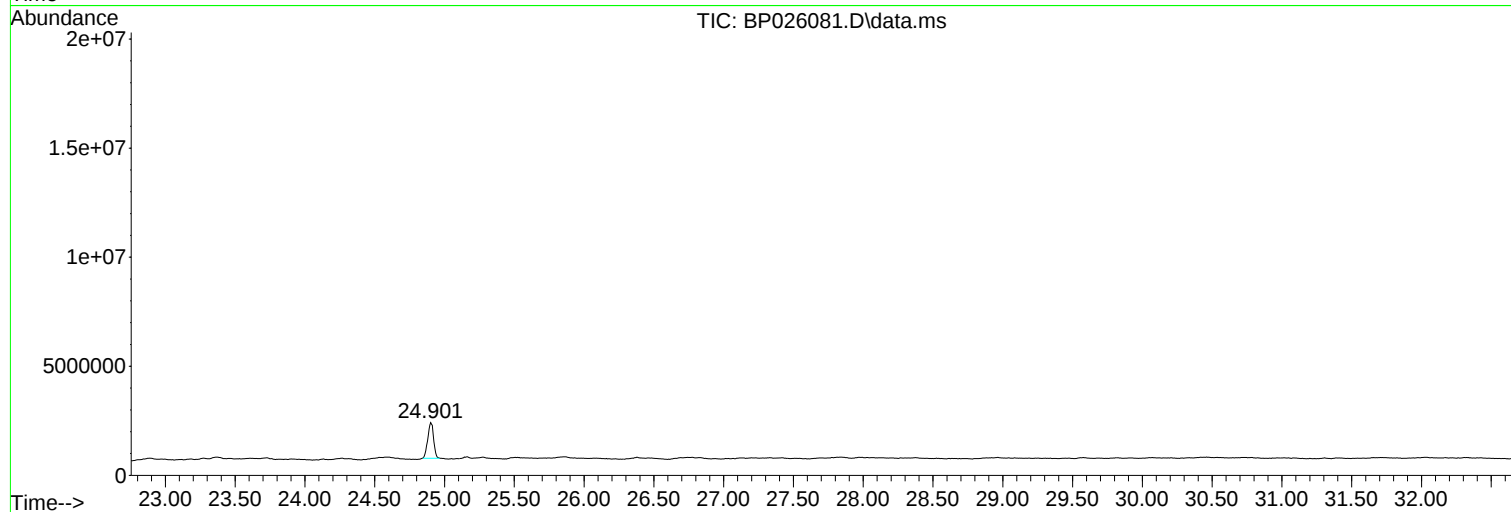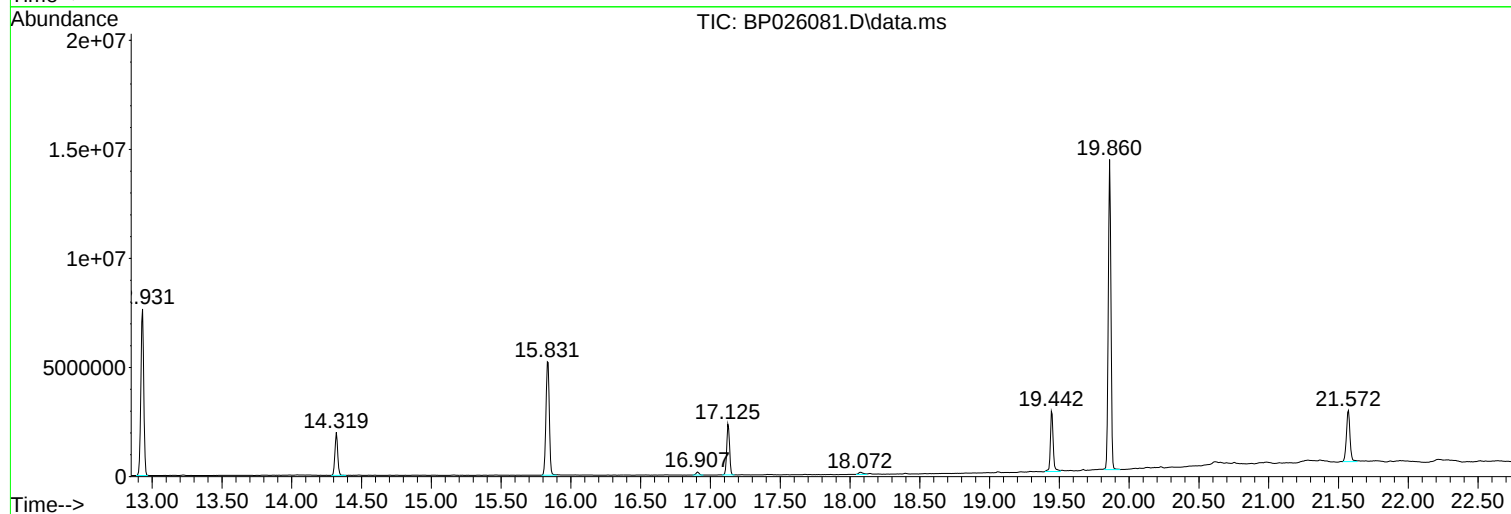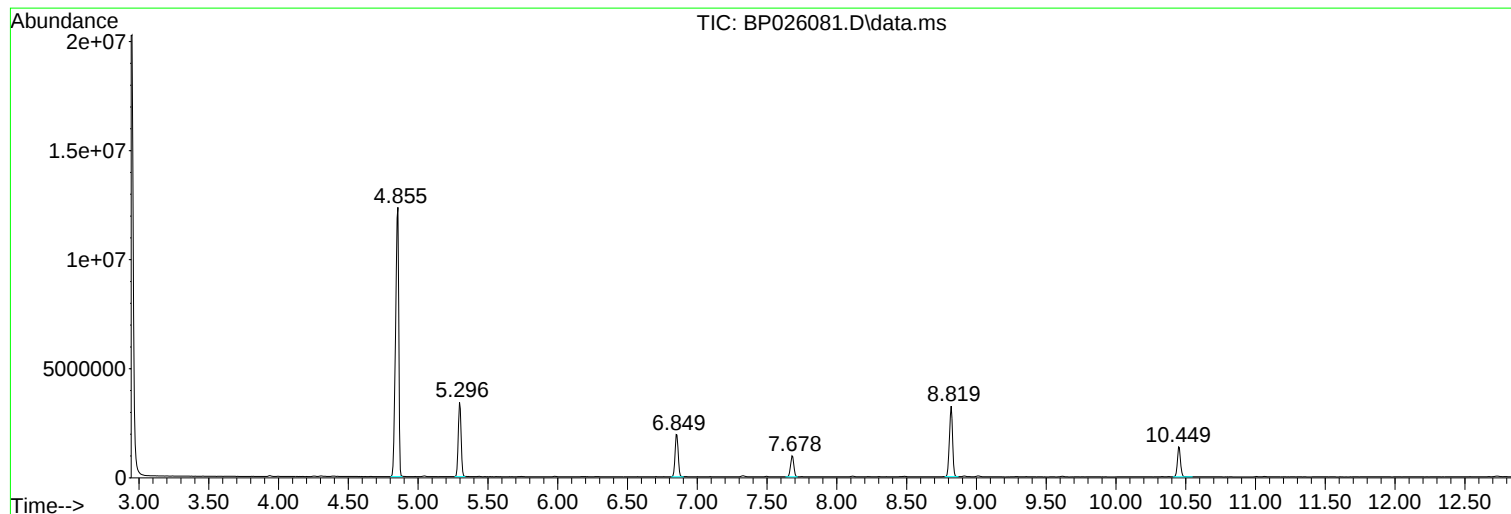

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110625\
Data File : BP026081.D
Acq On : 06 Nov 2025 17:45
Operator : RC/JU
Sample : Q3534-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110625\
Data File : BP026081.D
Acq On : 06 Nov 2025 17:45
Operator : RC/JU
Sample : Q3534-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------