


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110425\
Data File : VV039305.D
Acq On : 04 Nov 2025 10:24
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Title : SW846 8260
Last Update : Wed Oct 08 05:01:26 2025

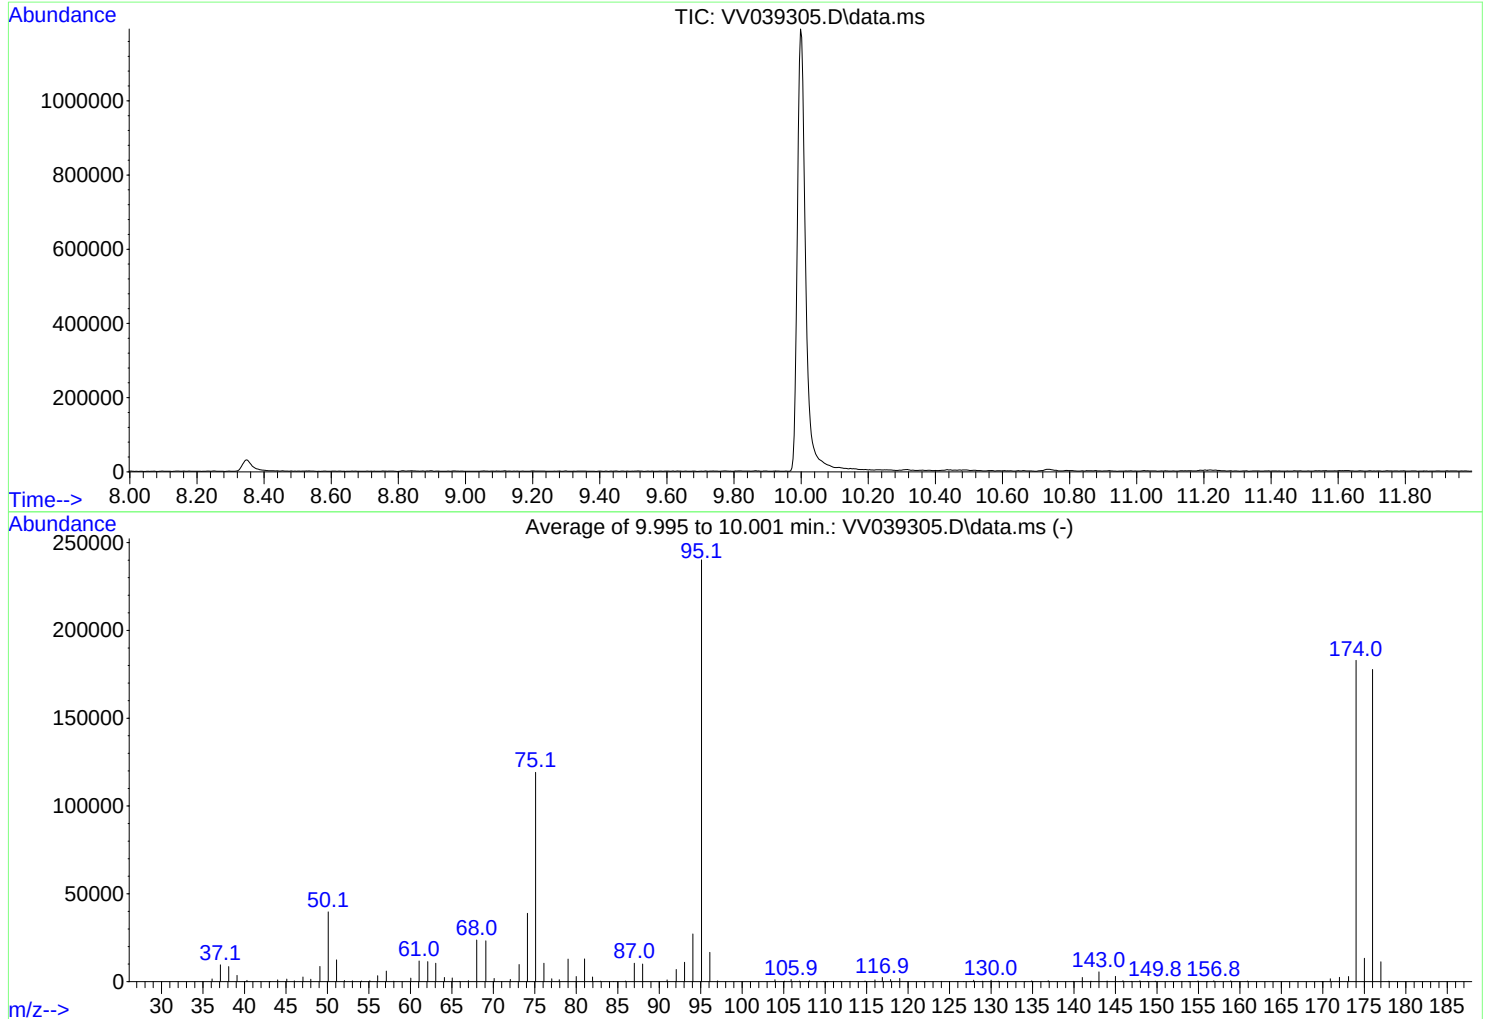

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2773

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	39680	PASS
75	95	30	60	49.6	119211	PASS
95	95	100	100	100.0	240171	PASS
96	95	5	9	6.9	16644	PASS
173	174	0.00	2	1.6	2957	PASS
174	95	50	100	76.2	182912	PASS
175	174	5	9	7.3	13300	PASS
176	174	95	101	97.2	177707	PASS
177	176	5	9	6.4	11330	PASS