

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110425\
 Data File : VV039321.D
 Acq On : 04 Nov 2025 17:47
 Operator : SY/MD
 Sample : Q3534-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
 Title : SW846 8260

Signal : TIC: VV039321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	20	27	38	rVB	778200	937658	16.67%	1.790%
2	1.204	38	51	72	rBV	2015145	5625132	100.00%	10.739%
3	1.918	265	273	294	rBV	635216	1064784	18.93%	2.033%
4	2.127	330	338	361	rVB3	75482	158925	2.83%	0.303%
5	2.568	466	475	495	rVB2	73974	166010	2.95%	0.317%
6	3.214	660	676	710	rBV	1585211	4197238	74.62%	8.013%
7	3.802	842	859	897	rBV2	135578	478043	8.50%	0.913%
8	4.240	983	995	1039	rBV3	222275	692165	12.30%	1.321%
9	4.500	1060	1076	1095	rBV2	769905	2024808	36.00%	3.866%
10	4.600	1095	1107	1157	rVB	1073423	2960681	52.63%	5.652%
11	4.940	1200	1213	1227	rBV	811108	1912171	33.99%	3.651%
12	5.011	1227	1235	1259	rVV2	337762	884805	15.73%	1.689%
13	5.114	1260	1267	1290	rVV3	46295	134395	2.39%	0.257%
14	5.214	1290	1298	1334	rVB3	99535	274985	4.89%	0.525%
15	5.529	1384	1396	1434	rBV	1763610	4009194	71.27%	7.654%
16	7.236	1915	1927	1954	rBV	3005475	5470536	97.25%	10.444%
17	7.403	1971	1979	2001	rVB2	54277	121866	2.17%	0.233%
18	8.146	2201	2210	2220	rBV5	26750	56779	1.01%	0.108%
19	8.773	2394	2405	2409	rBV	3079975	4633900	82.38%	8.847%
20	8.802	2410	2414	2425	rVB	3650836	5099397	90.65%	9.736%
21	8.860	2426	2432	2437	rBV	245490	329547	5.86%	0.629%
22	9.474	2617	2623	2639	rVB	45015	78743	1.40%	0.150%
23	9.641	2664	2675	2691	rBV2	94095	162669	2.89%	0.311%
24	9.857	2732	2742	2760	rBV	145371	243364	4.33%	0.465%
25	9.998	2776	2786	2811	rBV	2427661	3796707	67.50%	7.248%
26	10.288	2867	2876	2892	rBV5	46991	98289	1.75%	0.188%
27	10.667	2985	2994	3014	rBV	63480	113254	2.01%	0.216%
28	11.172	3140	3151	3173	rBV	2997830	5044746	89.68%	9.631%
29	11.416	3219	3227	3231	rBV2	66259	92891	1.65%	0.177%
30	11.451	3231	3238	3254	rVB	203549	357538	6.36%	0.683%
31	11.570	3266	3275	3298	rVB	164446	303697	5.40%	0.580%
32	11.943	3383	3391	3407	rBV2	55930	105781	1.88%	0.202%
33	12.040	3414	3421	3446	rVB4	39583	94713	1.68%	0.181%
34	12.339	3507	3514	3523	rBV3	43566	66287	1.18%	0.127%
35	12.586	3580	3591	3602	rBV4	64571	118032	2.10%	0.225%
36	12.808	3646	3660	3672	rBV3	90608	171413	3.05%	0.327%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110425\
Data File : VV039321.D
Acq On : 04 Nov 2025 17:47
Operator : SY/MD
Sample : Q3534-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-6

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Title : SW846 8260

37	14.557	4196	4204	4227	rVB	87504	173069	3.08%	0.330%
38	14.741	4251	4261	4277	rBV2	72092	125153	2.22%	0.239%




Sum of corrected areas: 52379365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110425\
Data File : VV039321.D
Acq On : 04 Nov 2025 17:47
Operator : SY/MD
Sample : Q3534-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

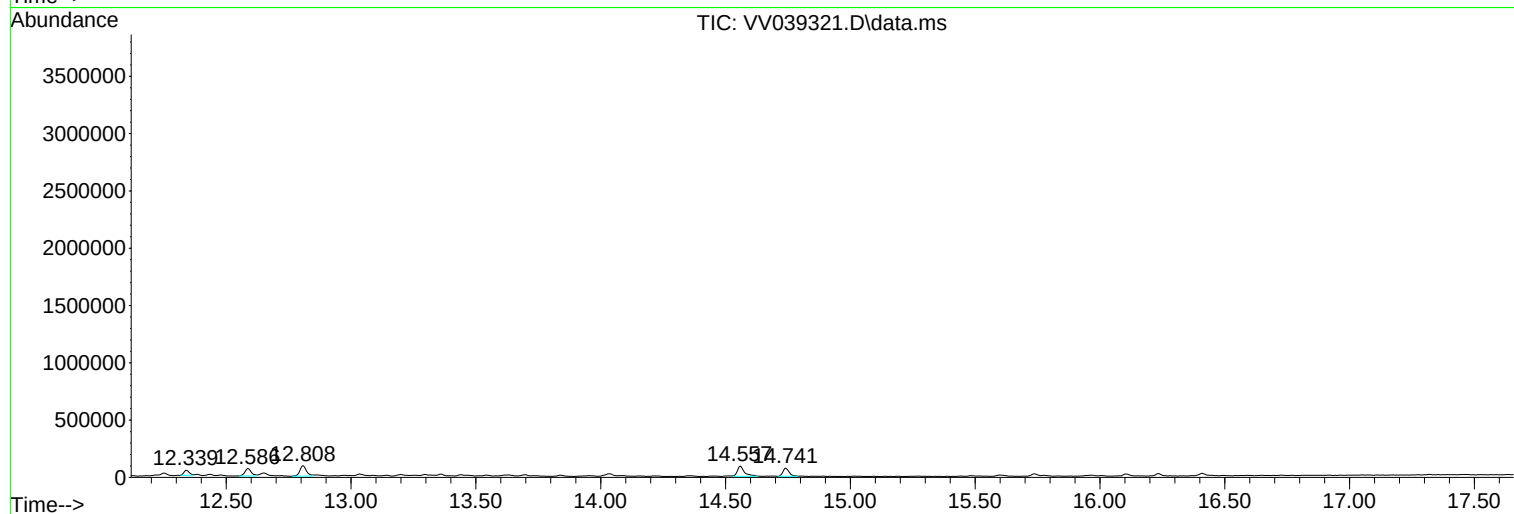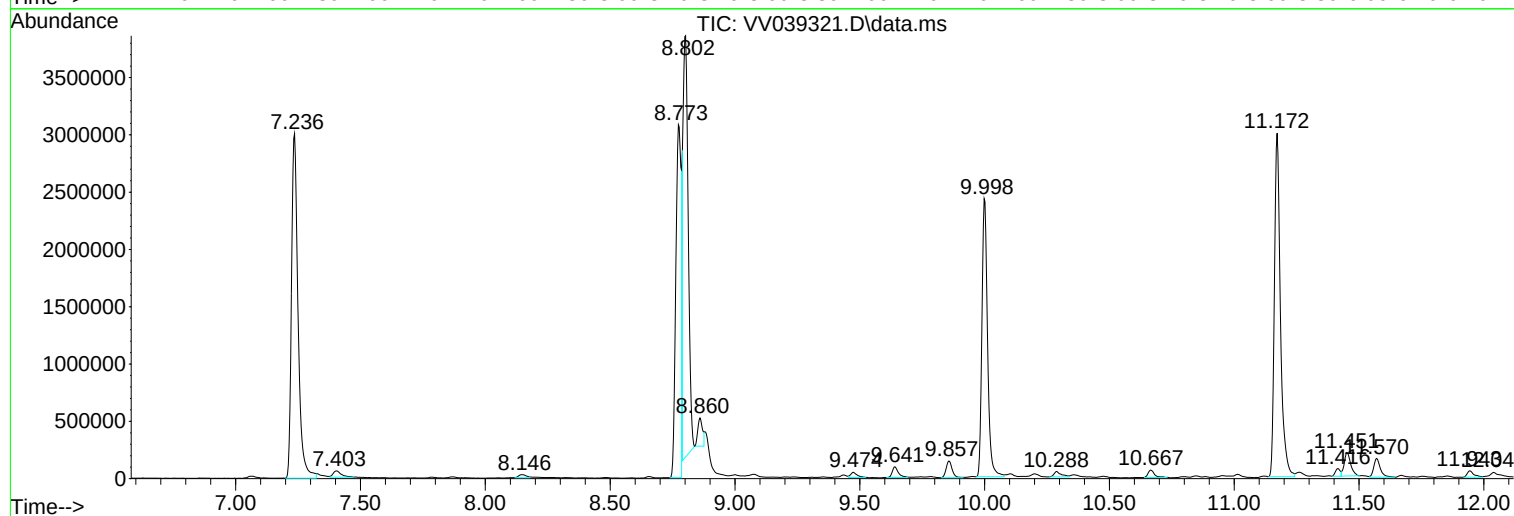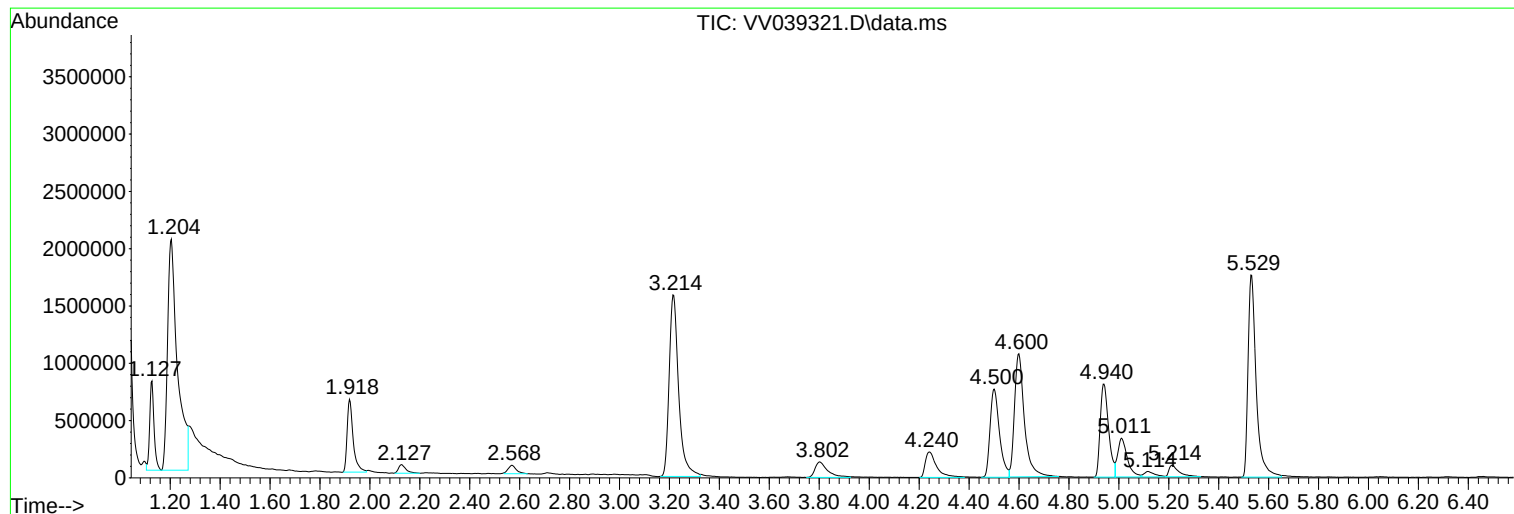

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110425\
Data File : VV039321.D
Acq On : 04 Nov 2025 17:47
Operator : SY/MD
Sample : Q3534-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110425\
Data File : VV039321.D
Acq On : 04 Nov 2025 17:47
Operator : SY/MD
Sample : Q3534-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------