

Test results

Aquakem 7.2AQ1

Page:

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

11/17/2025 16:36

Reviewed by : RM Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.002	0.0	0.107	
ICB1	0.003	0.0	0.007	
CCV1	0.972	0.0	0.104	
CCB1	0.007	0.0	0.007	
PB170566BL	0.005	0.0	0.007	
PB170566BS	0.989	0.0	0.106	
Q3530-10	0.031	0.0	0.009	
Q3530-11	0.056	0.0	0.012	
Q3551-01	0.363	0.0	0.043	
Q3630-02	0.014	0.0	0.008	
Q3630-06	-0.010	0.0	0.005	
Q3630-06DUP	0.024	0.0	0.009	
Q3630-06MS	1.055	0.0	0.112	
Q3630-06MSD	1.058	0.0	0.113	
CCV2	0.977	0.0	0.104	
CCB2	0.008	0.0	0.007	
N	16			
Mean	0.410			
SD	0.4876			
CV%	119.02			

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 17 15:46:38 2025

Mon Nov 17 16:36:26 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0005	mg/l	11/17/2025 15:46:38	
0.05PPM	A	Phenolics-	P	0.0582	mg/l	11/17/2025 15:46:39	
0.1PPM	A	Phenolics-	P	0.1053	mg/l	11/17/2025 15:46:40	
0.25PPM	A	Phenolics-	P	0.251	mg/l	11/17/2025 15:46:41	
0.50PPM	A	Phenolics-	P	0.4996	mg/l	11/17/2025 15:46:42	
1.0PPM	A	Phenolics-	P	0.9739	mg/l	11/17/2025 15:46:43	
2.0PPM	A	Phenolics-	P	2.0125	mg/l	11/17/2025 15:46:44	
ICV1	S	Phenolics-	P	1.0023	mg/l	11/17/2025 16:20:29	
ICB1	S	Phenolics-	P	0.0028	mg/l	11/17/2025 16:20:32	
CCV1	S	Phenolics-	P	0.9715	mg/l	11/17/2025 16:20:33	
CCB1	S	Phenolics-	P	0.0066	mg/l	11/17/2025 16:20:35	
PB170566BL	S	Phenolics-	P	0.0051	mg/l	11/17/2025 16:20:38	
PB170566BS	S	Phenolics-	P	0.9891	mg/l	11/17/2025 16:20:39	
Q3530-10	S	Phenolics-	P	0.031	mg/l	11/17/2025 16:30:31	
Q3530-11	S	Phenolics-	P	0.0563	mg/l	11/17/2025 16:30:34	
Q3551-01	S	Phenolics-	P	0.3628	mg/l	11/17/2025 16:30:35	
Q3630-02	S	Phenolics-	P	0.0143	mg/l	11/17/2025 16:30:37	
Q3630-06	S	Phenolics-	P	-0.0102	mg/l	11/17/2025 16:30:39	
Q3630-06DUP	S	Phenolics-	P	0.0244	mg/l	11/17/2025 16:30:40	
Q3630-06MS	S	Phenolics-	P	1.0554	mg/l	11/17/2025 16:30:41	
Q3630-06MSD	S	Phenolics-	P	1.0578	mg/l	11/17/2025 16:30:42	
CCV2	S	Phenolics-	P	0.9773	mg/l	11/17/2025 16:36:23	
CCB2	S	Phenolics-	P	0.0082	mg/l	11/17/2025 16:36:26	

Calibration results

Aquakem 7.2AQ1

Page:

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

11/17/2025 15:48


Test Phenolics-

Accepted 11/17/2025 15:48

Factor 9.96
Bias 0.006

Coeff. of det. 0.999704

Errors

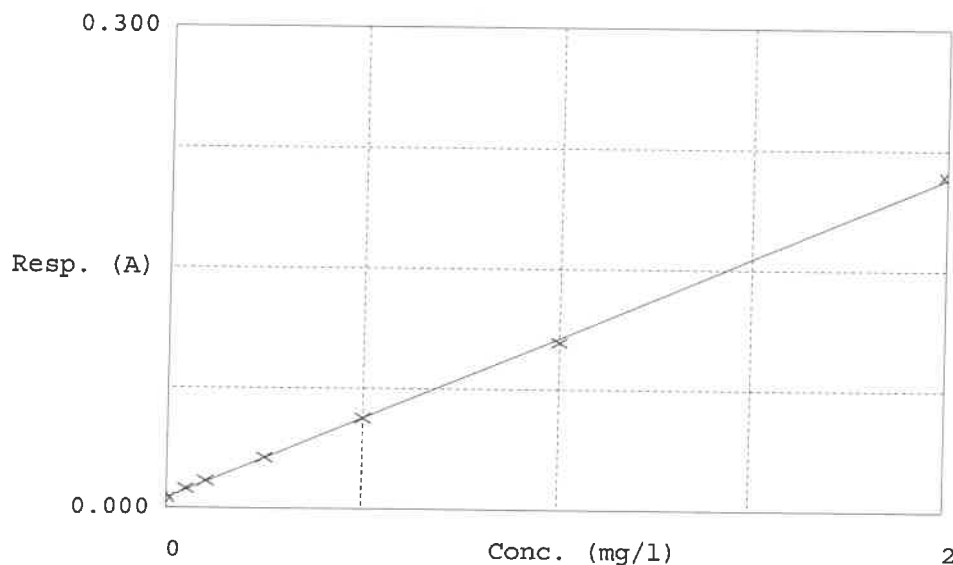

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.006	-0.0005	0.0000	-
2	Phenol-2	0.012	0.0582	0.0500	16.4
3	Phenol-2	0.017	0.1053	0.1000	5.3
4	Phenol-2	0.032	0.2510	0.2500	0.4
5	Phenol-2	0.057	0.4996	0.5000	-0.1
6	Phenol-2	0.104	0.9739	1.0000	-2.6
7	Phenol-2	0.208	2.0125	2.0000	0.6

11/17/2025
RM