


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110725\
Data File : BG064712.D
Acq On : 7 Nov 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 03 18:16:26 2025

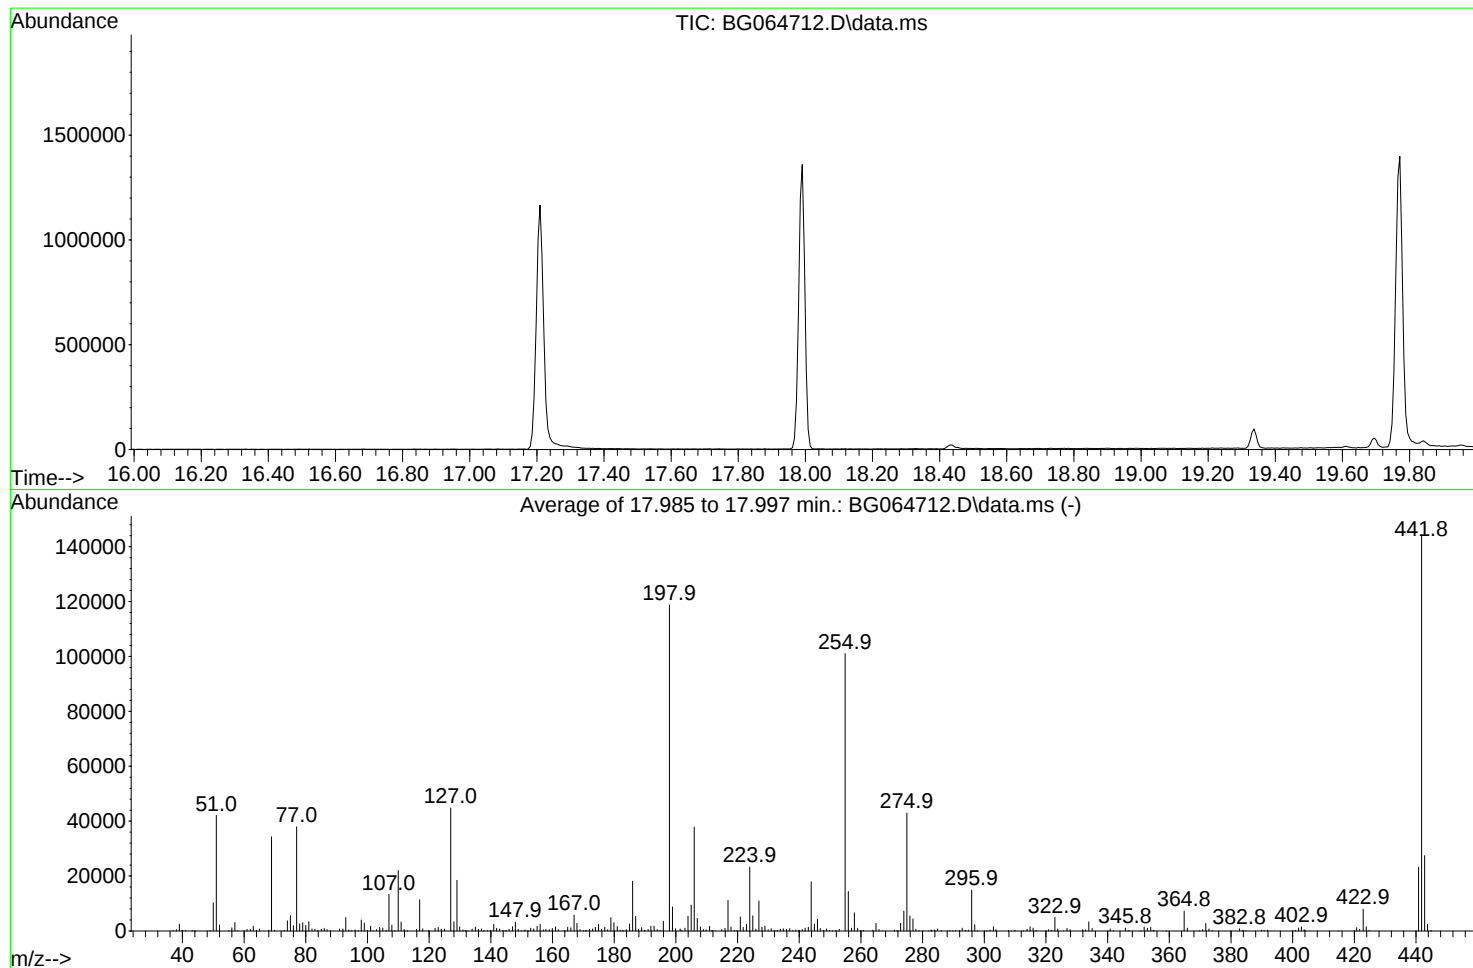




AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.8	264	PASS
69	69	100	100	100.0	34307	PASS
70	69	0.00	2	0.6	198	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118811	PASS
199	198	5	9	7.3	8731	PASS
365	198	1	100	6.1	7189	PASS
441	443	0.01	150	84.6	23229	PASS
442	442	100	100	100.0	143856	PASS
443	442	15	24	19.1	27459	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110725\
Data File : BG064712.D
Acq On : 7 Nov 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 07 11:06:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

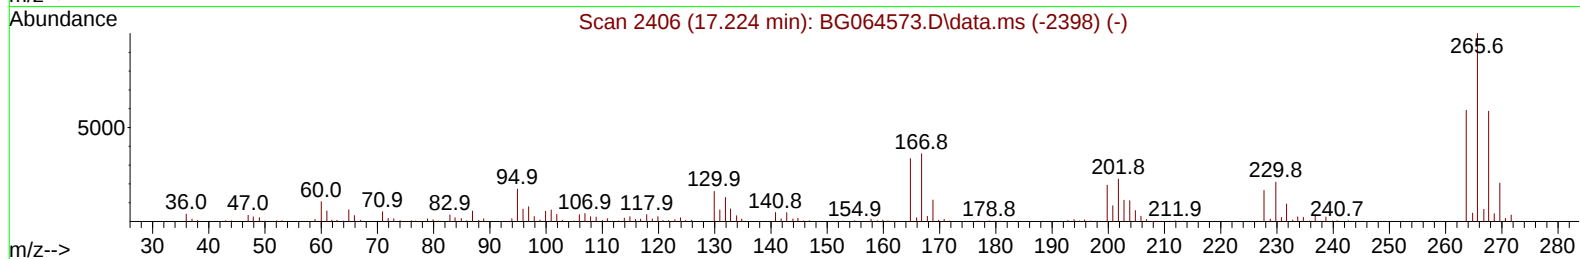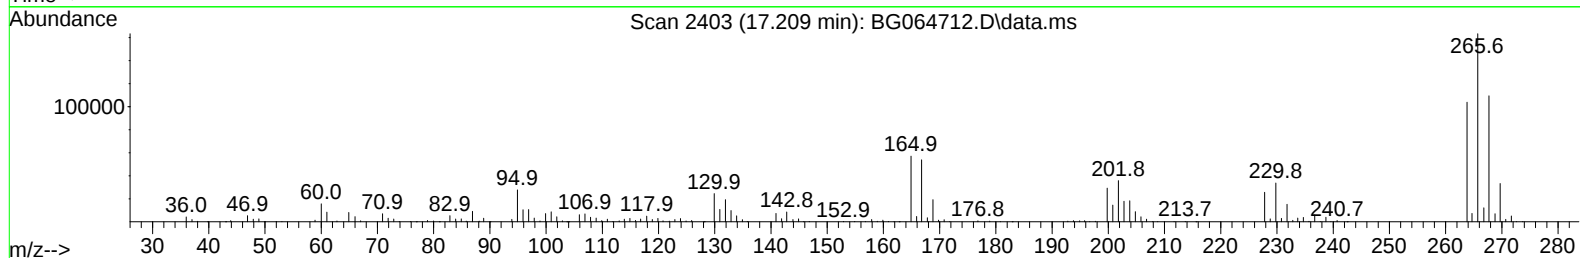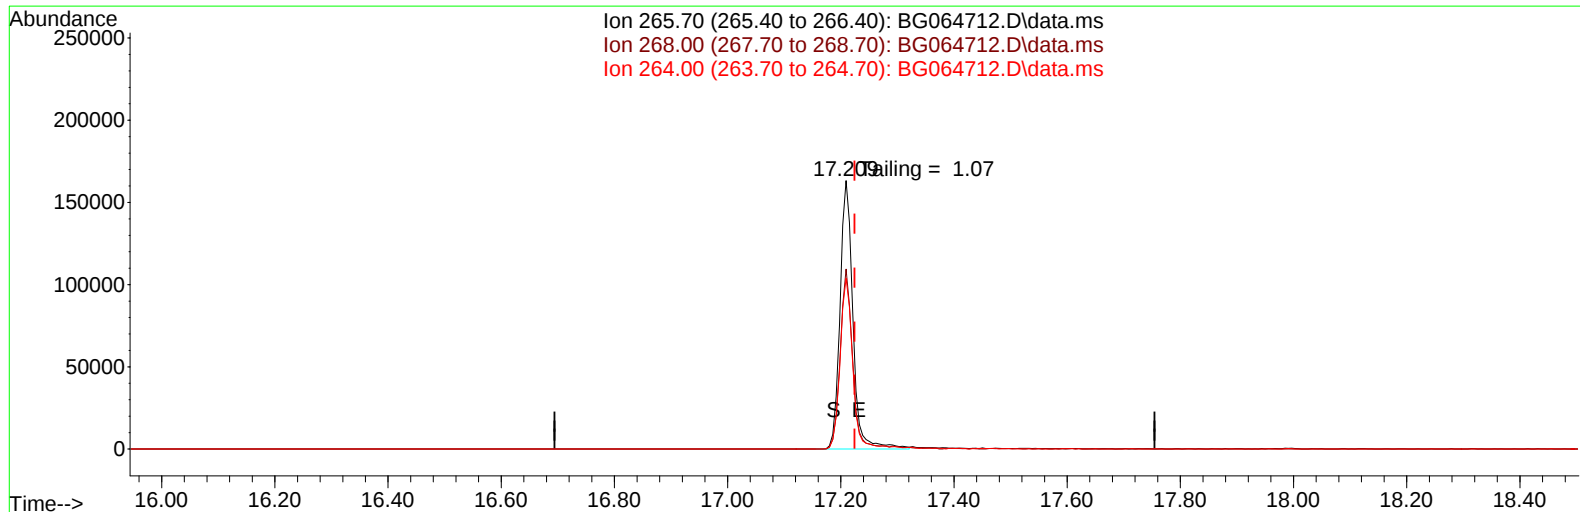

TIC: BG064712.D\data.ms

(70) Pentachlorophenol (C)

17.209min (-0.015) 37237.71 ng

response 262760

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	67.03
264.00	59.10	68.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2025	BNA_G	<u>BG064712.D</u>
Compound Name	Response	Retention Time
DDT	555848	21.005
DDD	20925	20.558
DDE	69	19.695
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20994	576842	3.64

Instrument :
BNA_G
ClientSampleId :
DFTPP