


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111425\
Data File : VN088281.D
Acq On : 14 Nov 2025 08:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N111325W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Nov 14 00:49:21 2025

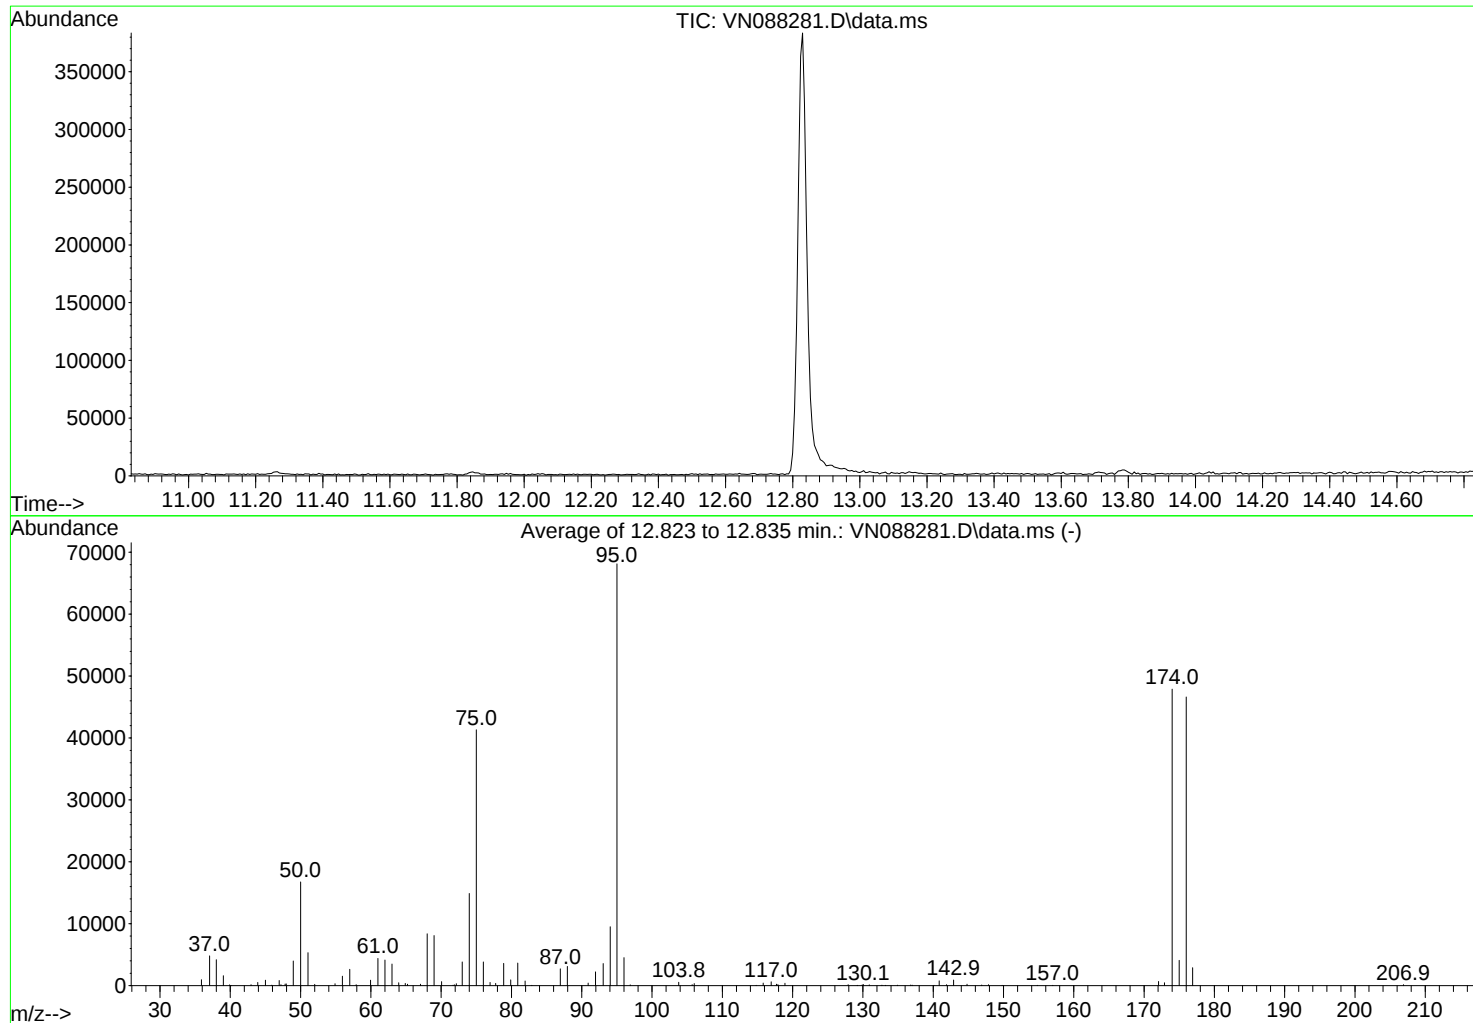

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1841

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	16738	PASS
75	95	30	60	60.7	41339	FAIL*
95	95	100	100	100.0	68131	PASS
96	95	5	9	6.7	4538	PASS
173	174	0.00	2	1.0	462	PASS
174	95	50	100	70.3	47893	PASS
175	174	5	9	8.5	4073	PASS
176	174	95	101	97.4	46637	PASS
177	176	5	9	6.2	2894	PASS