

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110625\
 Data File : PP076366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 17:49
 Operator : YP\AJ
 Sample : Q3552-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MW-3

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/07/2025
 Supervised By :Yogesh Patel 11/07/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:28:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.636	3.778	39666227	147.2E6	27.756m	22.239m
2) SA Decachlor...	10.405	8.774	23879995	168.1E6	22.182	20.439

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110625\
Data File : PP076366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 17:49
Operator : YP\AJ
Sample : Q3552-05
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MW-3


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/07/2025
Supervised By :Yogesh Patel 11/07/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:28:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

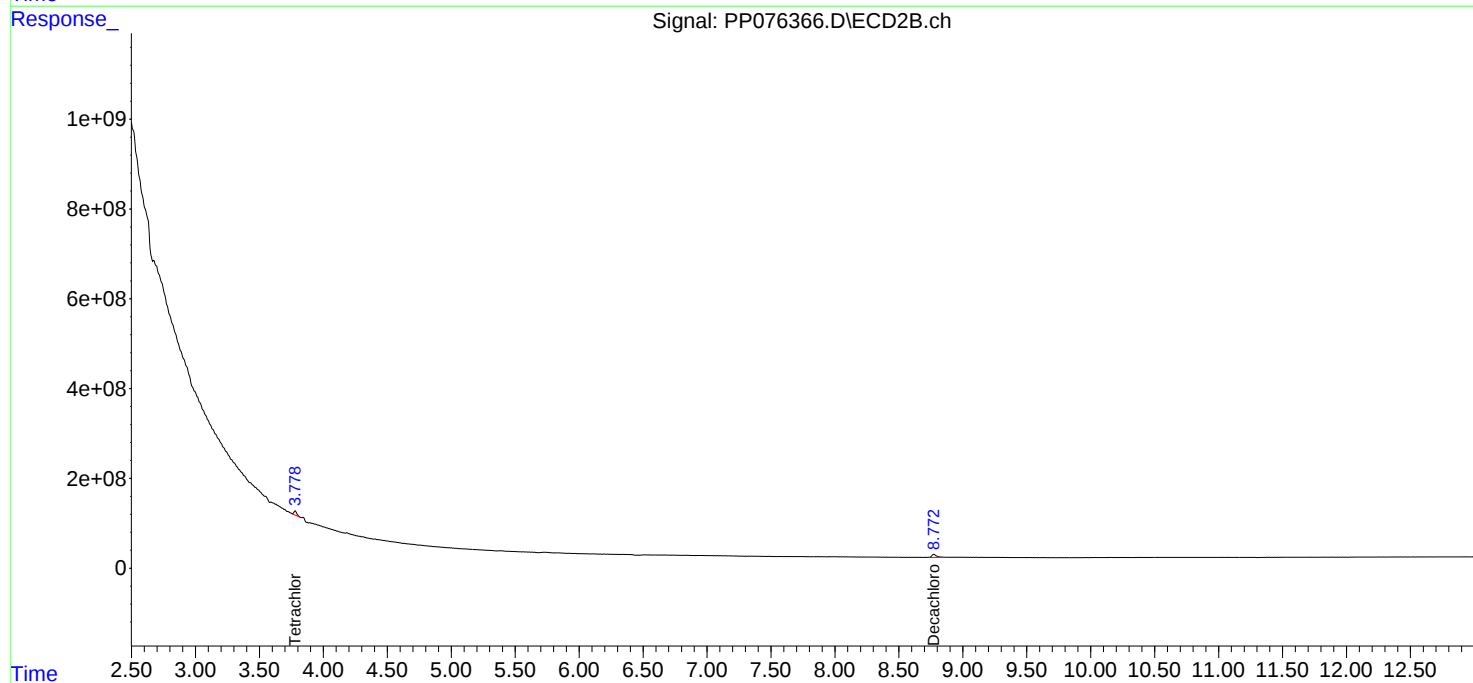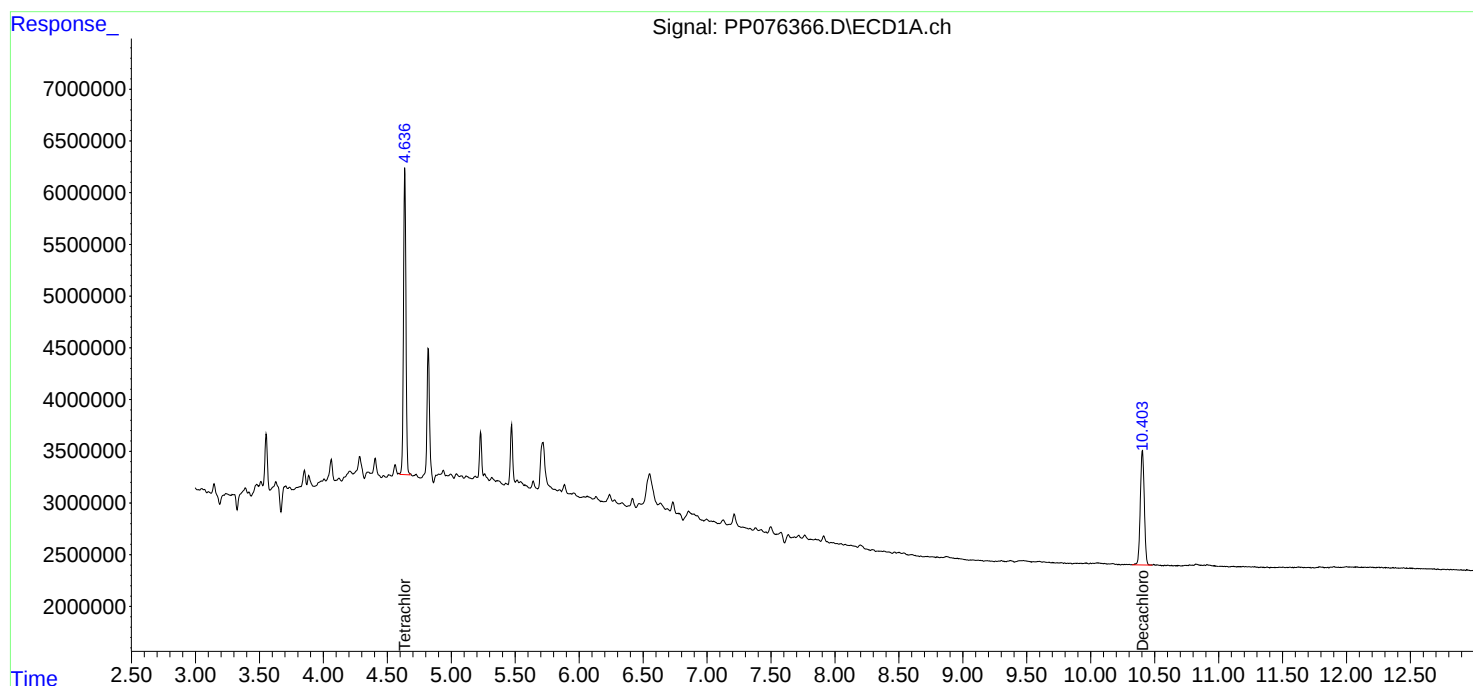

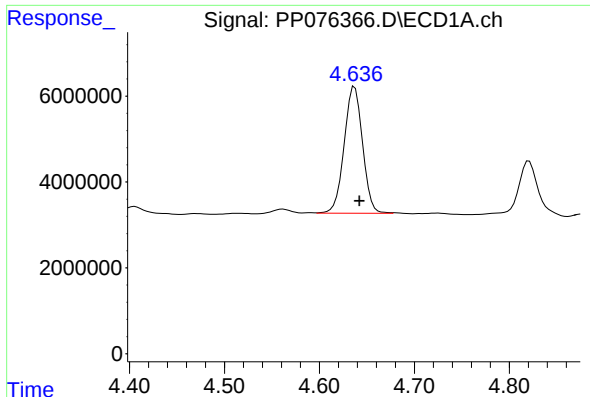


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.006 min
Response: 39666227
Conc: 27.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
MW-3


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/07/2025
Supervised By :Yogesh Patel 11/07/2025

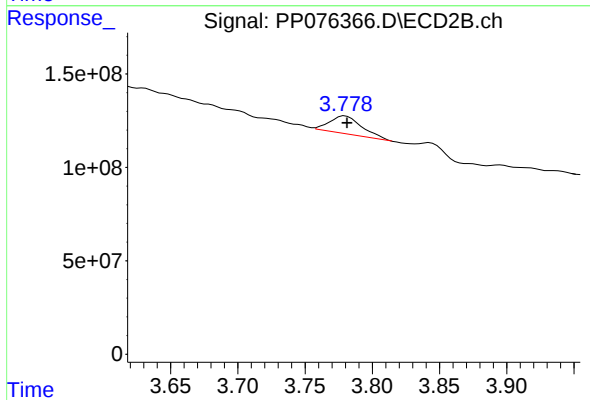


#1 Tetrachloro-m-xylene

R.T.: 3.778 min
Delta R.T.: -0.003 min
Response: 147182192
Conc: 22.24 ng/ml m

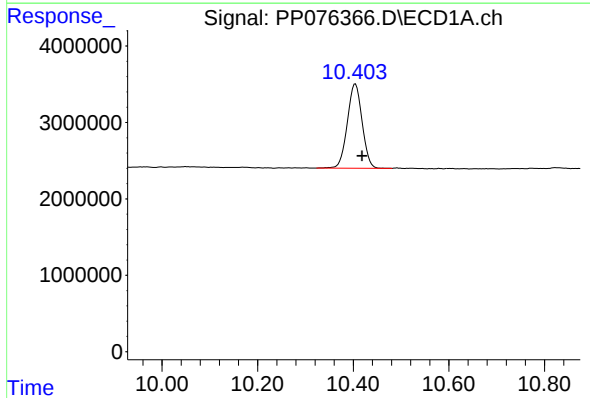

#2 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.014 min
Response: 23879995
Conc: 22.18 ng/ml

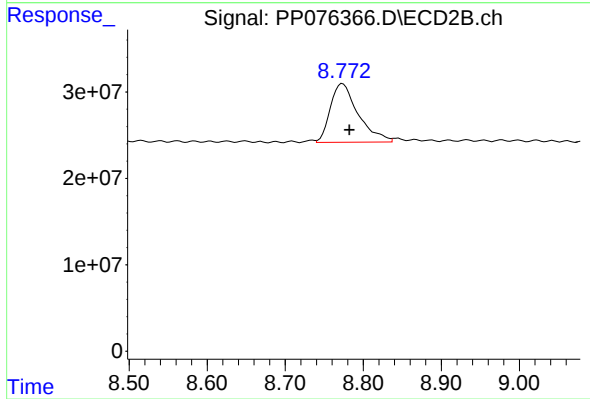

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.009 min
Response: 168067902
Conc: 20.44 ng/ml