


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110625\
Data File : BF144179.D
Acq On : 06 Nov 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

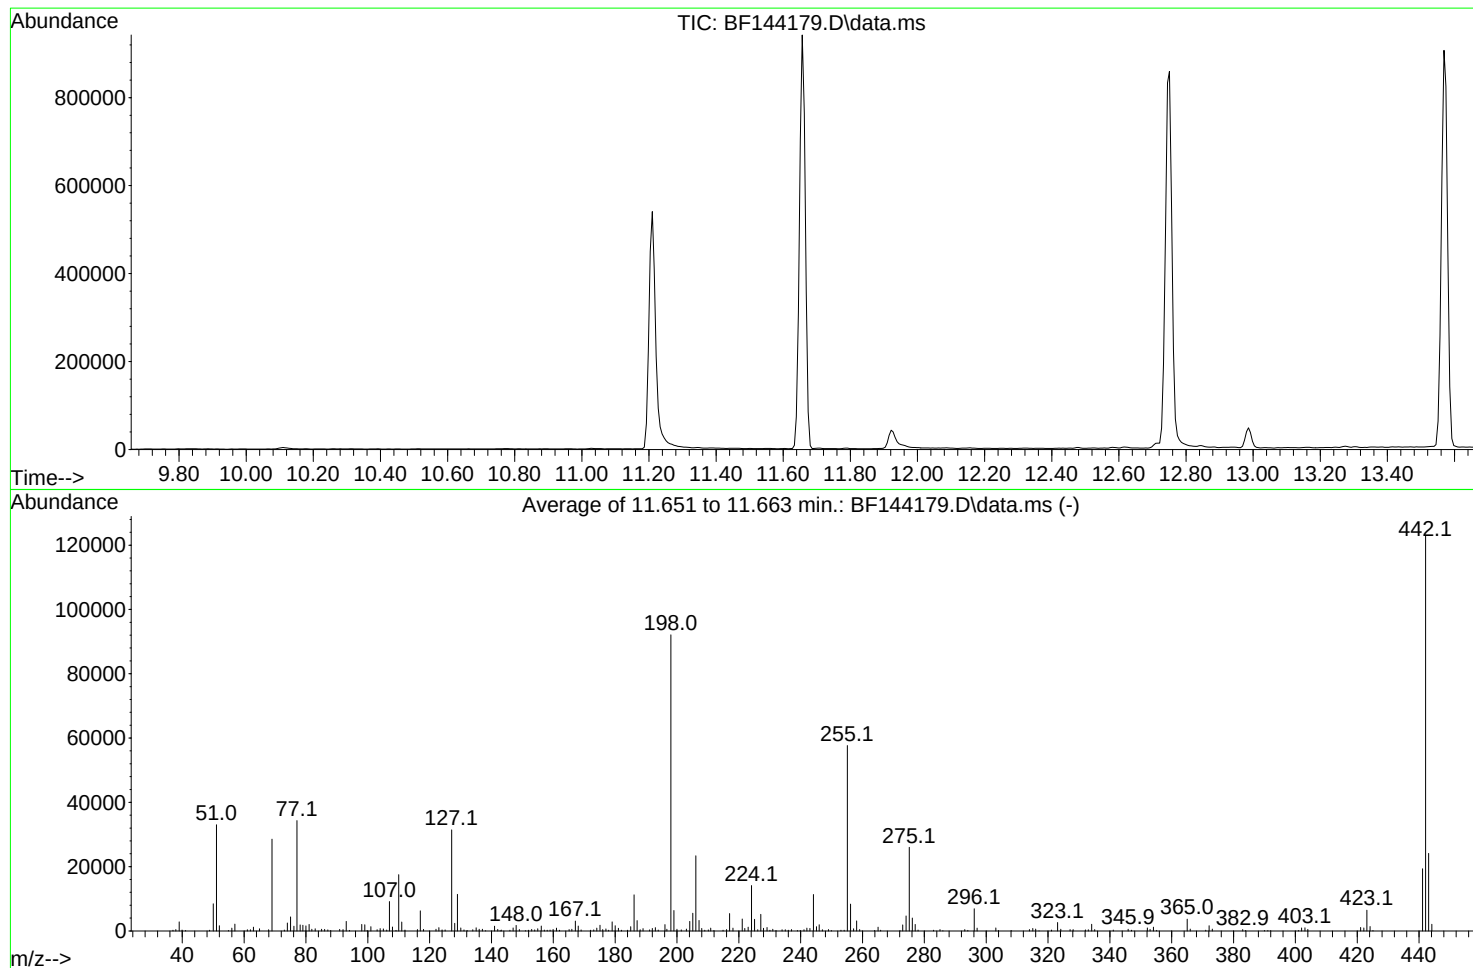




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.4	388	PASS
69	69	100	100	100.0	28549	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.6	527	PASS
198	198	100	100	100.0	92085	PASS
199	198	5	9	6.9	6362	PASS
365	198	1	100	4.0	3685	PASS
441	443	0.01	150	80.1	19318	PASS
442	442	100	100	100.0	122819	PASS
443	442	15	24	19.6	24107	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110625\
Data File : BF144179.D
Acq On : 06 Nov 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 06 11:08:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

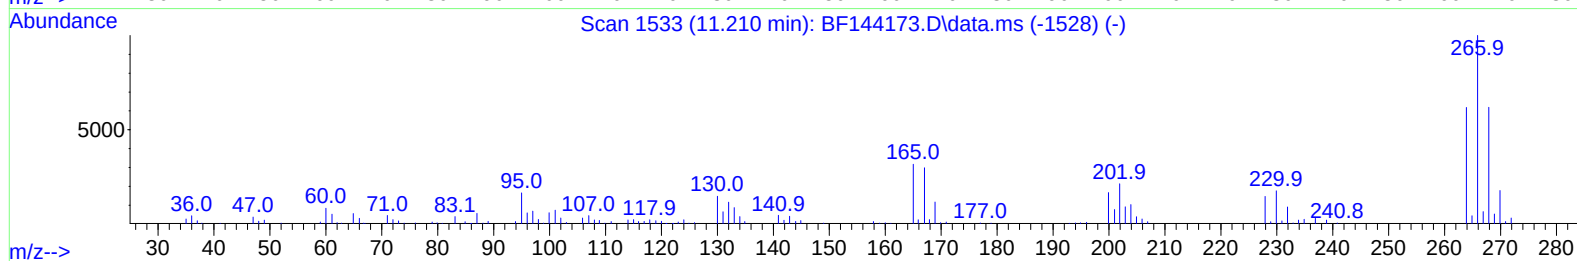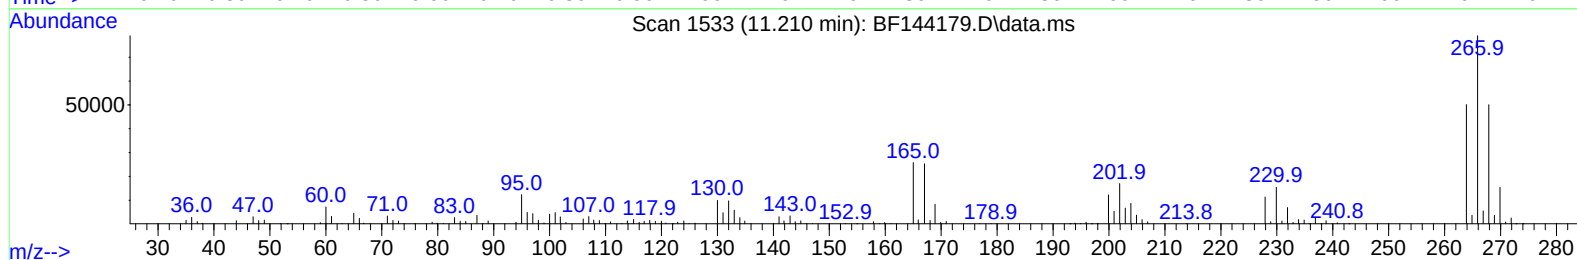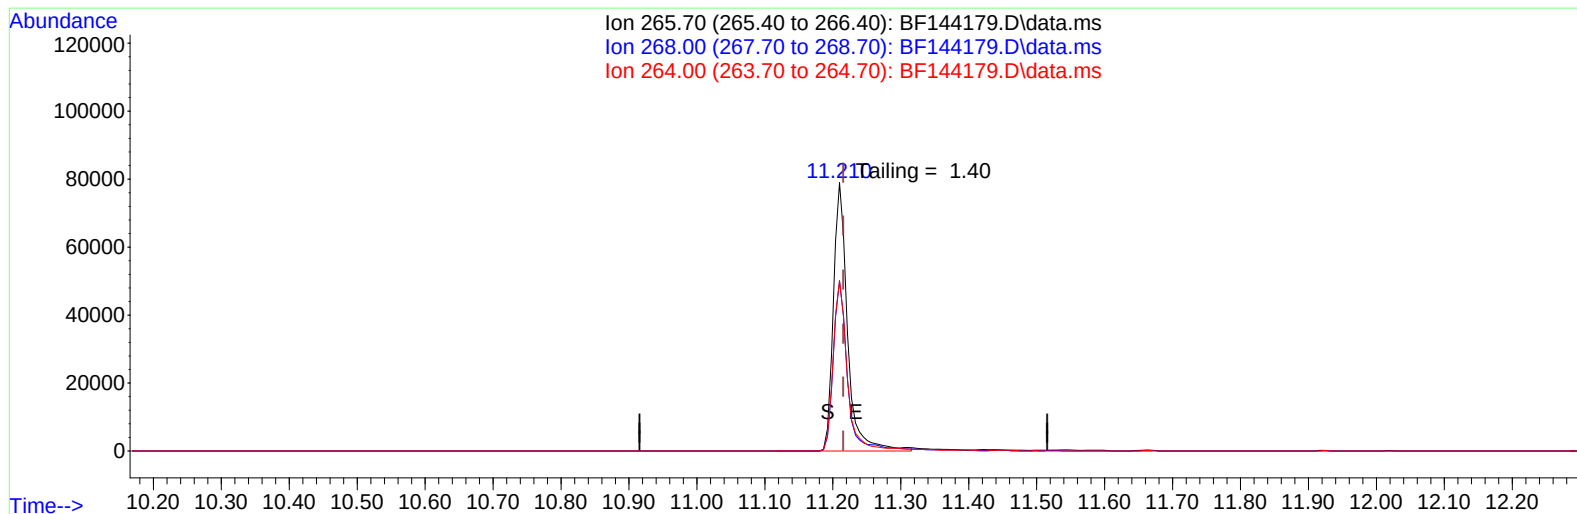

TIC: BF144179.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 79231.71 ng




response 113889

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.36
264.00	61.80	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110625\
Data File : BF144179.D
Acq On : 06 Nov 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 06 11:08:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

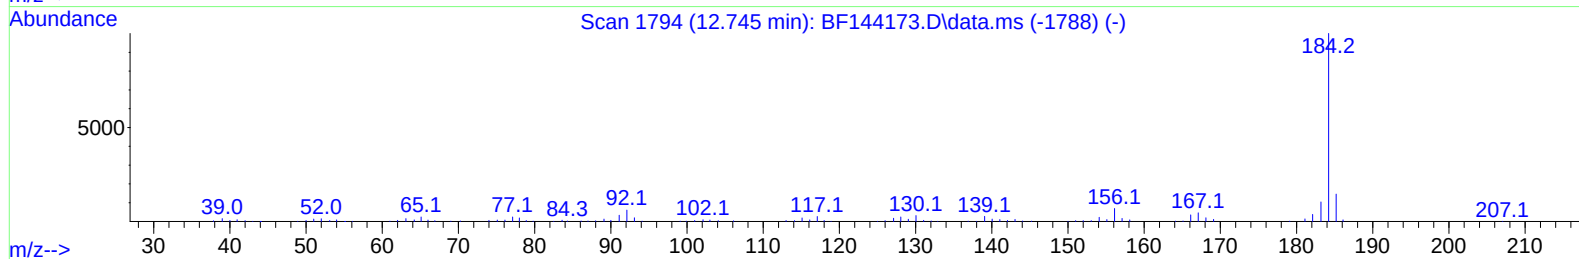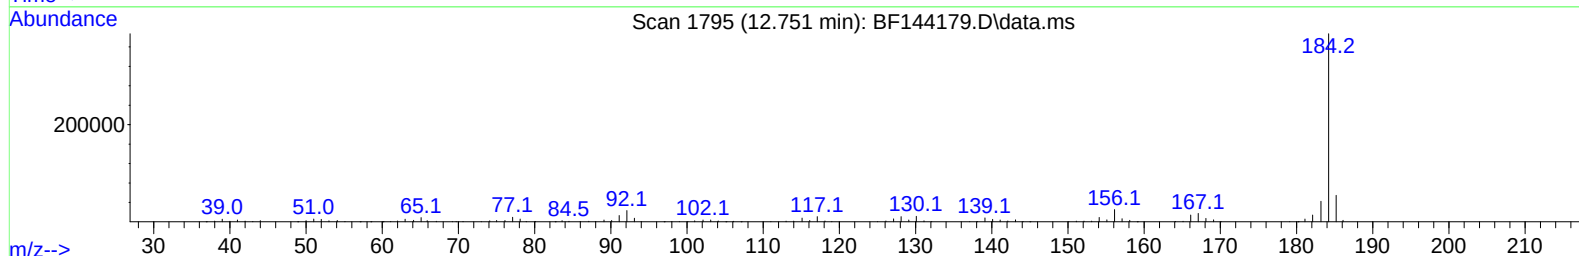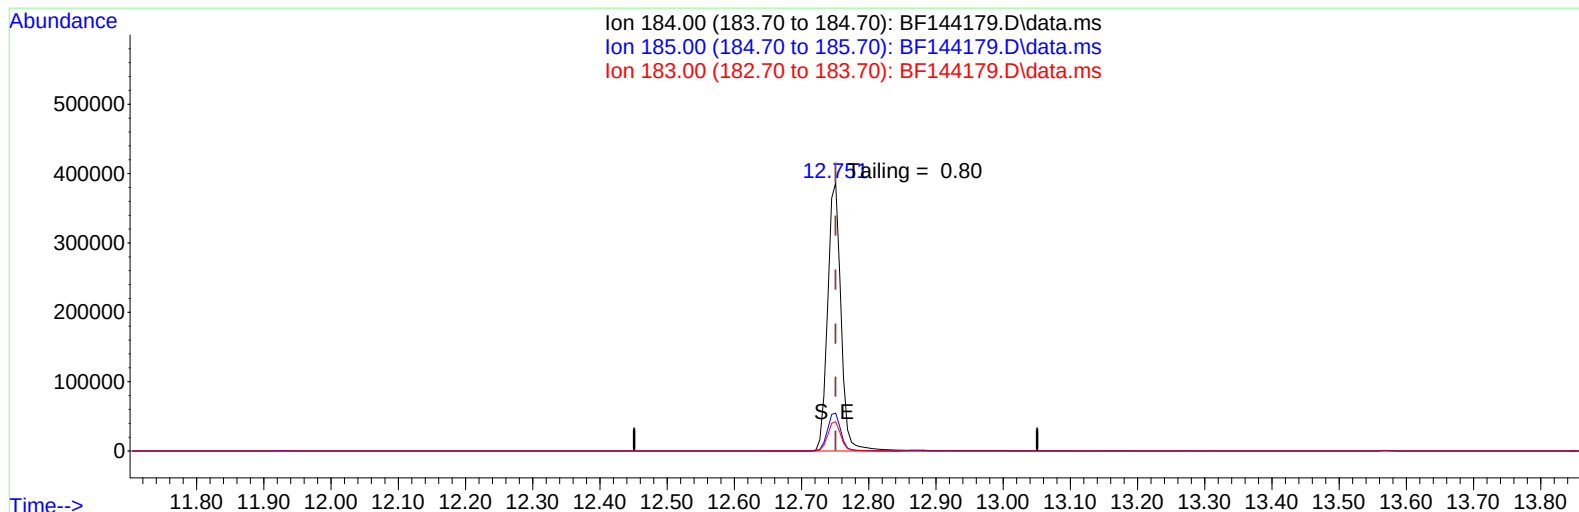

TIC: BF144179.D\data.ms

(77) Benzidine

12.751min (-0.000) 11408.92 ng

response 534549

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.13
183.00	10.40	10.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/6/2025	BNA_F	<u>BF144179.D</u>
Compound Name	Response	Retention Time
DDT	252393	13.568
DDD	2828	13.274
DDE	499	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3327	255720	1.30

Instrument :
BNA_F
ClientSampleId :
DFTPP