

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110525\
 Data File : VV039339.D
 Acq On : 05 Nov 2025 16:35
 Operator : SY/MD
 Sample : Q3552-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-9

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
 Title : SW846 8260

Signal : TIC: VV039339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	23	27	38	rVB	78622	93613	2.48%	0.335%
2	1.195	39	48	68	rBV2	189168	413767	10.95%	1.482%
3	1.281	70	75	89	rVB2	55589	88700	2.35%	0.318%
4	1.921	266	274	291	rBV	69459	115181	3.05%	0.413%
5	2.564	459	474	502	rBV3	291338	715225	18.92%	2.562%
6	3.796	836	857	895	rBV	548755	1832012	48.47%	6.561%
7	4.243	985	996	1028	rBV3	111135	345399	9.14%	1.237%
8	4.500	1061	1076	1095	rBV	555189	1464092	38.74%	5.244%
9	4.600	1095	1107	1156	rVB	768573	2133889	56.46%	7.643%
10	4.940	1201	1213	1225	rBV	597905	1358729	35.95%	4.866%
11	5.011	1226	1235	1266	rVB	495844	1253246	33.16%	4.489%
12	5.532	1384	1397	1438	rBV	1232453	2821988	74.67%	10.107%
13	7.236	1915	1927	1949	rBV	2058593	3779369	100.00%	13.536%
14	7.860	2110	2121	2134	rBV	24289	49588	1.31%	0.178%
15	8.773	2393	2405	2411	rBV	2145699	3622965	95.86%	12.976%
16	9.471	2614	2622	2642	rVB2	50123	88591	2.34%	0.317%
17	9.857	2732	2742	2755	rBV	76661	127124	3.36%	0.455%
18	9.998	2776	2786	2811	rBV	1555063	2561603	67.78%	9.175%
19	10.284	2865	2875	2892	rBV	33948	76798	2.03%	0.275%
20	10.667	2984	2994	3007	rBV	52604	88795	2.35%	0.318%
21	11.011	3086	3101	3113	rBV5	80337	137943	3.65%	0.494%
22	11.172	3140	3151	3175	rBV	2158258	3765948	99.64%	13.488%
23	11.455	3229	3239	3255	rBV2	114642	239107	6.33%	0.856%
24	11.574	3269	3276	3295	rVB8	38491	91004	2.41%	0.326%
25	11.943	3384	3391	3405	rBV4	17109	37935	1.00%	0.136%
26	12.040	3413	3421	3446	rVB3	37827	100651	2.66%	0.360%
27	12.252	3472	3487	3498	rBV3	43832	92756	2.45%	0.332%
28	12.590	3581	3592	3602	rBV3	26587	54600	1.44%	0.196%
29	12.651	3603	3611	3624	rVB2	35162	61958	1.64%	0.222%
30	12.808	3646	3660	3670	rBV4	61009	112635	2.98%	0.403%
31	13.037	3723	3731	3739	rBV6	26929	43287	1.15%	0.155%
32	14.033	4025	4041	4050	rBV6	17558	38837	1.03%	0.139%
33	14.564	4196	4206	4224	rVB	25335	47579	1.26%	0.170%
34	14.744	4251	4262	4275	rBV2	36374	65910	1.74%	0.236%

Sum of corrected areas: 27920824




Instrument :
MSVOA_V
ClientSampleId :
MW-9

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110525\
Data File : VV039339.D
Acq On : 05 Nov 2025 16:35
Operator : SY/MD
Sample : Q3552-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

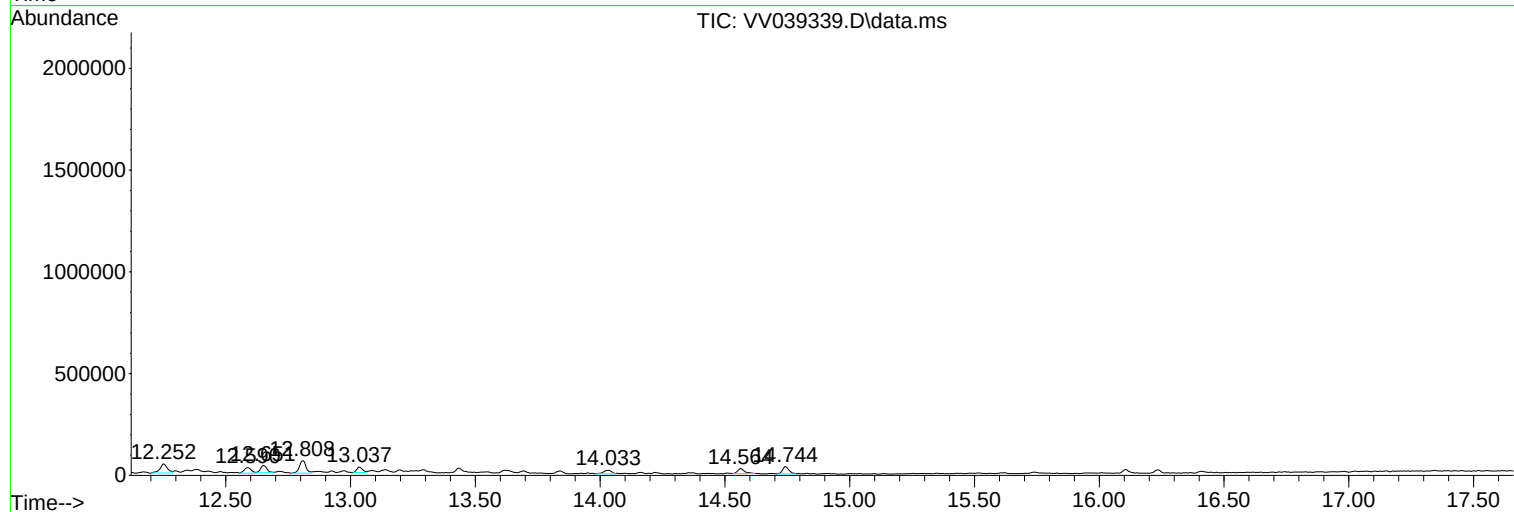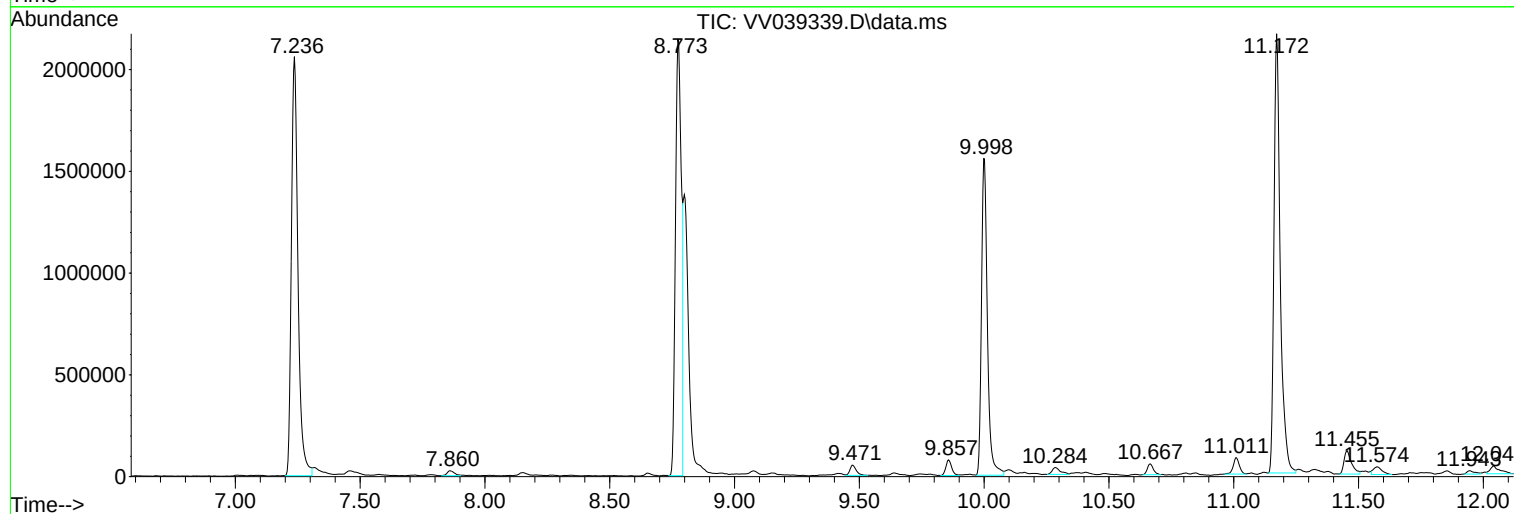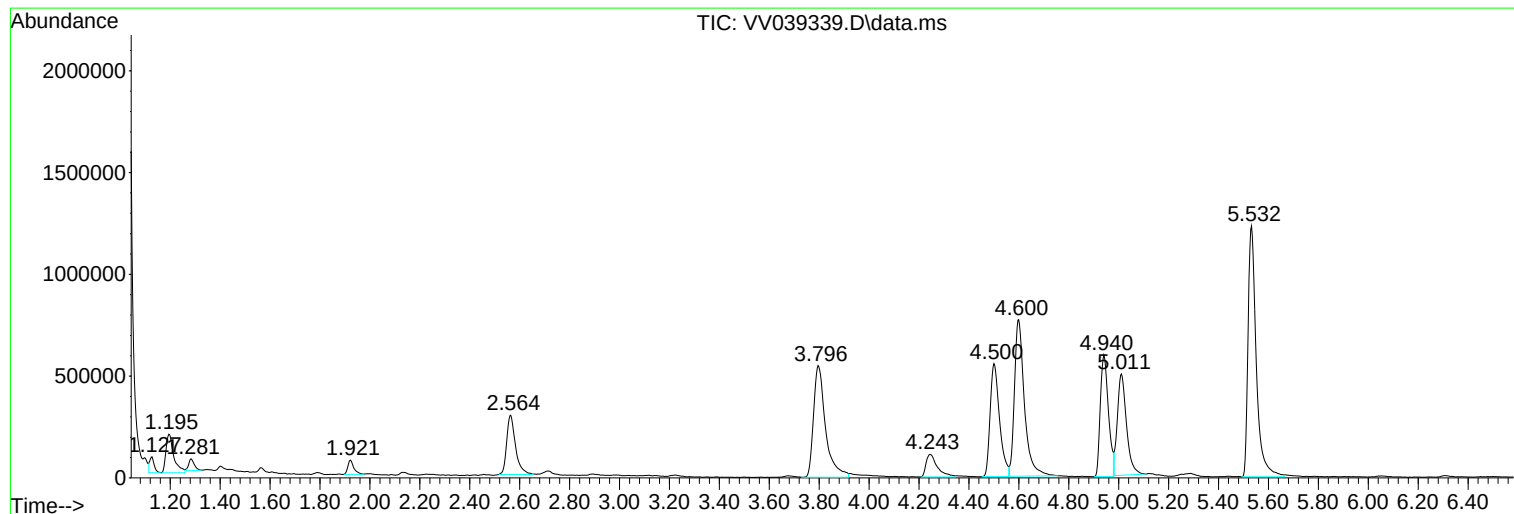

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110525\
Data File : VV039339.D
Acq On : 05 Nov 2025 16:35
Operator : SY/MD
Sample : Q3552-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110525\
Data File : VV039339.D
Acq On : 05 Nov 2025 16:35
Operator : SY/MD
Sample : Q3552-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------